

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091919\
 Data File : FF005625.D
 Signal(s) : FID2B.ch
 Acq On : 19 Sep 2019 12:57
 Operator : DD\AJ
 Sample : PB123221BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB123221BS

Integration File: autoint1.e
 Quant Time: Sep 20 01:16:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.621	2156222	20.150 ug/ml
Target Compounds			
2) N-DECANE	4.346	2599866	18.184 ug/ml
3) N-DODECANE	6.366	2543655	17.745 ug/ml
4) N-TETRADECANE	8.158	2450935	17.383 ug/ml
5) N-HEXADECANE	9.760	2532751	18.109 ug/ml
6) N-OCTADECANE	11.203	2515378	18.696 ug/ml
7) N-EICOSANE	12.516	2482567	18.930 ug/ml
8) N-DOCOSANE	13.718	2468092	19.603 ug/ml
10) N-TETRACOSANE	14.825	2515802	20.571 ug/ml
11) N-HEXACOSANE	15.851	2562058	21.403 ug/ml
12) N-OCTACOSANE	16.806	2638050	22.108 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091919\
Data File : FF005625.D
Signal(s) : FID2B.ch
Acq On : 19 Sep 2019 12:57
Operator : DD\AJ
Sample : PB123221BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB123221BS

Integration File: autoint1.e
Quant Time: Sep 20 01:16:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

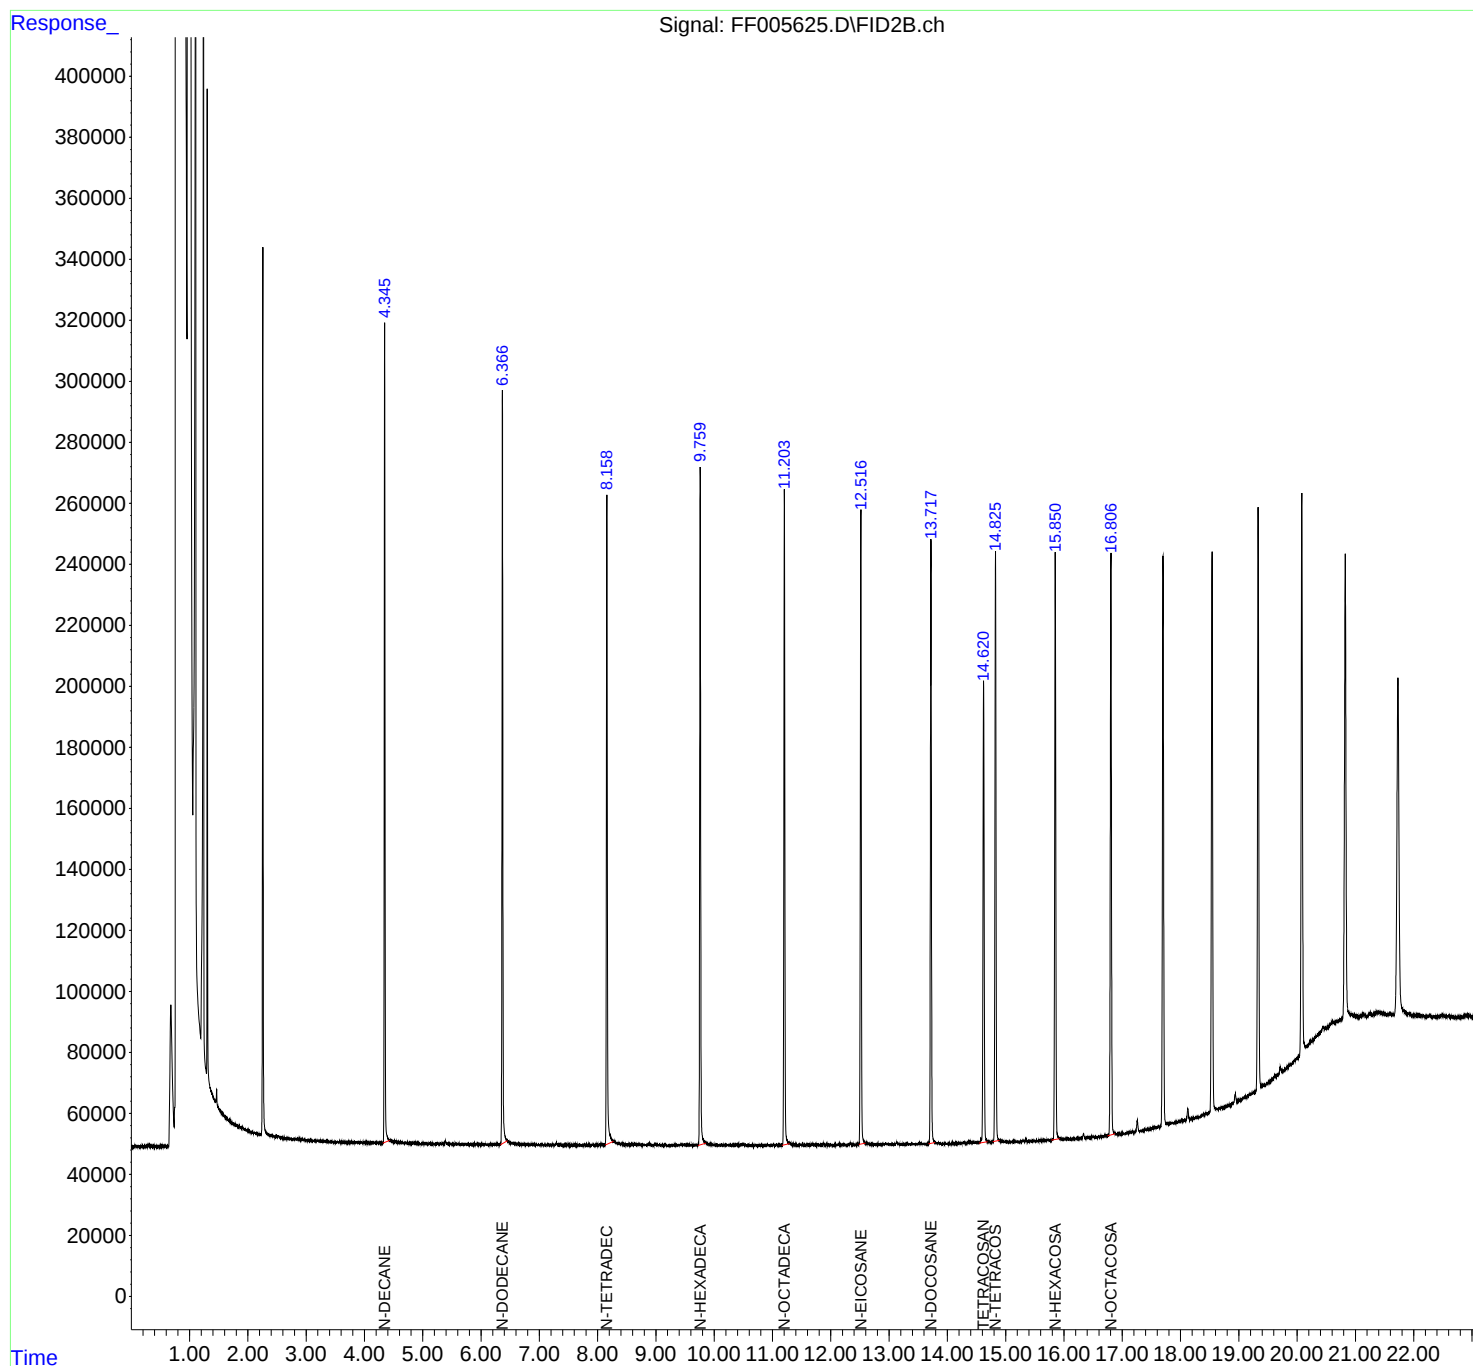


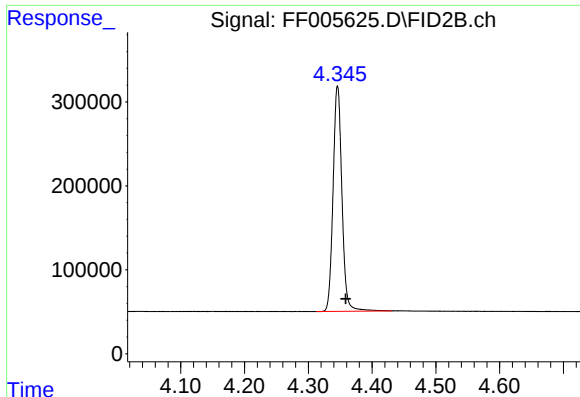

#2 N-DECANE


R.T.: 4.346 min
Delta R.T.: -0.013 min
Response: 2599866
Conc: 18.18 ug/ml

Instrument :
FID_F
ClientSampleId :
PB123221BS

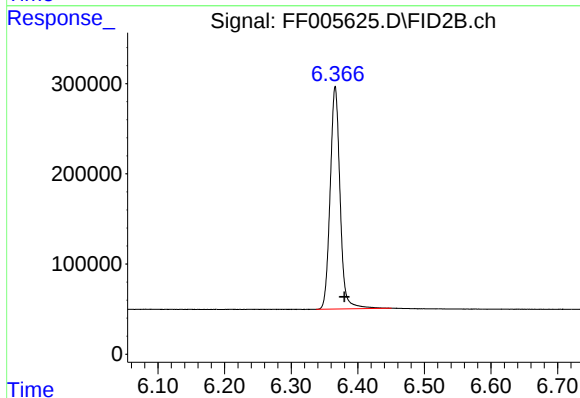


#3 N-DODECANE

R.T.: 6.366 min
Delta R.T.: -0.014 min
Response: 2543655
Conc: 17.74 ug/ml

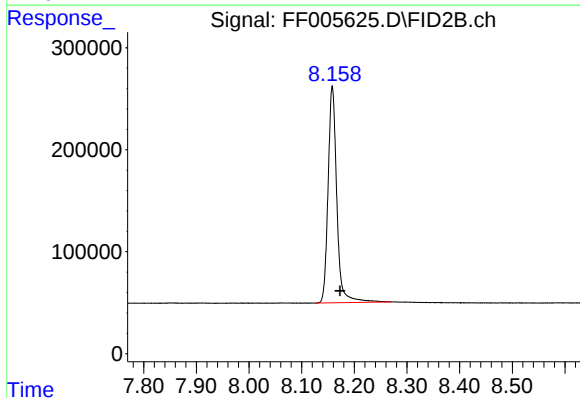


#4 N-TETRADECANE

R.T.: 8.158 min
Delta R.T.: -0.014 min
Response: 2450935
Conc: 17.38 ug/ml

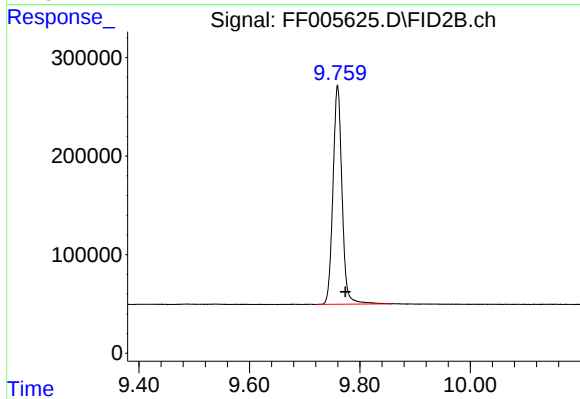

#5 N-HEXADECANE


R.T.: 9.760 min
Delta R.T.: -0.014 min
Response: 2532751
Conc: 18.11 ug/ml

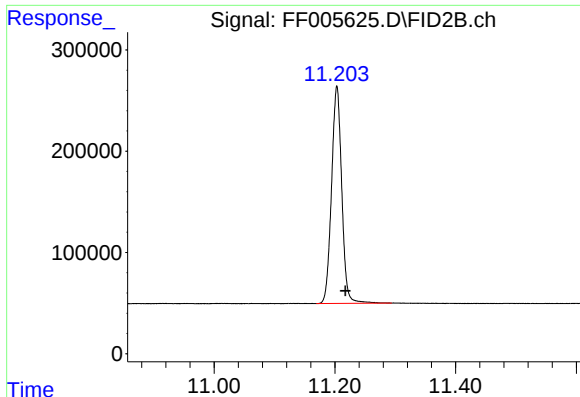

#6 N-OCTADECANE


R.T.: 11.203 min
Delta R.T.: -0.014 min
Response: 2515378
Conc: 18.70 ug/ml

Instrument :
FID_F
ClientSampleId :
PB123221BS

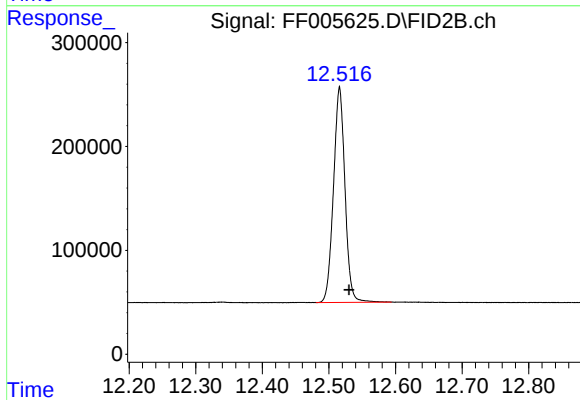


#7 N-EICOSANE

R.T.: 12.516 min
Delta R.T.: -0.014 min
Response: 2482567
Conc: 18.93 ug/ml

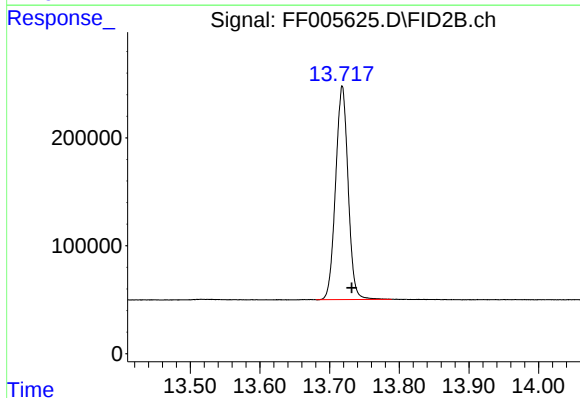


#8 N-DOCOSANE

R.T.: 13.718 min
Delta R.T.: -0.014 min
Response: 2468092
Conc: 19.60 ug/ml

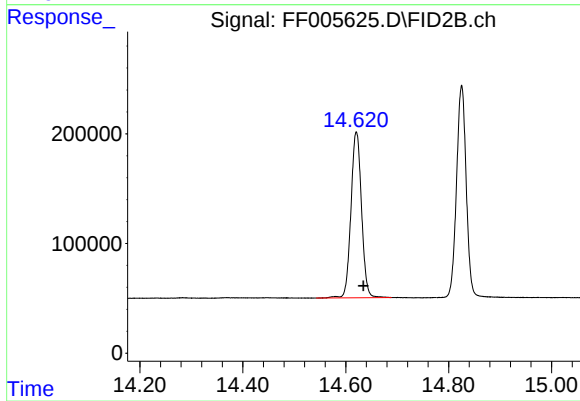

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.621 min
Delta R.T.: -0.014 min
Response: 2156222
Conc: 20.15 ug/ml

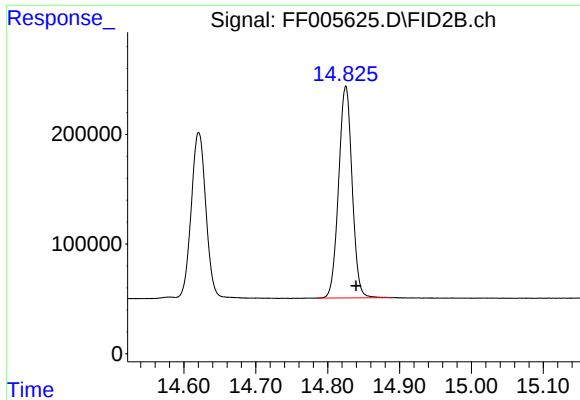

#10 N-TETRACOSANE


R.T.: 14.825 min
Delta R.T.: -0.014 min
Response: 2515802
Conc: 20.57 ug/ml

Instrument :
FID_F
ClientSampleId :
PB123221BS

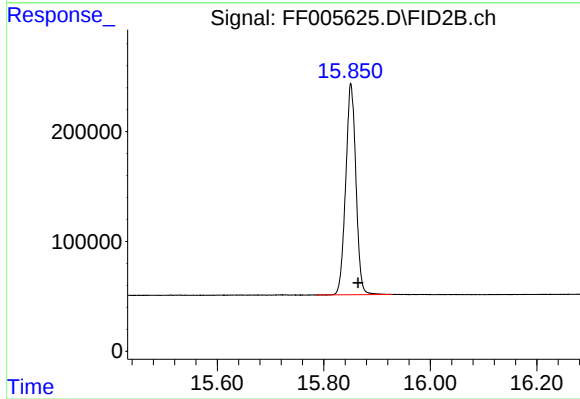

#11 N-HEXACOSANE

R.T.: 15.851 min
Delta R.T.: -0.013 min
Response: 2562058
Conc: 21.40 ug/ml

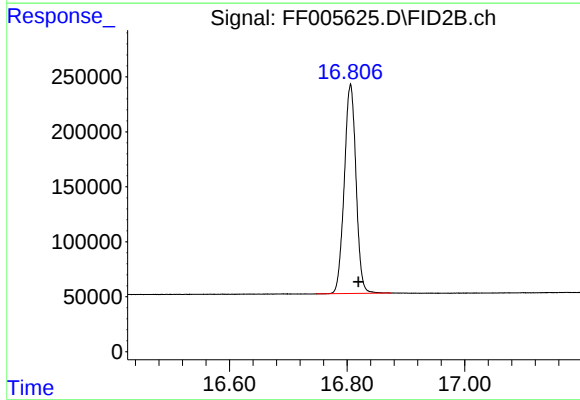

#12 N-OCTACOSANE

R.T.: 16.806 min
Delta R.T.: -0.013 min
Response: 2638050
Conc: 22.11 ug/ml