

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091924\
Data File : FF014534.D
Signal(s) : FID2B.ch
Acq On : 19 Sep 2024 16:03
Operator : YP\AJ
Sample : P4103-10
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-14-7.5-10A

Integration File: autoint1.e
Quant Time: Sep 20 02:27:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF091124.M
Quant Title :
QLast Update : Tue Sep 10 16:18:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.896	1220334	11.372 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091924\
Data File : FF014534.D
Signal(s) : FID2B.ch
Acq On : 19 Sep 2024 16:03
Operator : YP\AJ
Sample : P4103-10
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WC-14-7.5-10A

Integration File: autoint1.e
Quant Time: Sep 20 02:27:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF091124.M
Quant Title :
QLast Update : Tue Sep 10 16:18:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

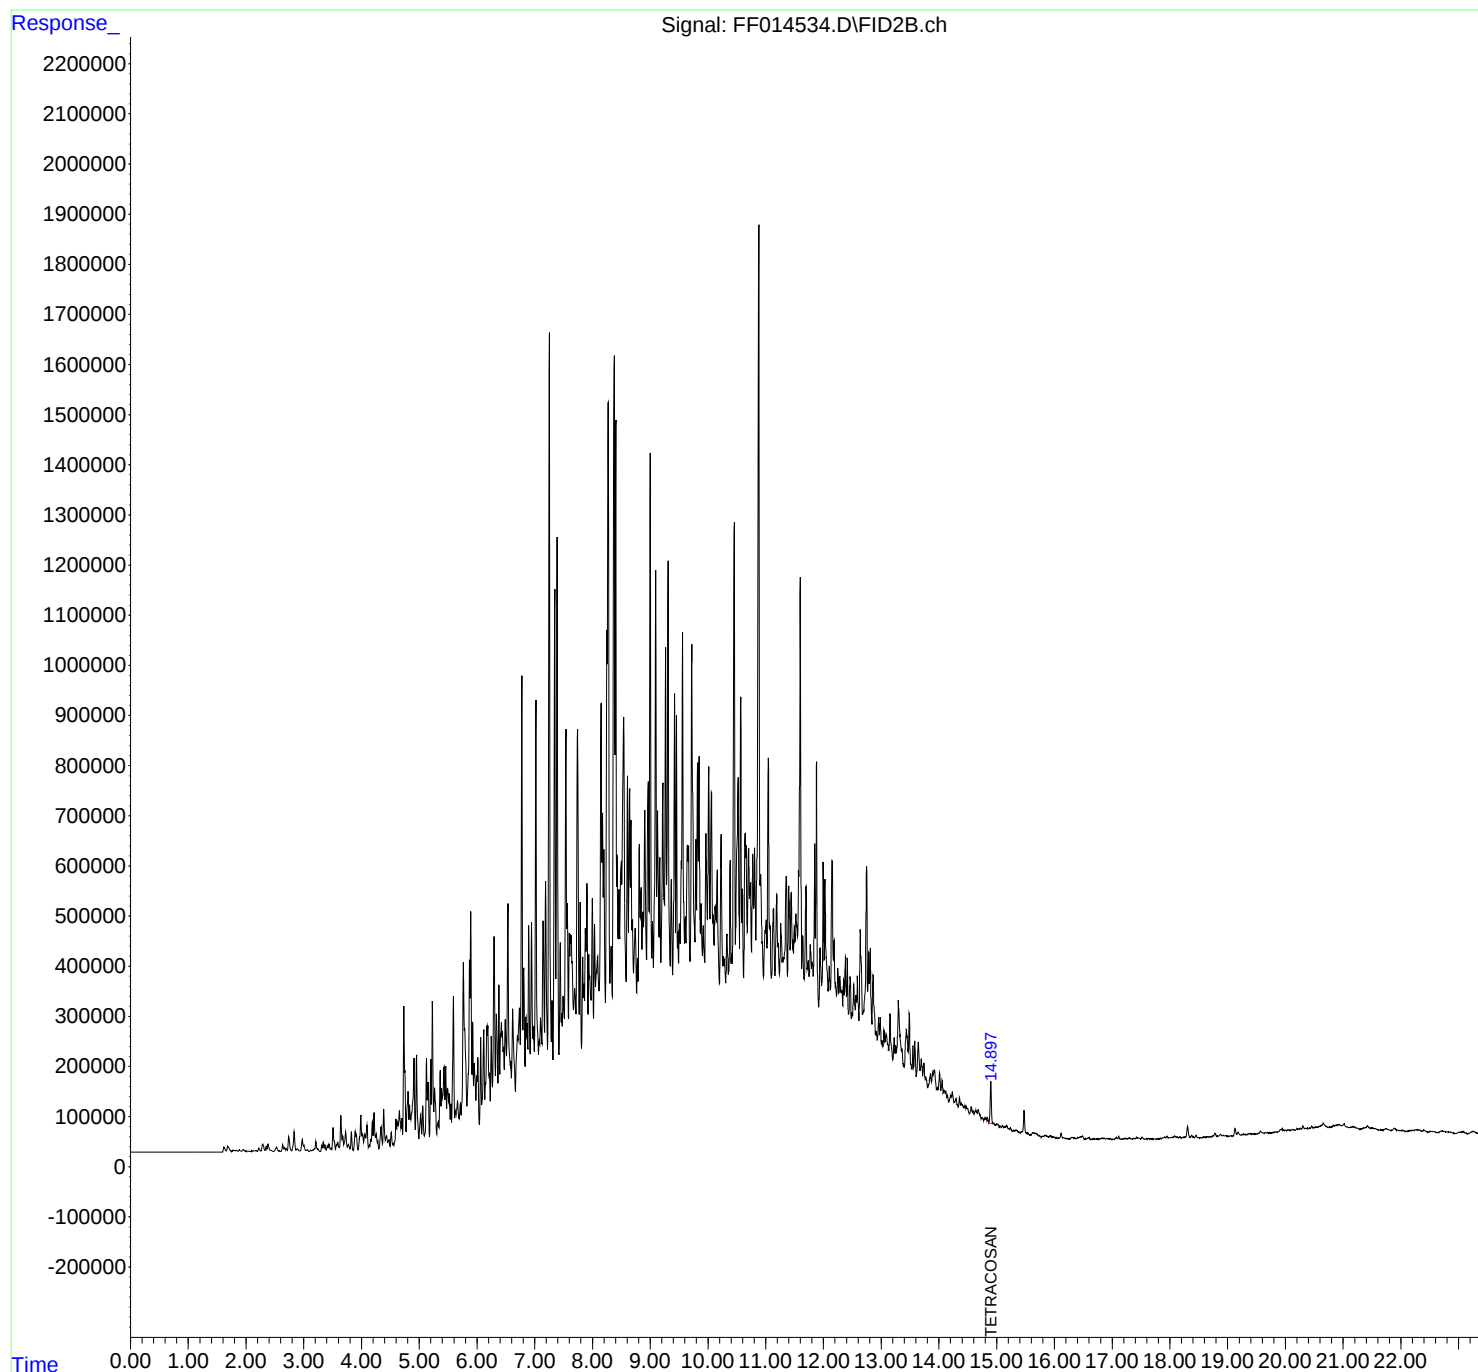

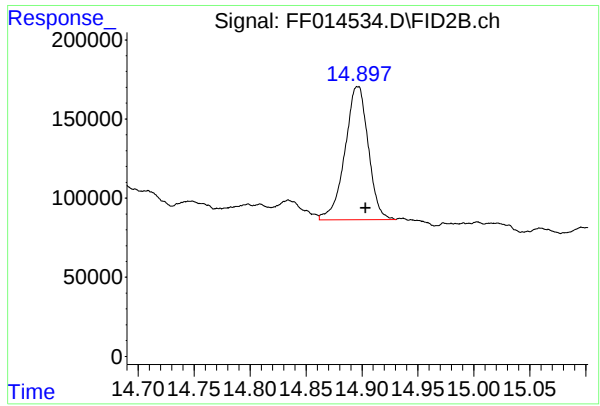

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.896 min
Delta R.T.: -0.007 min
Response: 1220334
Conc: 11.37 ug/ml

Instrument :
FID_F
ClientSampleId :
WC-14-7.5-10A