

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092021\
Data File : FF008970.D
Signal(s) : FID2B.ch
Acq On : 20 Sep 2021 12:34
Operator : DD\AJ
Sample : PB139086BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 21 09:34:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.716	2310040	19.665 ug/ml
Target Compounds				
16)	N-HEXATRIACONTANE	20.147	152965	1.750 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092021\
Data File : FF008970.D
Signal(s) : FID2B.ch
Acq On : 20 Sep 2021 12:34
Operator : DD\AJ
Sample : PB139086BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 21 09:34:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

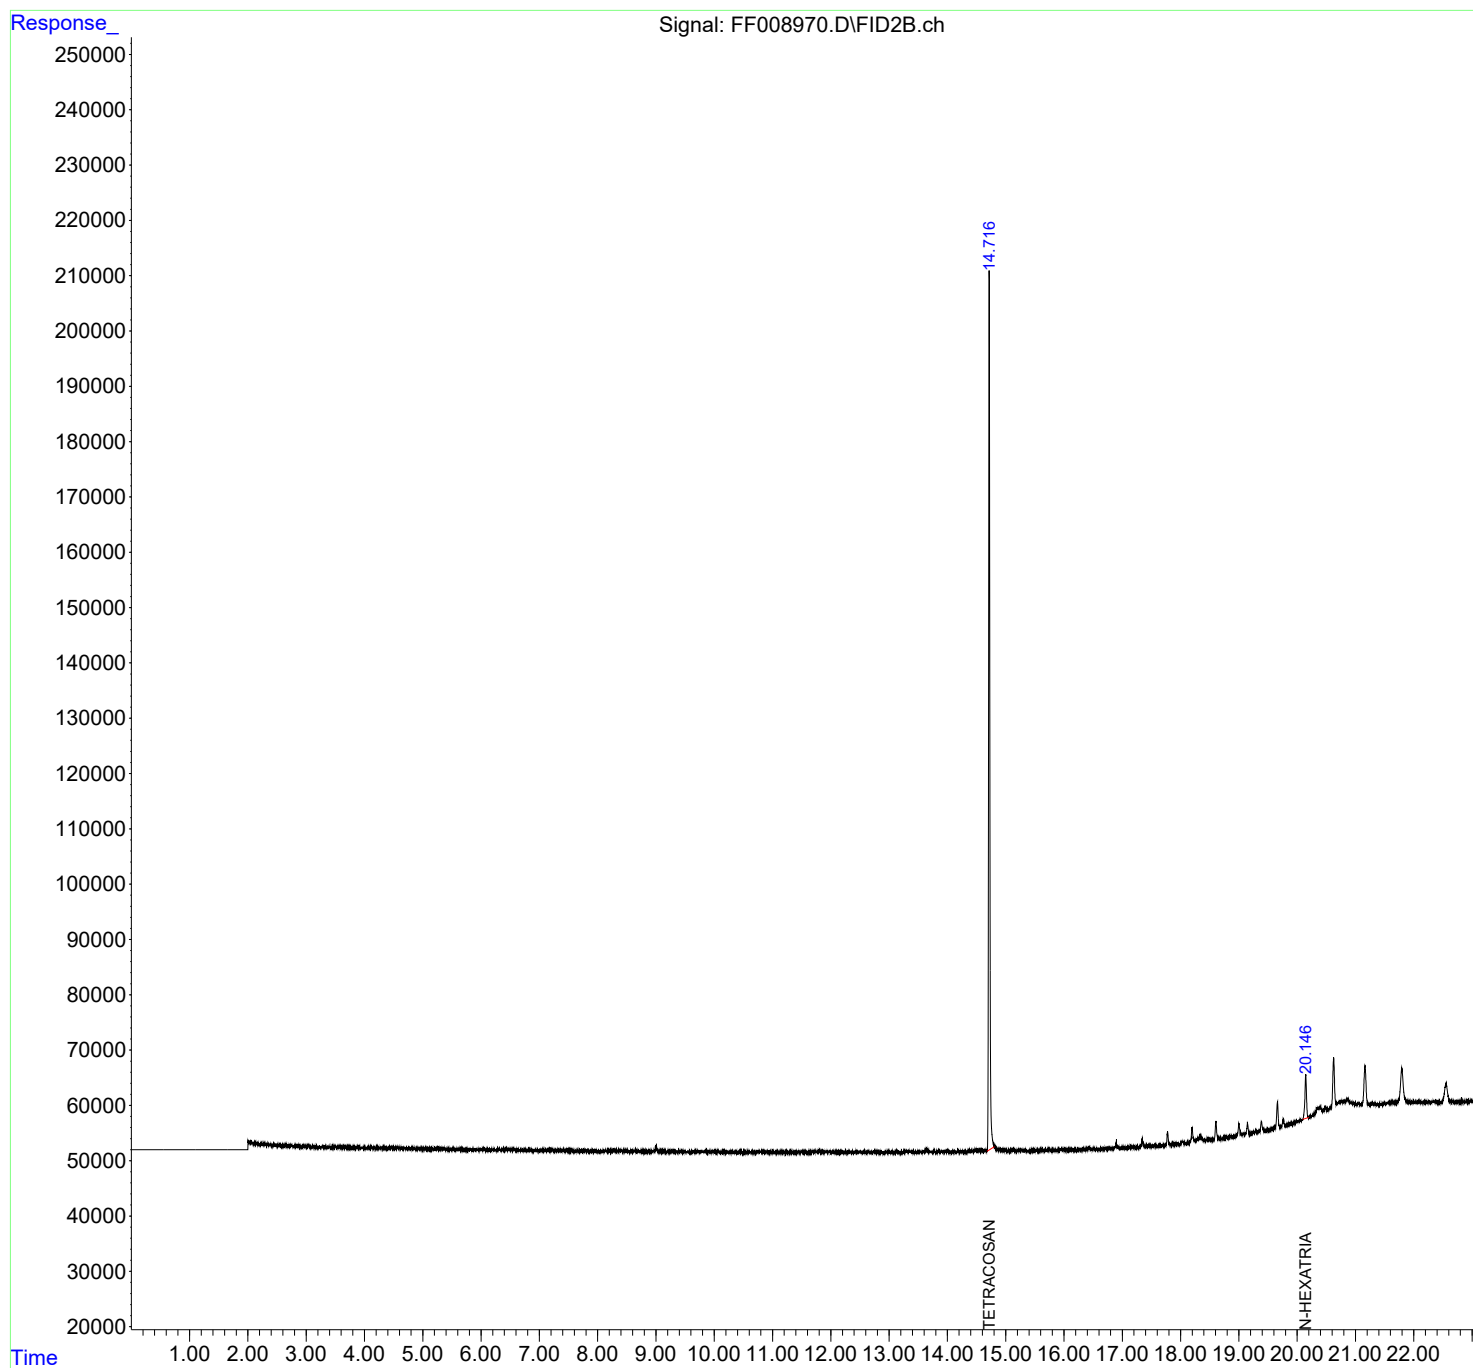


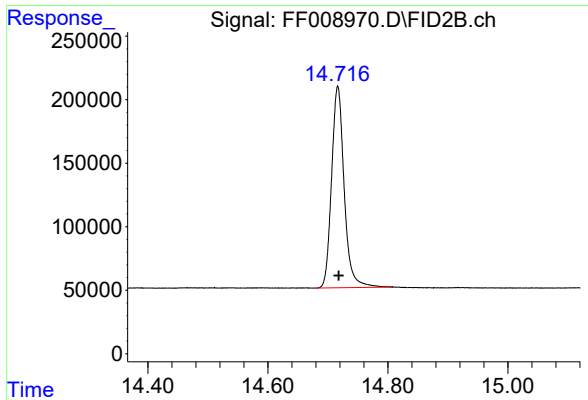

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.716 min
Delta R.T.: -0.002 min
Response: 2310040
Conc: 19.66 ug/ml

Instrument :
FID_F
ClientSampleId :

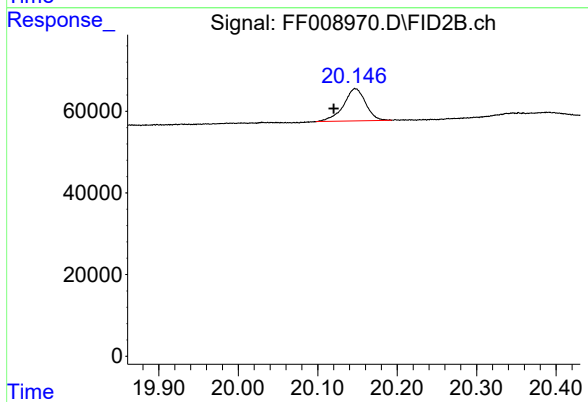

#16 N-HEXATRIACONTANE

R.T.: 20.147 min
Delta R.T.: 0.026 min
Response: 152965
Conc: 1.75 ug/ml