

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092021\
 Data File : FF008972.D
 Signal(s) : FID2B.ch
 Acq On : 20 Sep 2021 15:58
 Operator : DD\AJ
 Sample : M3702-19 5X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
ClientSampleId :
 RR-DIES-WP

Integration File: Sample.e
 Quant Time: Sep 21 09:35:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
 Quant Title :
 QLast Update : Wed Sep 08 10:20:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.717	523526	4.457 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092021\
 Data File : FF008972.D
 Signal(s) : FID2B.ch
 Acq On : 20 Sep 2021 15:58
 Operator : DD\AJ
 Sample : M3702-19 5X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RR-DIES-WP

Integration File: Sample.e
 Quant Time: Sep 21 09:35:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
 Quant Title :
 QLast Update : Wed Sep 08 10:20:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

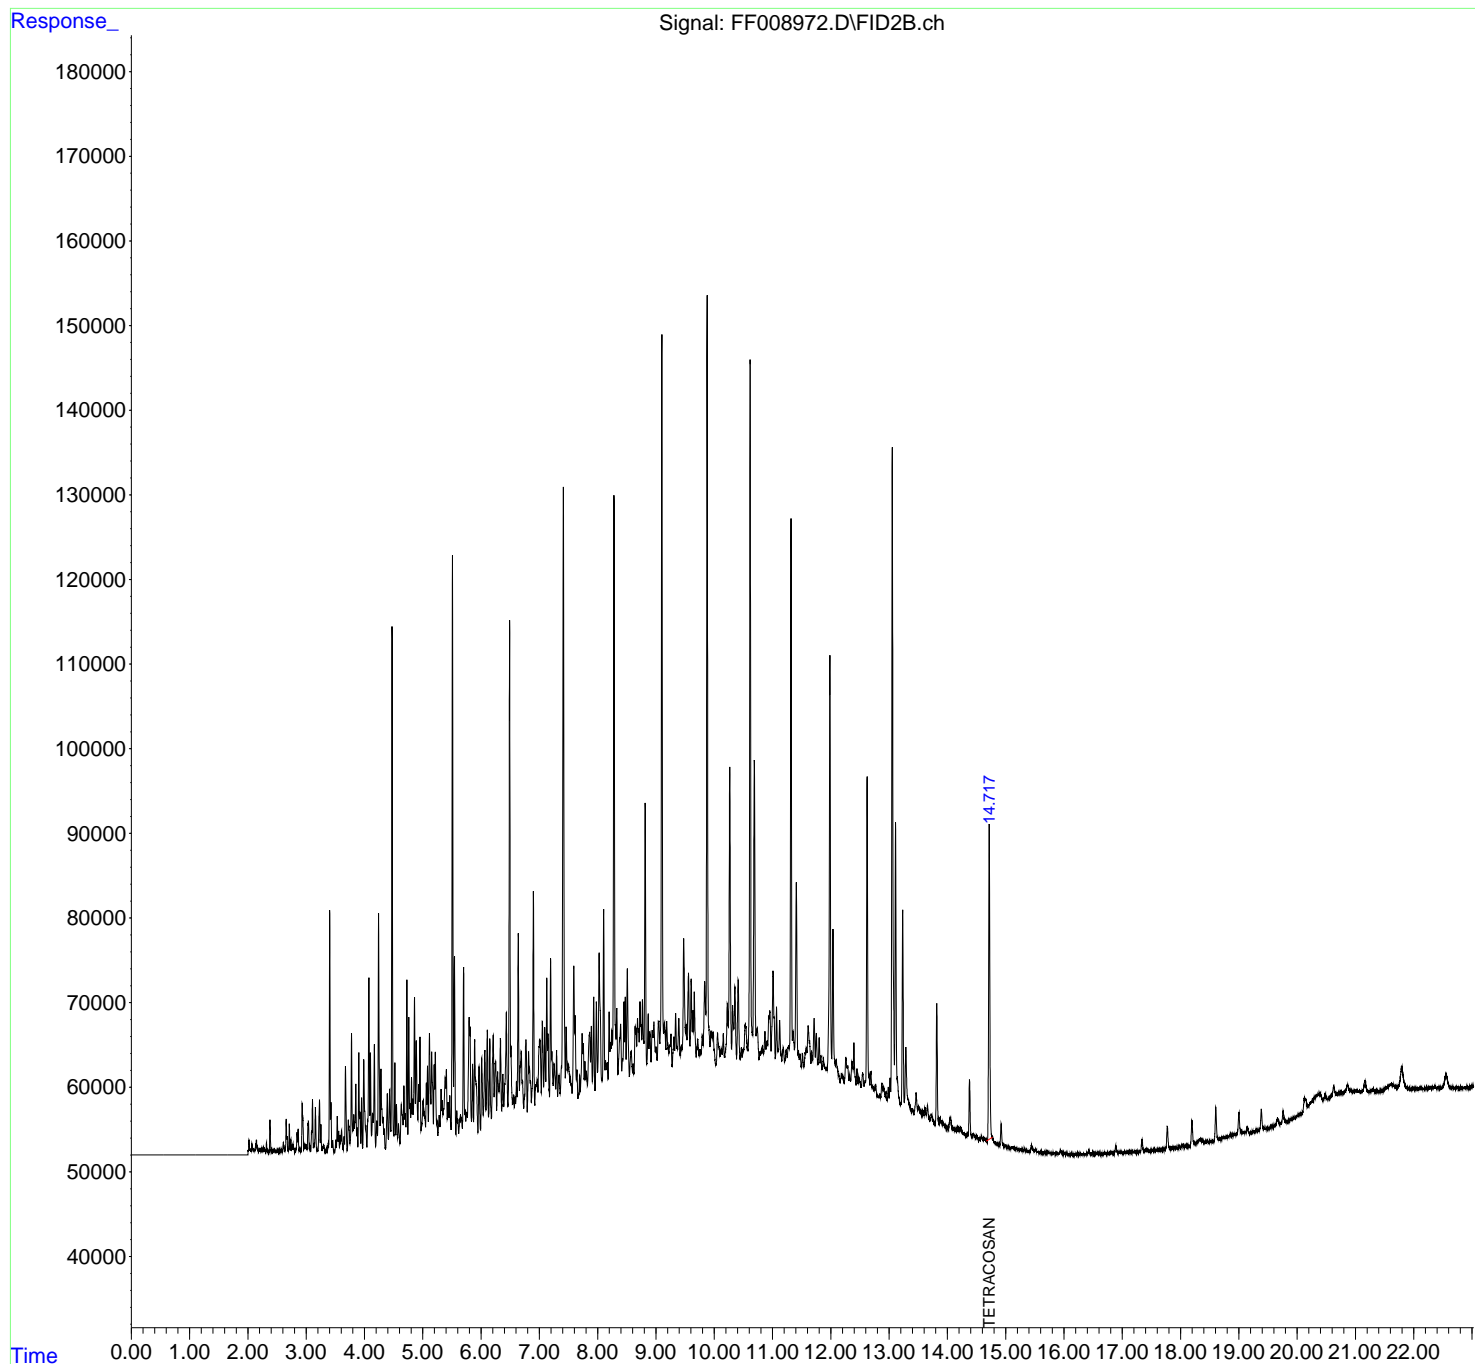

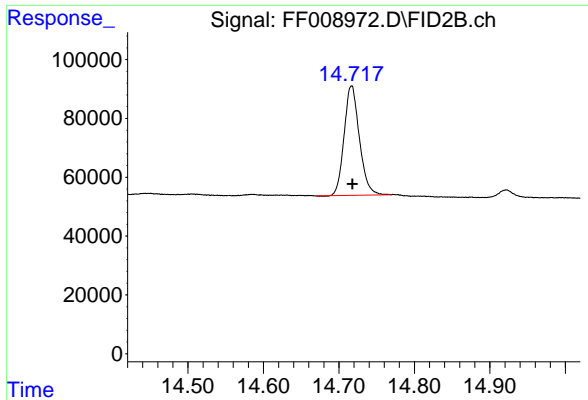

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.717 min
Delta R.T.: -0.001 min
Response: 523526
Conc: 4.46 ug/ml

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP