

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092024\
 Data File : FF014560.D
 Signal(s) : FID2B.ch
 Acq On : 20 Sep 2024 13:04
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 21 00:29:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF091124.M
 Quant Title :
 QLast Update : Tue Sep 10 16:18:04 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.612	2127982	18.783 ug/ml
12)	N-OCTACOSANE	17.064	2082435	18.084 ug/ml
13)	N-TRIACONTANE	17.950	174687	1.509 ug/ml
14)	N-DOTRIACONTANE	18.781	233575	2.064 ug/ml
15)	N-TETRATRIACONTANE	19.561	191649	1.782 ug/ml
16)	N-HEXATRIACONTANE	20.302	115301	1.177 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092024\
Data File : FF014560.D
Signal(s) : FID2B.ch
Acq On : 20 Sep 2024 13:04
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 21 00:29:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF091124.M
Quant Title :
QLast Update : Tue Sep 10 16:18:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

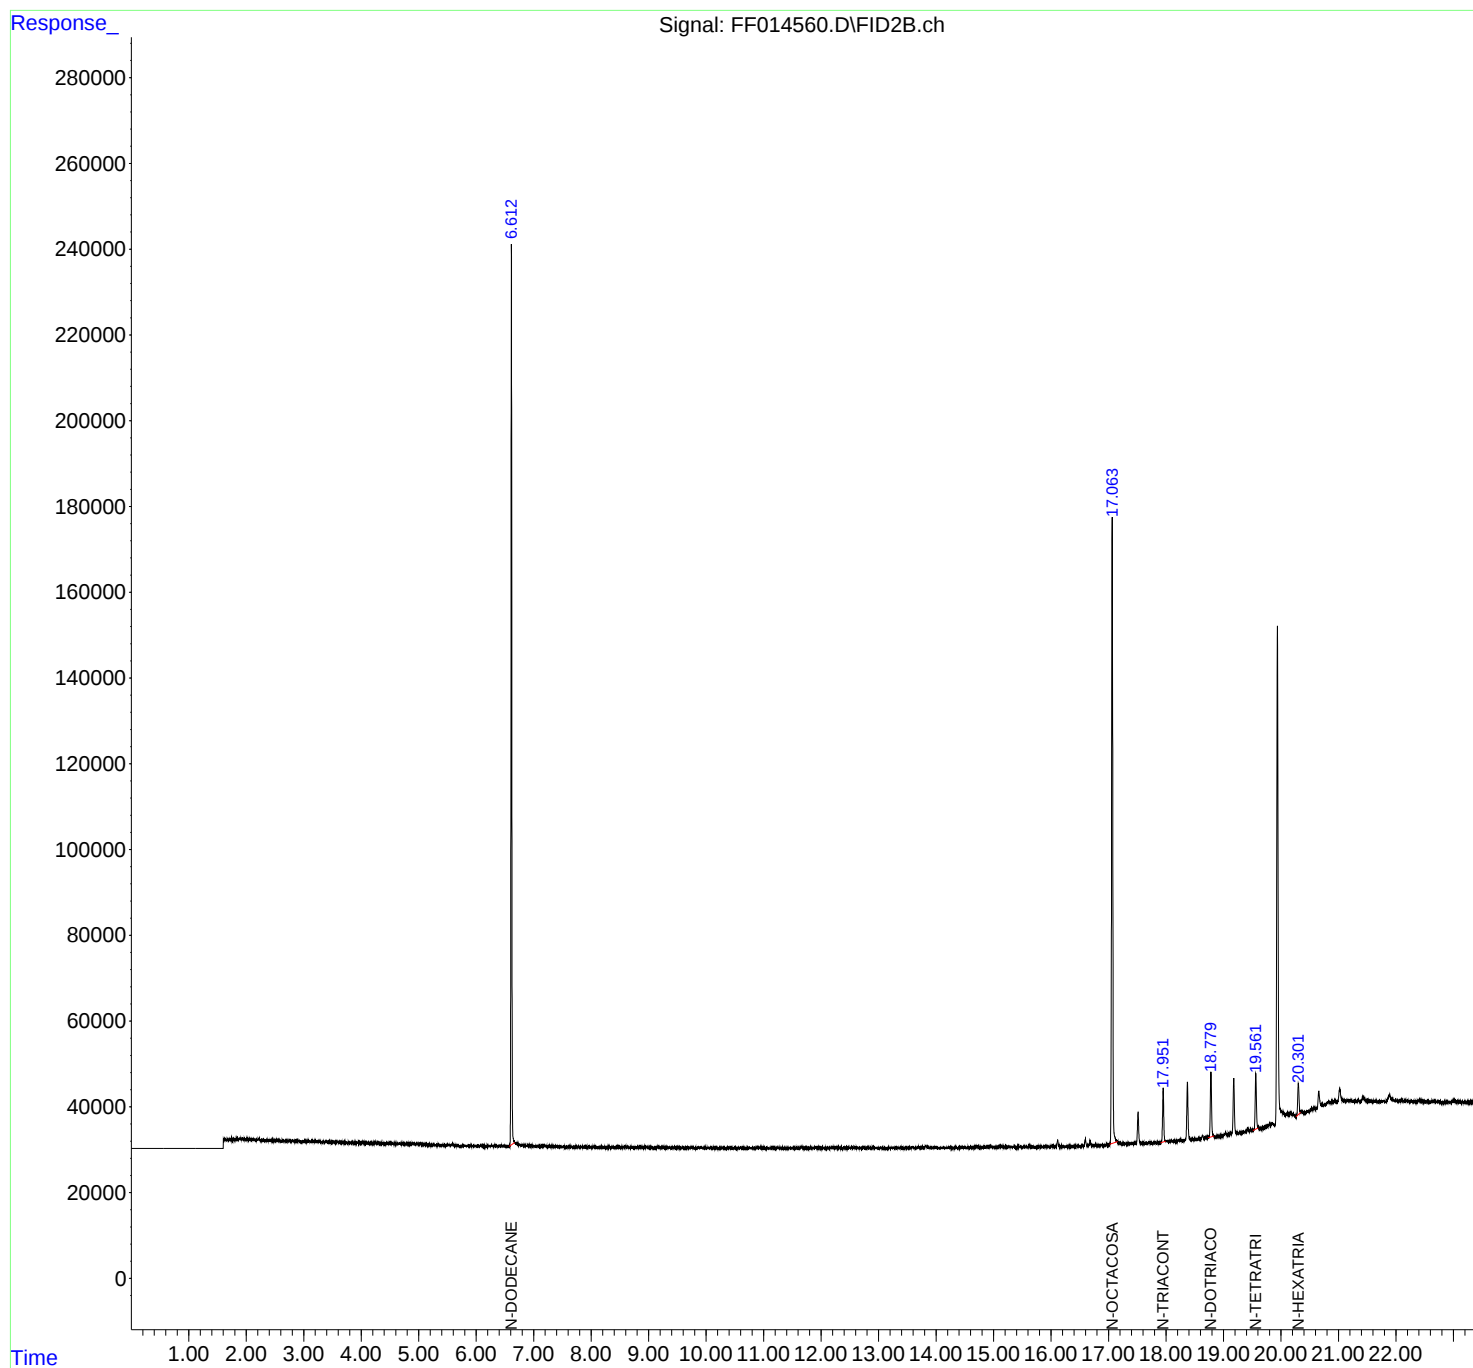


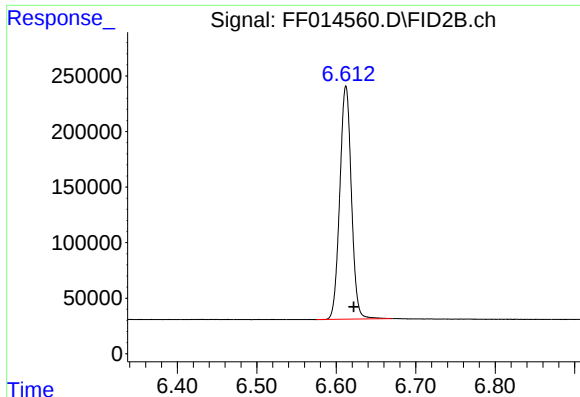

#3 N-DODECANE


R.T.: 6.612 min
Delta R.T.: -0.010 min
Response: 2127982
Conc: 18.78 ug/ml

Instrument :
FID_F
ClientSampleId :

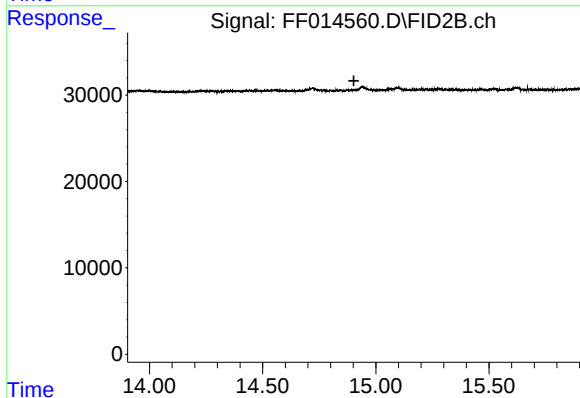


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.903 min
Response: 0
Conc: N.D.

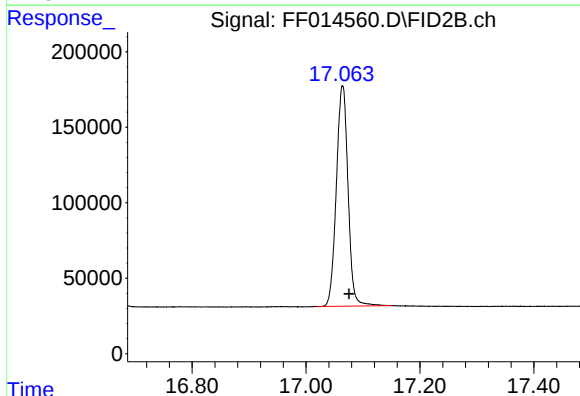


#12 N-OCTACOSANE

R.T.: 17.064 min
Delta R.T.: -0.011 min
Response: 2082435
Conc: 18.08 ug/ml

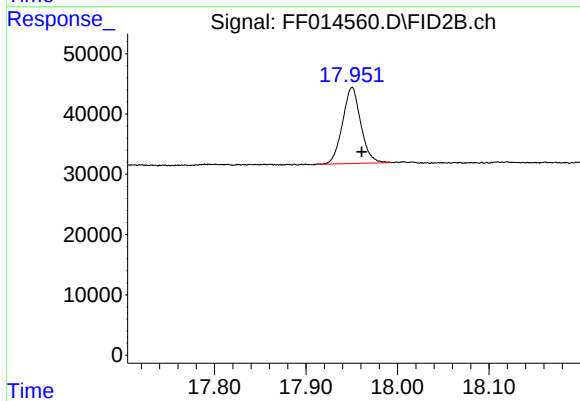

#13 N-TRIACONTANE


R.T.: 17.950 min
Delta R.T.: -0.011 min
Response: 174687
Conc: 1.51 ug/ml

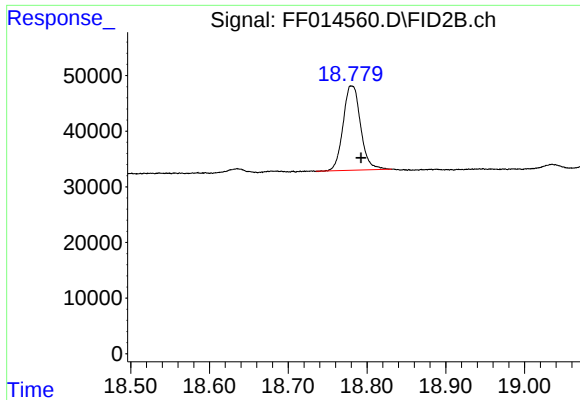

#14 N-DOTRIACONTANE


R.T.: 18.781 min
Delta R.T.: -0.012 min
Response: 233575
Conc: 2.06 ug/ml

Instrument :
FID_F
ClientSampleId :

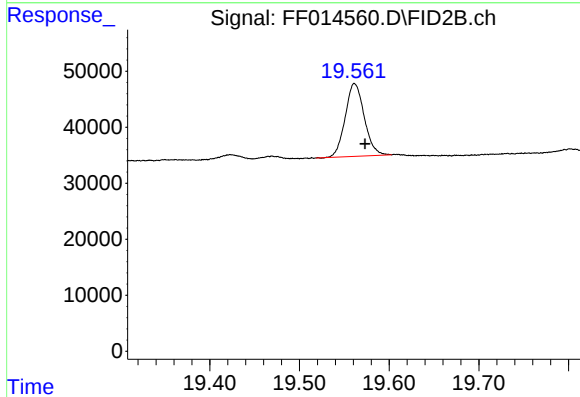

#15 N-TETRATRIACONTANE

R.T.: 19.561 min
Delta R.T.: -0.012 min
Response: 191649
Conc: 1.78 ug/ml

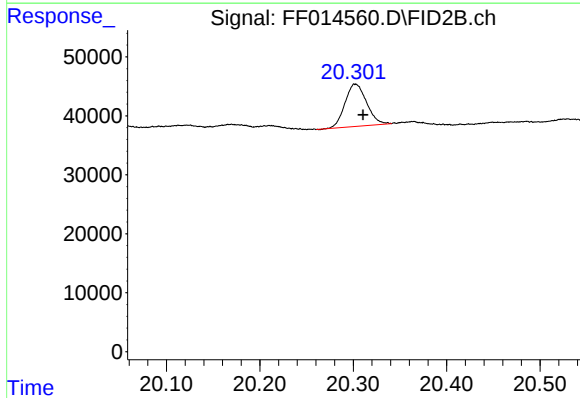

#16 N-HEXATRIACONTANE

R.T.: 20.302 min
Delta R.T.: -0.008 min
Response: 115301
Conc: 1.18 ug/ml