

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092024\
Data File : FF014552.D
Signal(s) : FID2B.ch
Acq On : 20 Sep 2024 07:29
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 20 09:54:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF091124.M
Quant Title :
QLast Update : Tue Sep 10 16:18:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.891	2288802	21.329 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092024\
Data File : FF014552.D
Signal(s) : FID2B.ch
Acq On : 20 Sep 2024 07:29
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 20 09:54:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF091124.M
Quant Title :
QLast Update : Tue Sep 10 16:18:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

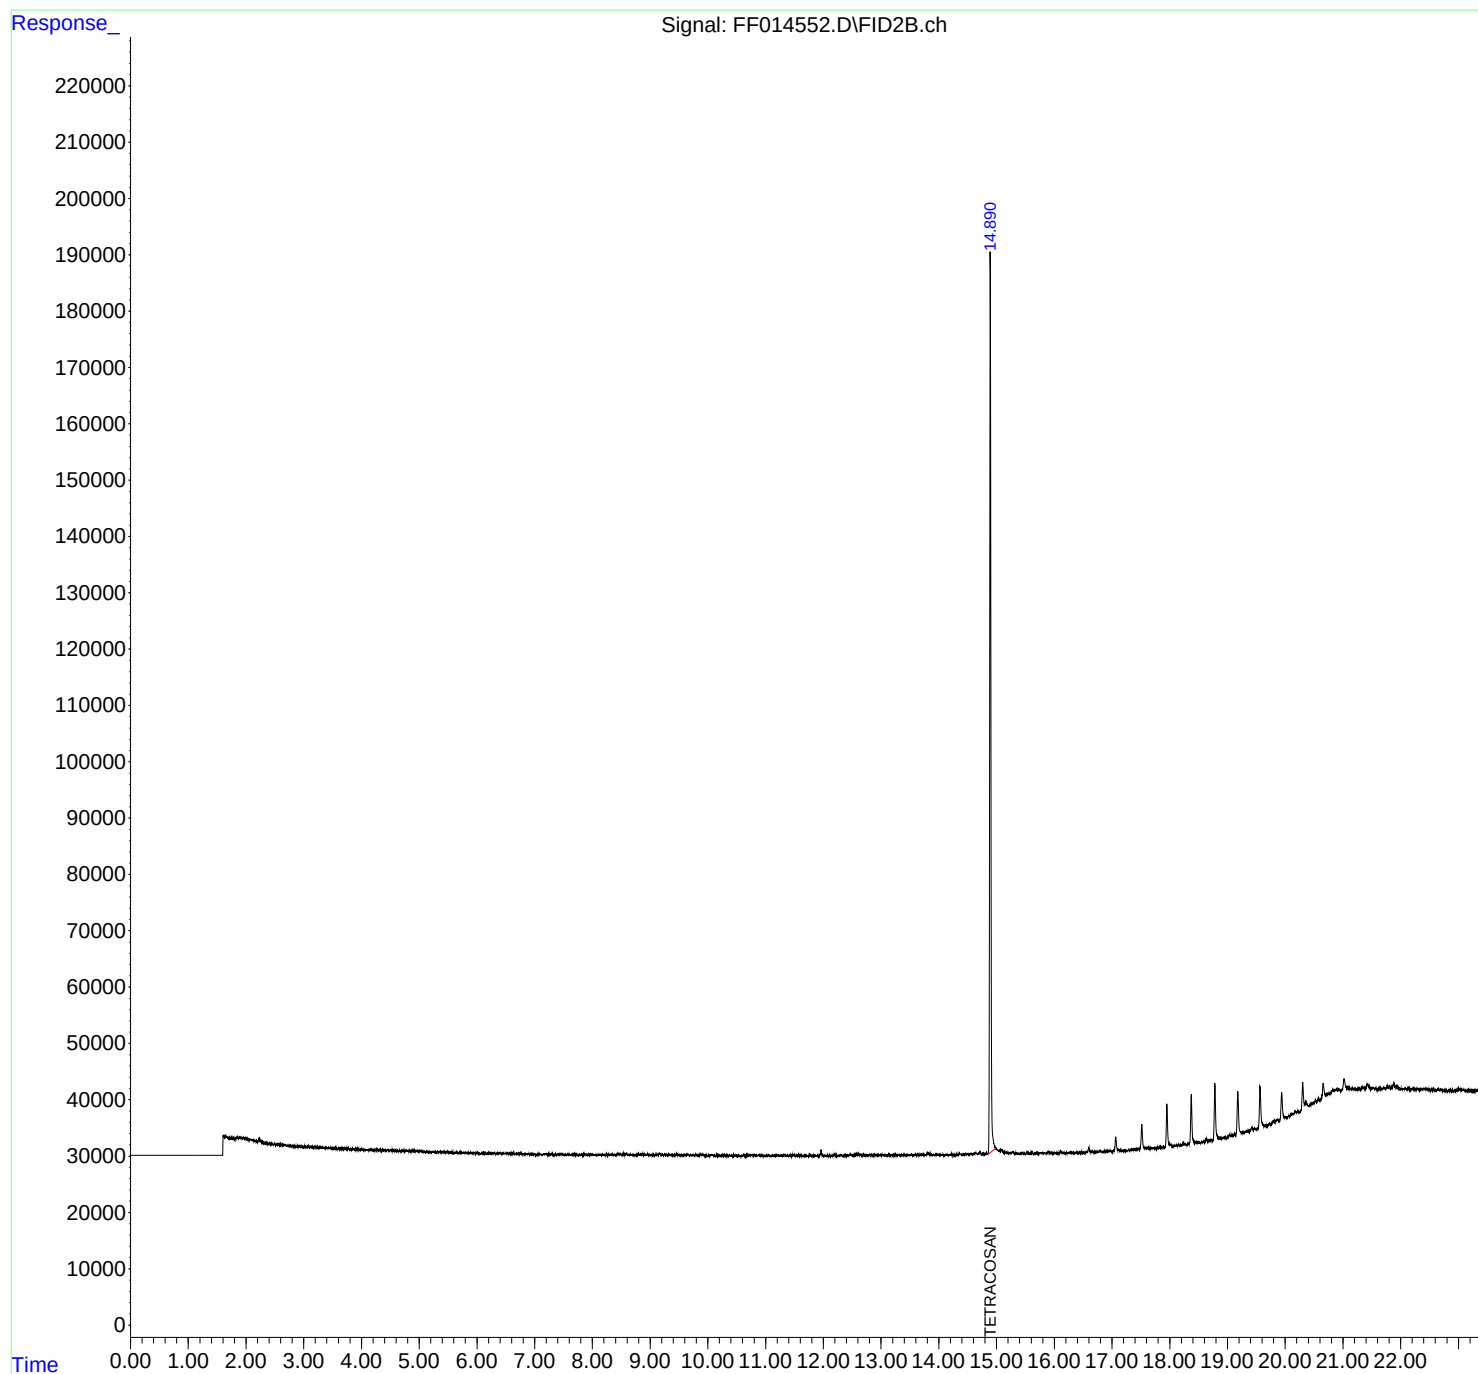

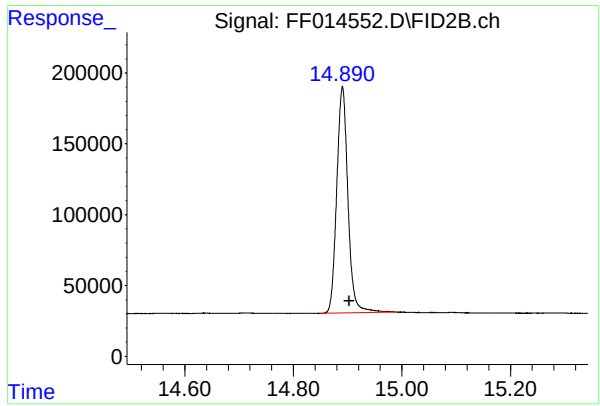

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.891 min
Delta R.T.: -0.012 min
Response: 2288802
Conc: 21.33 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK