

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092121\
Data File : FF008983.D
Signal(s) : FID2B.ch
Acq On : 21 Sep 2021 15:14
Operator : DD\AJ
Sample : M3823-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 22 01:28:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.715	2244161	19.104 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.594	145916	1.352 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092121\
Data File : FF008983.D
Signal(s) : FID2B.ch
Acq On : 21 Sep 2021 15:14
Operator : DD\AJ
Sample : M3823-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 22 01:28:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

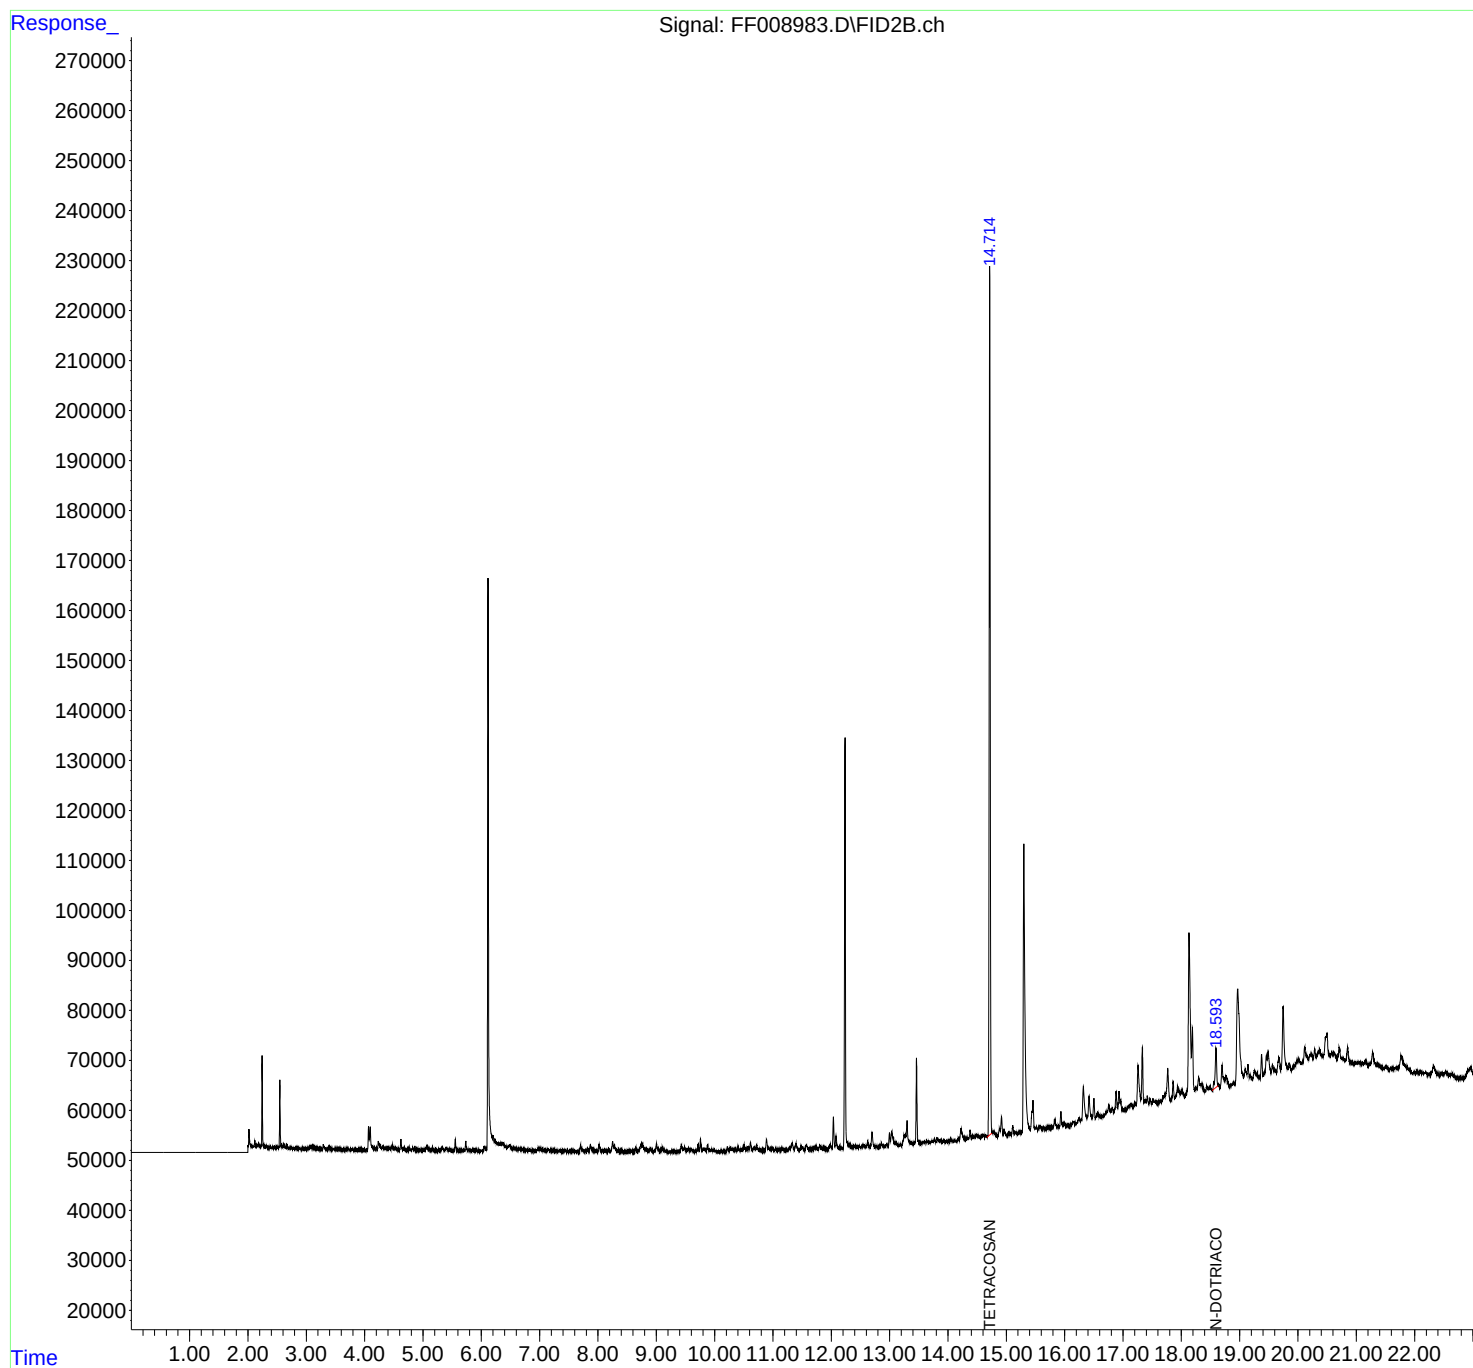


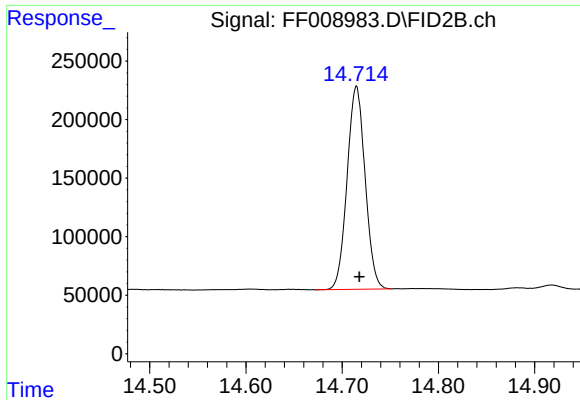

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.715 min
Delta R.T.: -0.003 min
Response: 2244161
Conc: 19.10 ug/ml

Instrument :
FID_F
ClientSampleId :

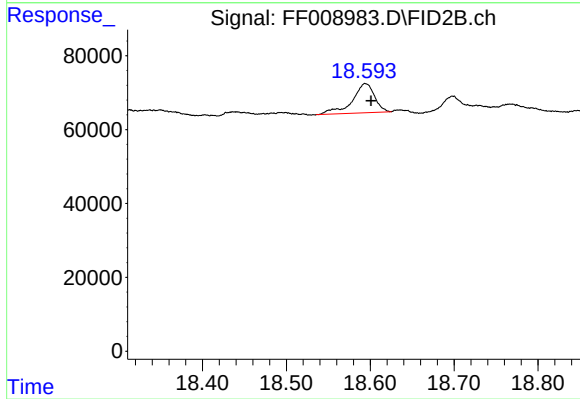

#14 N-DOTRIACONTANE

R.T.: 18.594 min
Delta R.T.: -0.008 min
Response: 145916
Conc: 1.35 ug/ml