

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092121\
Data File : FF008979.D
Signal(s) : FID2B.ch
Acq On : 21 Sep 2021 11:26
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Sep 22 01:27:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.483	3591124	25.431 ug/ml
12) N-OCTACOSANE	16.884	3217719	26.300 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092121\
Data File : FF008979.D
Signal(s) : FID2B.ch
Acq On : 21 Sep 2021 11:26
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Sep 22 01:27:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

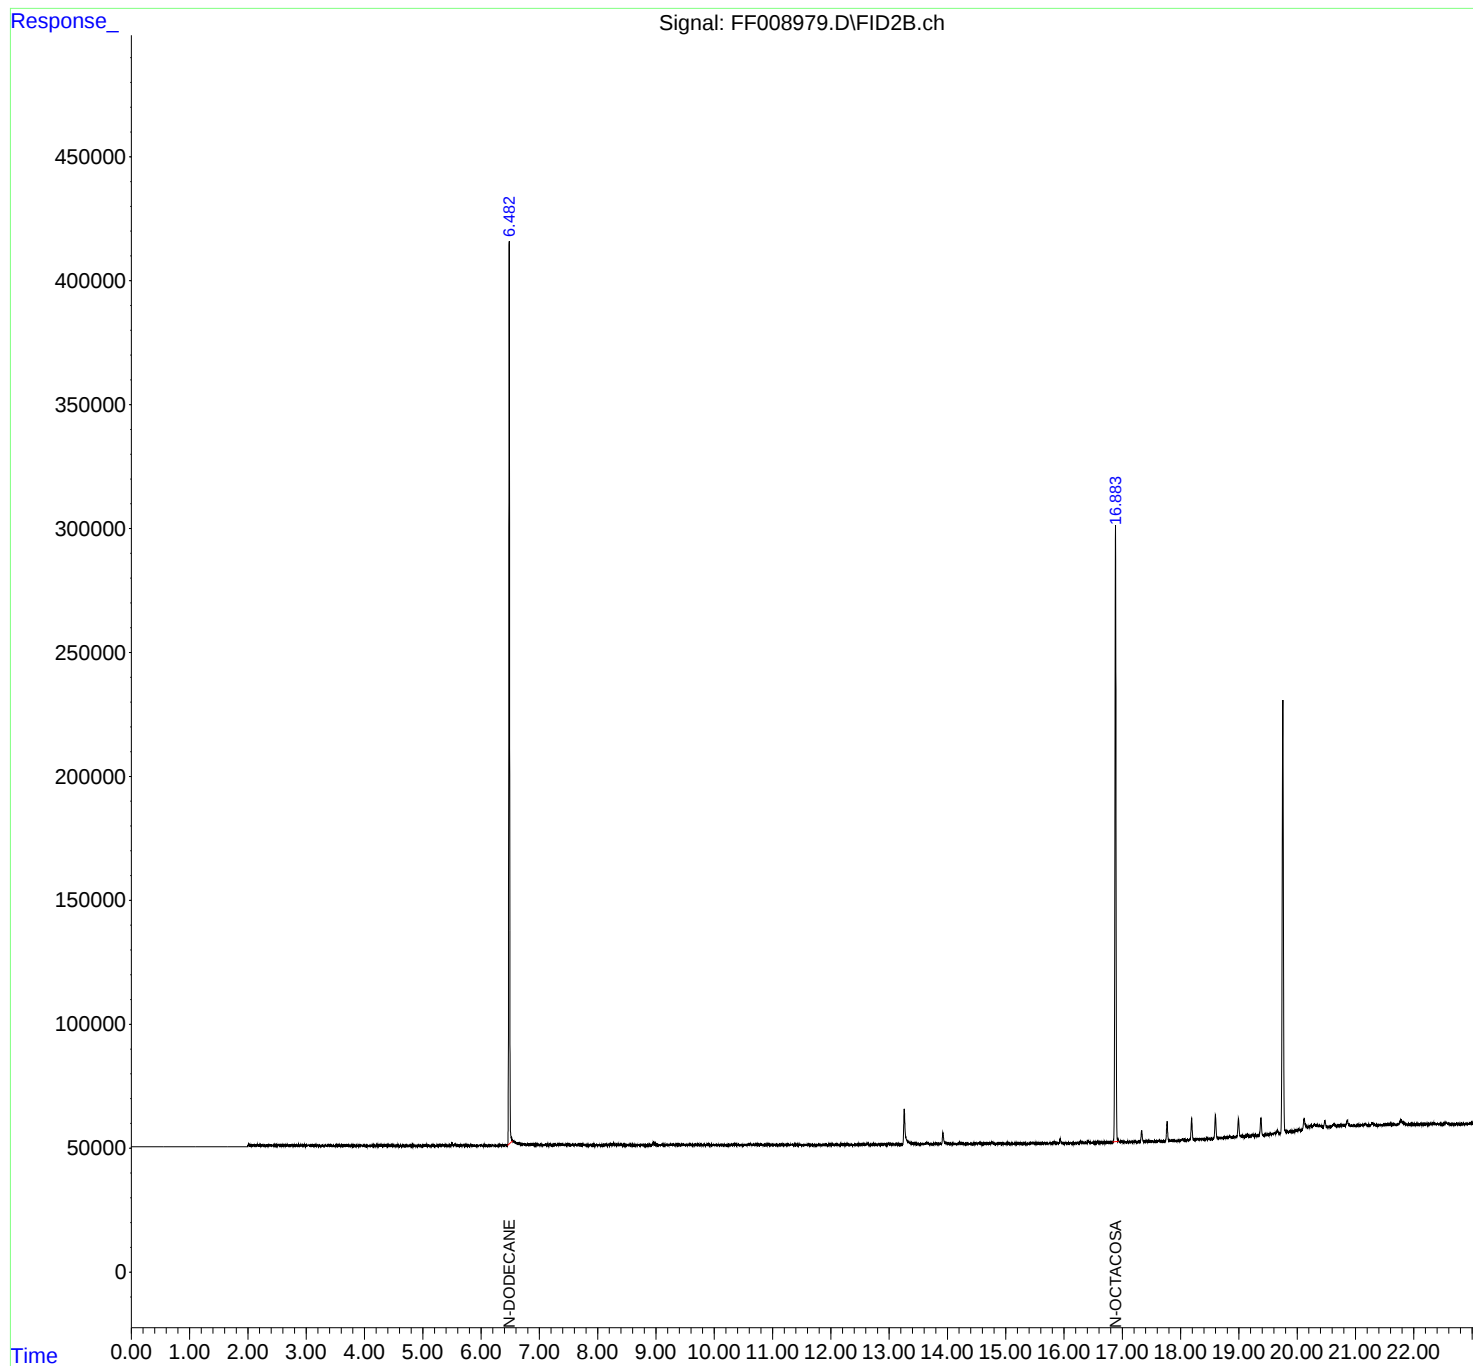


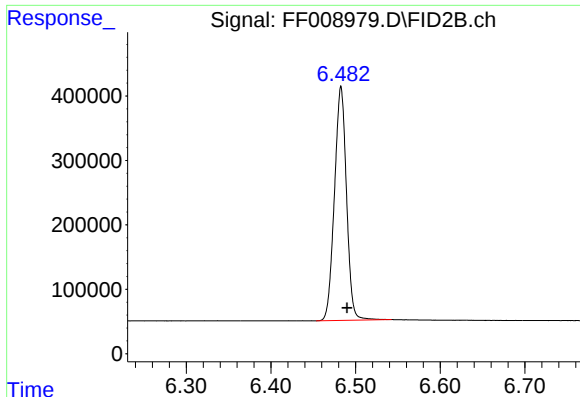

#3 N-DODECANE


R.T.: 6.483 min
Delta R.T.: -0.007 min
Response: 3591124
Conc: 25.43 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

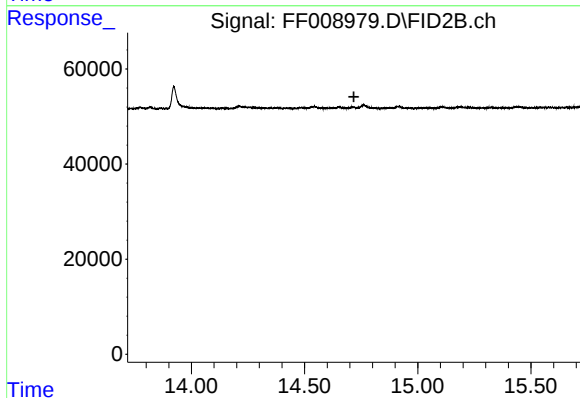

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.718 min
Response: 0
Conc: N.D.

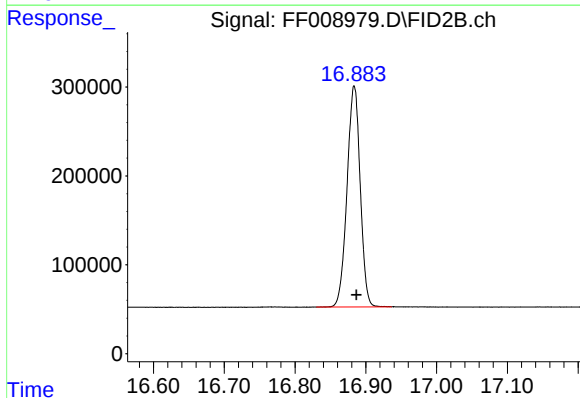

#12 N-OCTACOSANE

R.T.: 16.884 min
Delta R.T.: -0.003 min
Response: 3217719
Conc: 26.30 ug/ml