

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092121\
Data File : FF008980.D
Signal(s) : FID2B.ch
Acq On : 21 Sep 2021 13:42
Operator : DD\AJ
Sample : PB139238BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB139238BL

Integration File: Sample.e
Quant Time: Sep 22 01:28:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	2242797	19.092 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092121\
Data File : FF008980.D
Signal(s) : FID2B.ch
Acq On : 21 Sep 2021 13:42
Operator : DD\AJ
Sample : PB139238BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB139238BL

Integration File: Sample.e
Quant Time: Sep 22 01:28:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

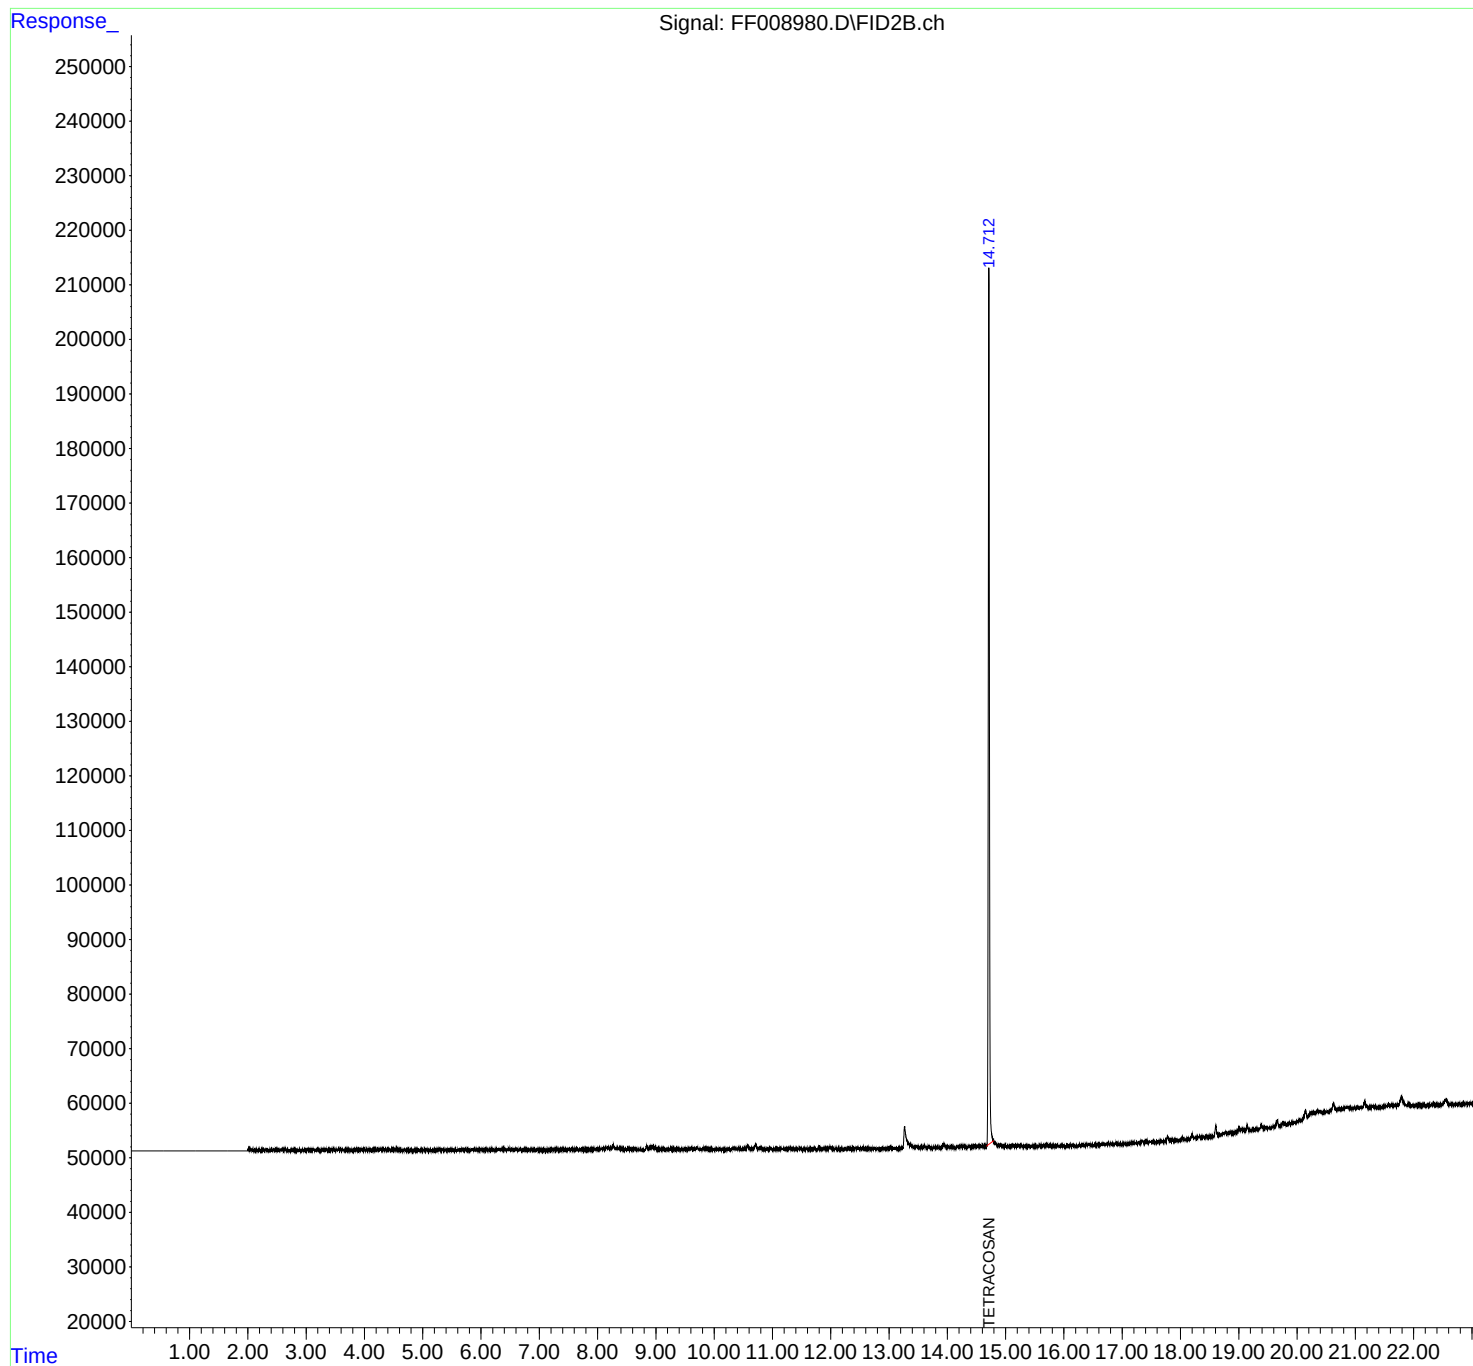

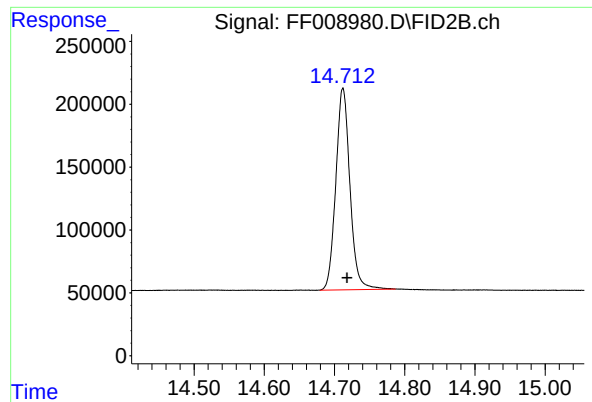

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.712 min
Delta R.T.: -0.006 min
Response: 2242797
Conc: 19.09 ug/ml

Instrument :
FID_F
ClientSampleId :
PB139238BL