

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092121\
 Data File : FF008982.D
 Signal(s) : FID2B.ch
 Acq On : 21 Sep 2021 14:43
 Operator : DD\AJ
 Sample : M3823-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 DKM-ENV-IG-COMP

Integration File: Sample.e
 Quant Time: Sep 22 01:28:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
 Quant Title :
 QLast Update : Wed Sep 08 10:20:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.714	1603156	13.647 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092121\
Data File : FF008982.D
Signal(s) : FID2B.ch
Acq On : 21 Sep 2021 14:43
Operator : DD\AJ
Sample : M3823-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
DKM-ENV-IG-COMP

Integration File: Sample.e
Quant Time: Sep 22 01:28:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

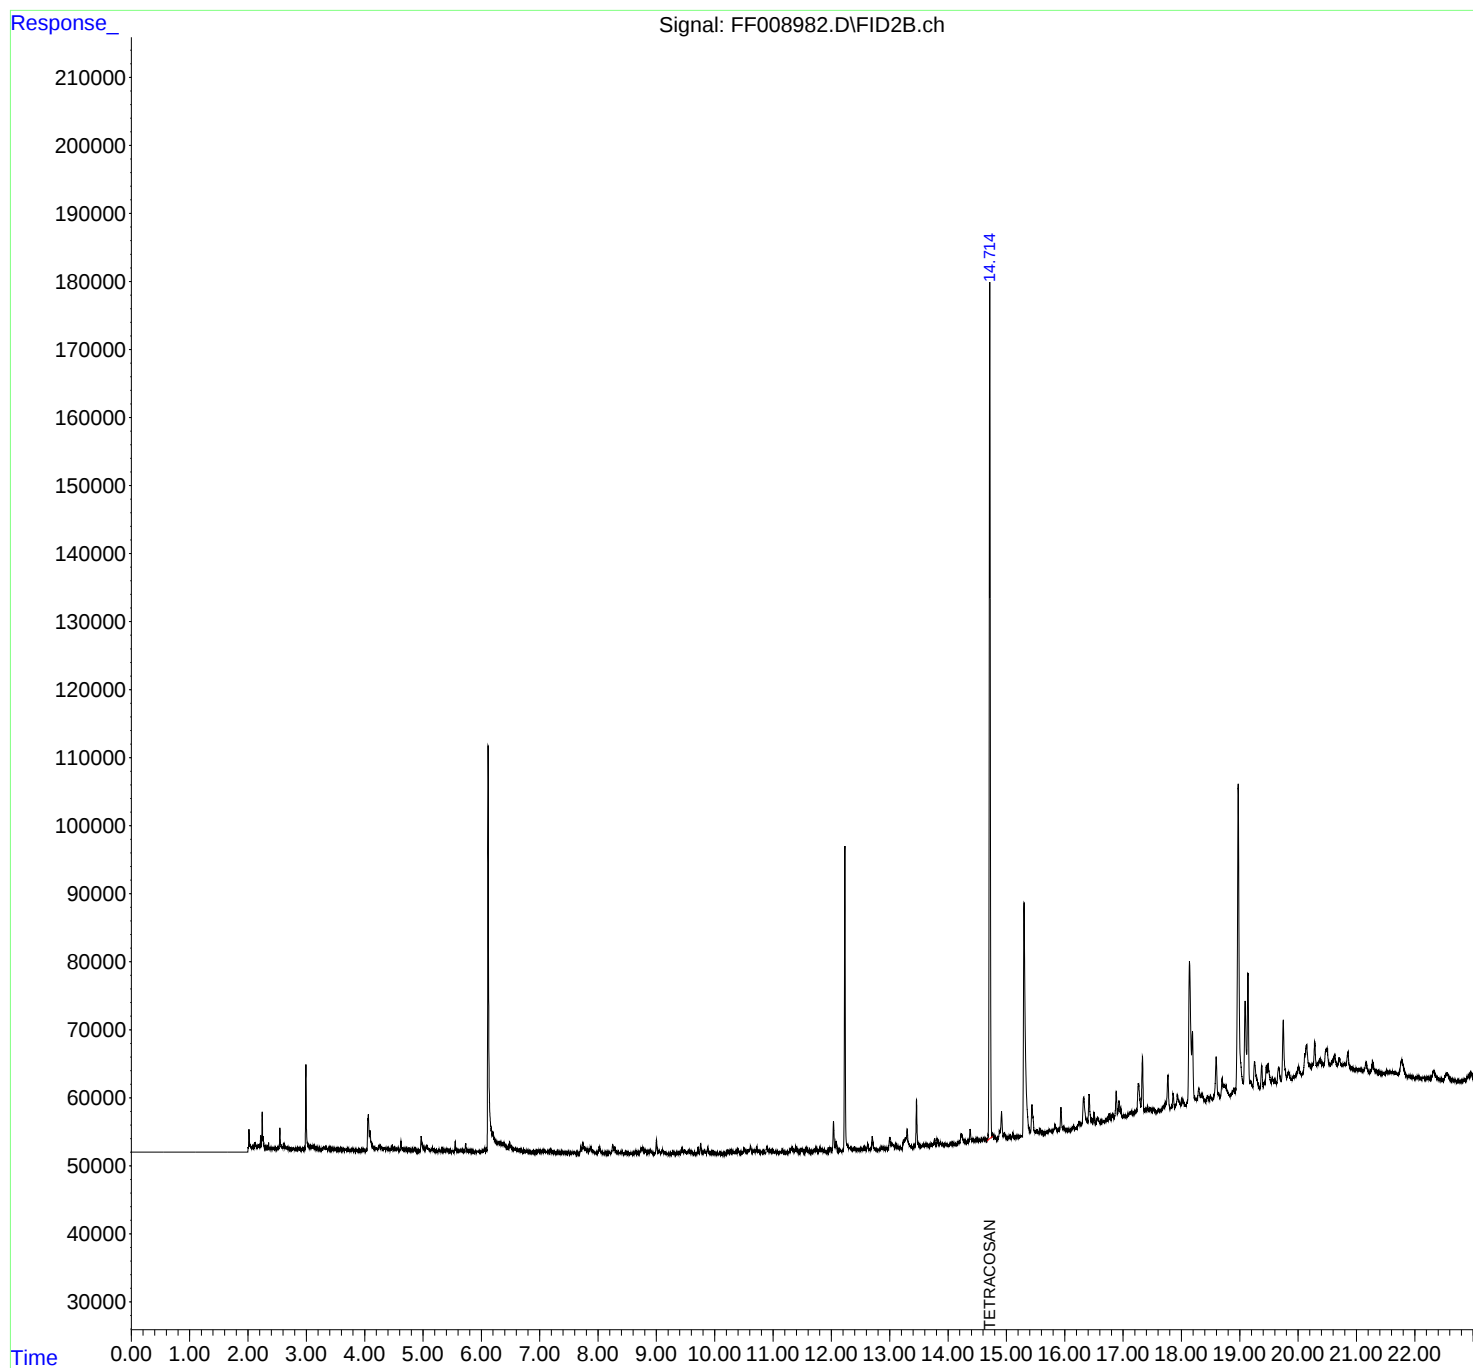

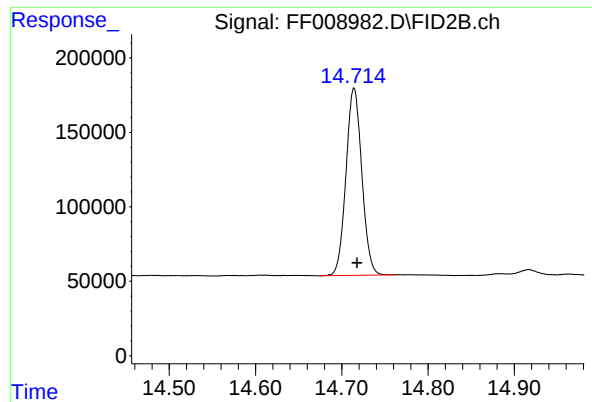

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.714 min
Delta R.T.: -0.004 min
Response: 1603156
Conc: 13.65 ug/ml

Instrument :
FID_F
ClientSampleId :
DKM-ENV-IG-COMP