

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092225AL\
 Data File : FE055933.D
 Signal(s) : FID1B.ch
 Acq On : 22 Sep 2025 19:57
 Operator : YP\AJ
 Sample : Q3135-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 23 04:35:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 082925.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 29 08:12:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.512	6318555	50.530 ug/ml
Spiked Amount 50.000		Recovery =	101.06%
Target Compounds			
17) T n-Tricontane (C30)	18.236	151087	1.022 ug/ml
18) T n-Dotriacontane (C32)	19.071	180071	1.227 ug/ml
19) T n-Tetratriacontane (C34)	19.856	137814	0.975 ug/ml
20) T n-Hexatriacontane (C36)	20.599	100950	0.765 ug/ml
22) T n-Tetracontane (C40)	22.357	202297	1.577 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092225AL\
Data File : FE055933.D
Signal(s) : FID1B.ch
Acq On : 22 Sep 2025 19:57
Operator : YP\AJ
Sample : Q3135-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 23 04:35:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 082925.M
Quant Title : GC Extractables
QLast Update : Fri Aug 29 08:12:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

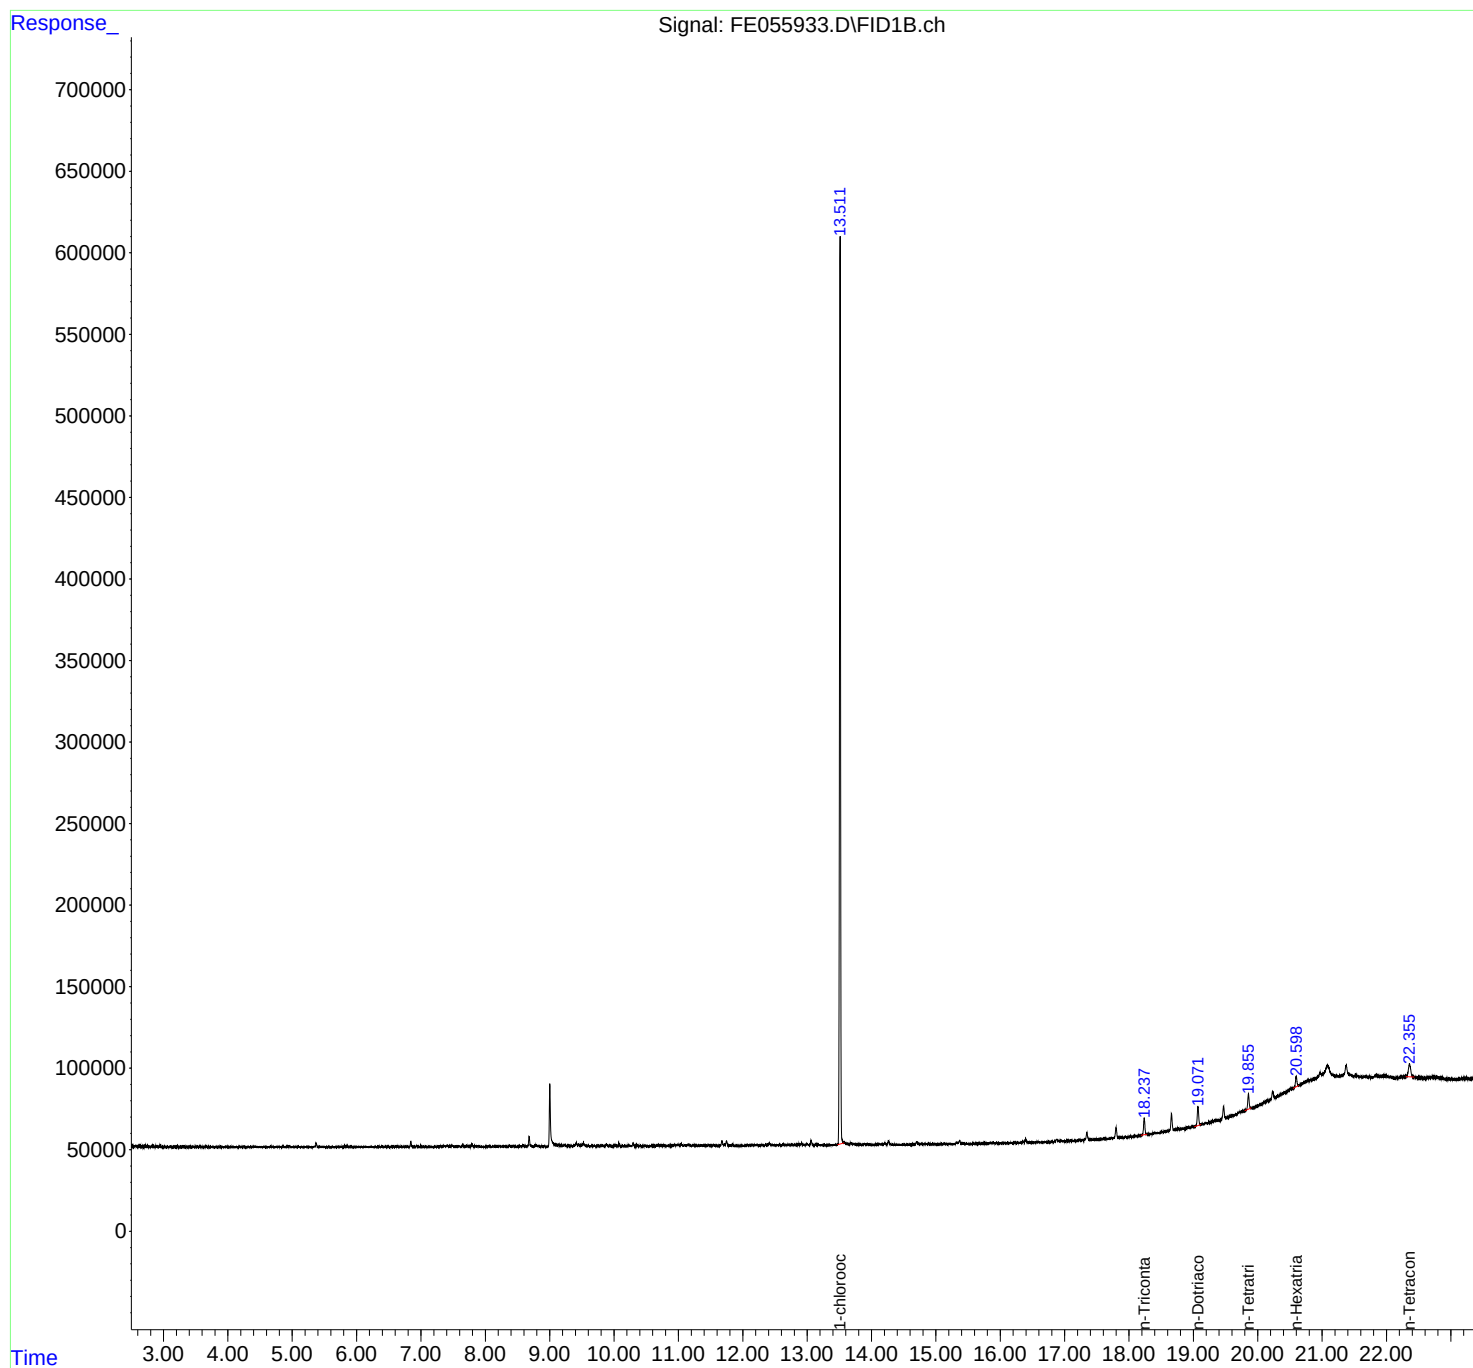


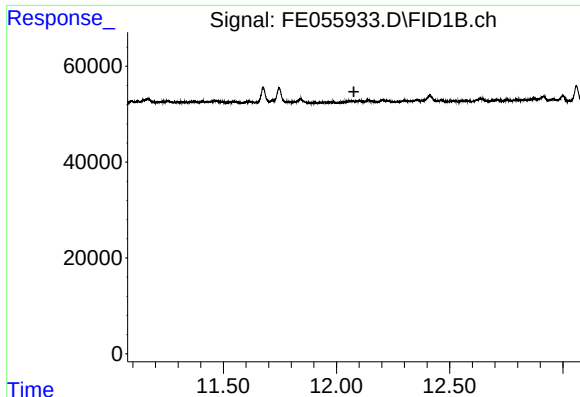

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 12.077 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

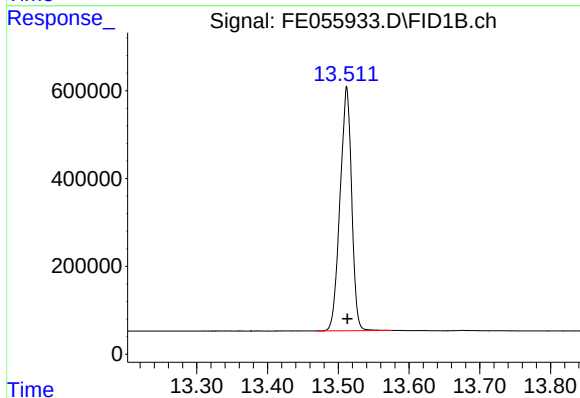


#12 1-chlorooctadecane (SURR)

R.T.: 13.512 min
Delta R.T.: 0.000 min
Response: 631855
Conc: 50.53 ug/ml

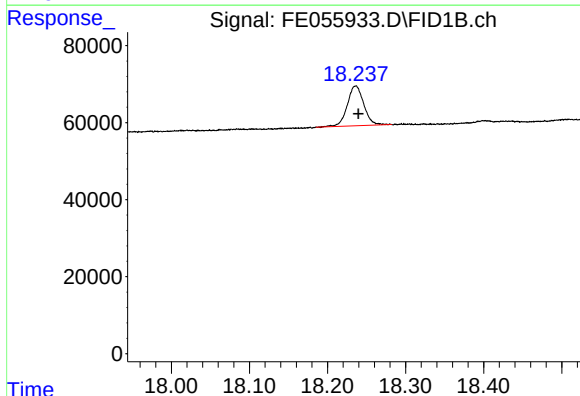


#17 n-Tricontane (C30)

R.T.: 18.236 min
Delta R.T.: -0.004 min
Response: 151087
Conc: 1.02 ug/ml

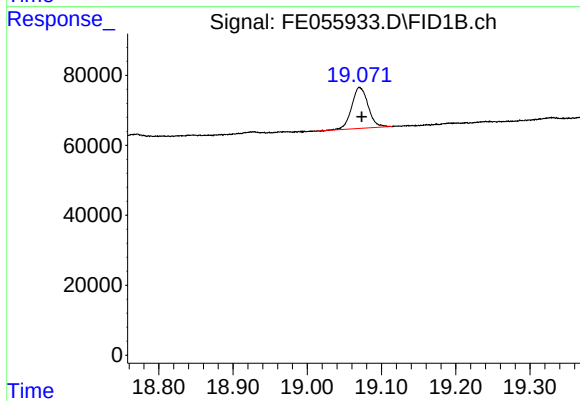

#18 n-Dotriacontane (C32)


R.T.: 19.071 min
Delta R.T.: -0.003 min
Response: 180071
Conc: 1.23 ug/ml

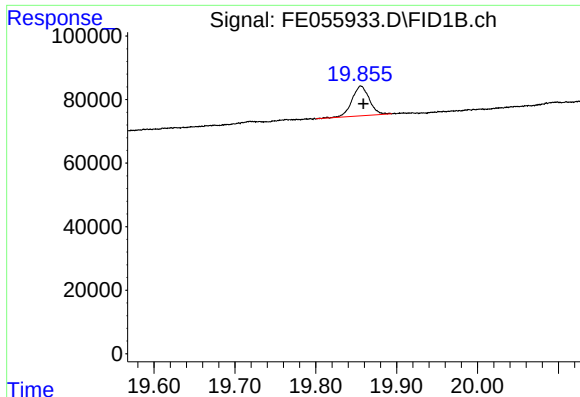

#19 n-Tetratriacontane (C34)


R.T.: 19.856 min
Delta R.T.: -0.003 min
Response: 137814
Conc: 0.98 ug/ml

Instrument :
FID_F
ClientSampleId :

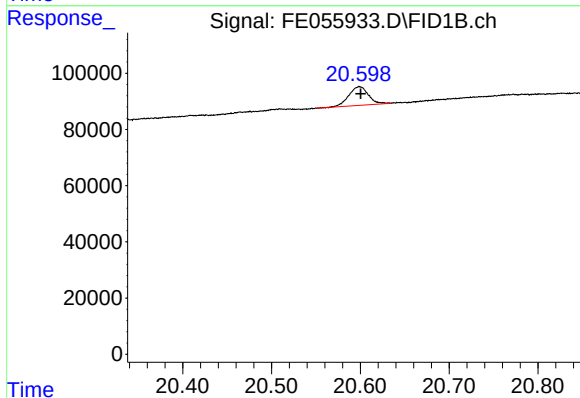

#20 n-Hexatriacontane (C36)

R.T.: 20.599 min
Delta R.T.: -0.002 min
Response: 100950
Conc: 0.77 ug/ml

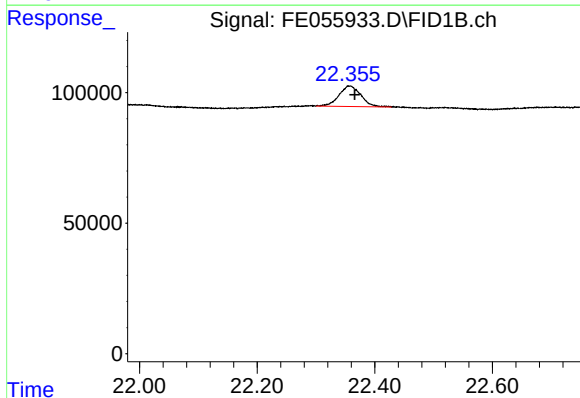

#22 n-Tetracontane (C40)

R.T.: 22.357 min
Delta R.T.: -0.009 min
Response: 202297
Conc: 1.58 ug/ml