

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092320\
Data File : FF007643.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2020 13:40
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 24 00:55:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.474	3774150	23.199 ug/ml
12)	N-OCTACOSANE	16.914	3031172	19.751 ug/ml
13)	N-TRIACONTANE	17.802	205613	1.391 ug/ml
14)	N-DOTRIACONTANE	18.638	243060	1.752 ug/ml
15)	N-TETRATRIACONTANE	19.425	180942	1.434 ug/ml
16)	N-HEXATRIACONTANE	20.170	86900	0.727 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092320\
Data File : FF007643.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2020 13:40
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 24 00:55:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

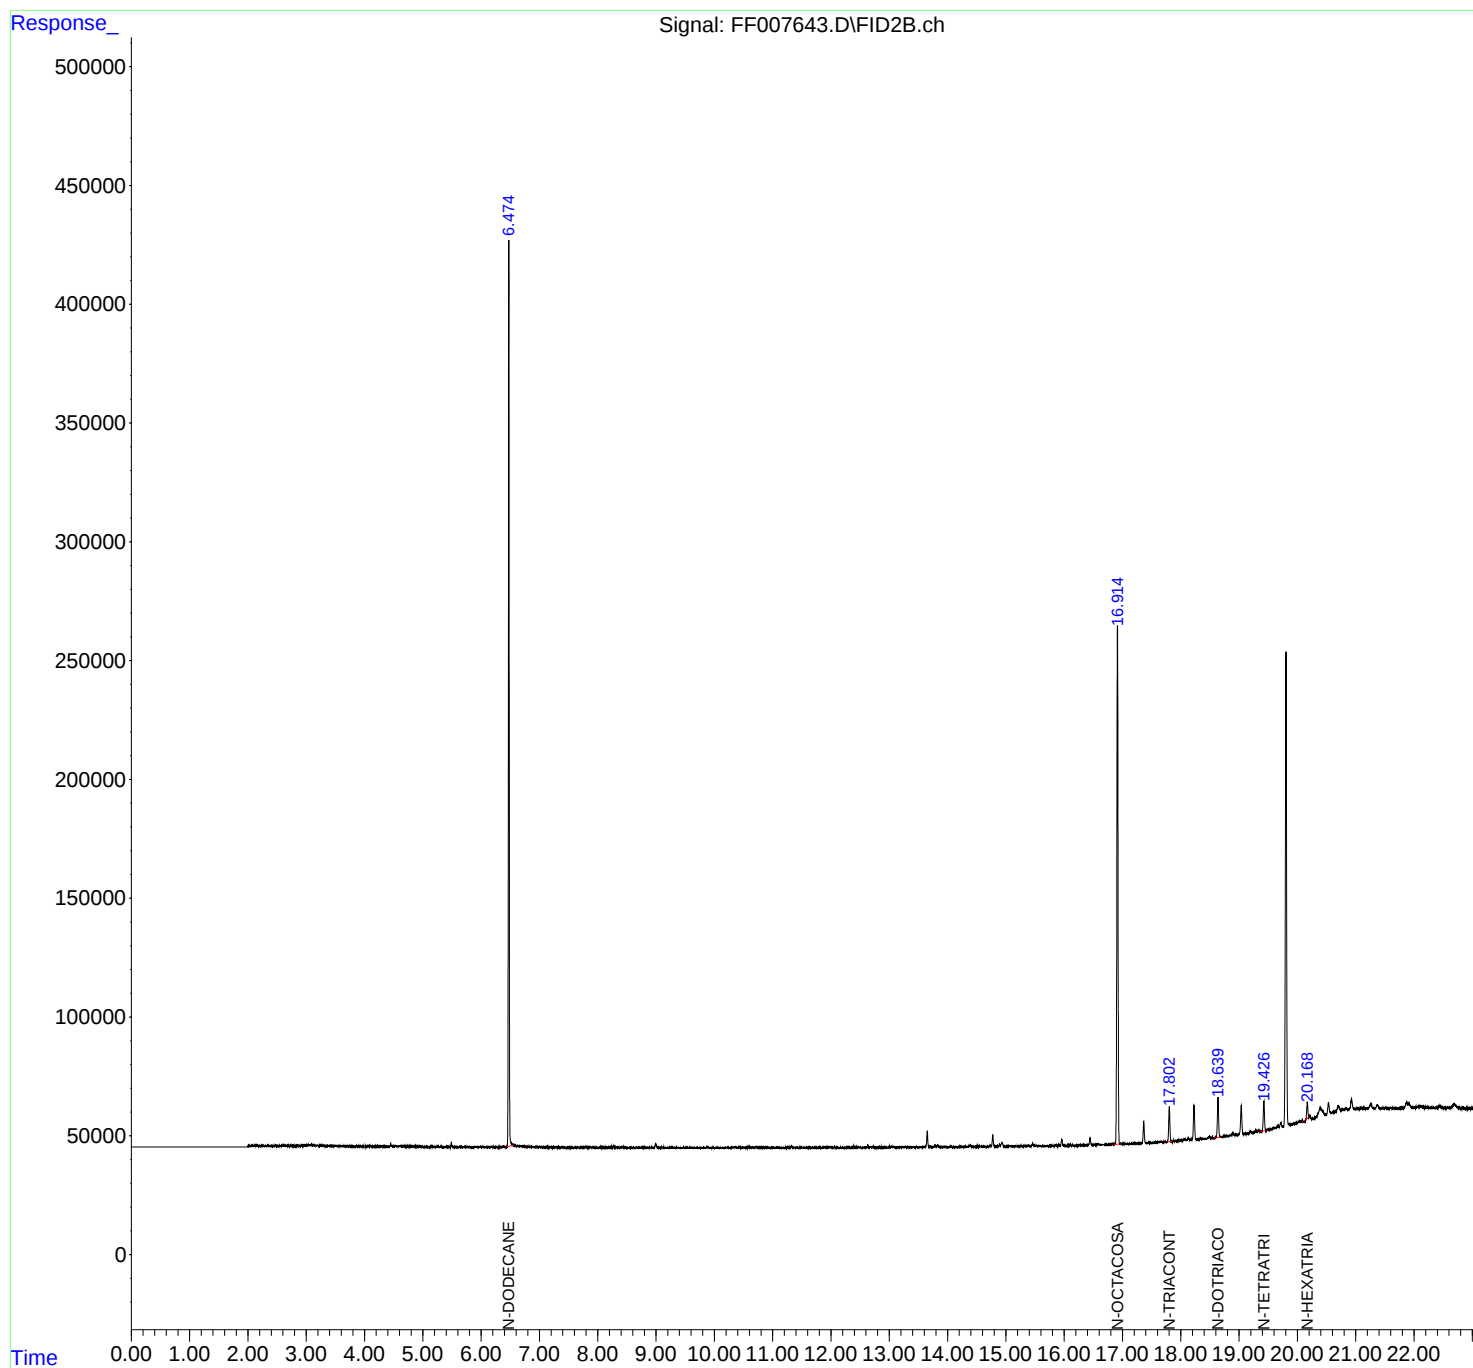


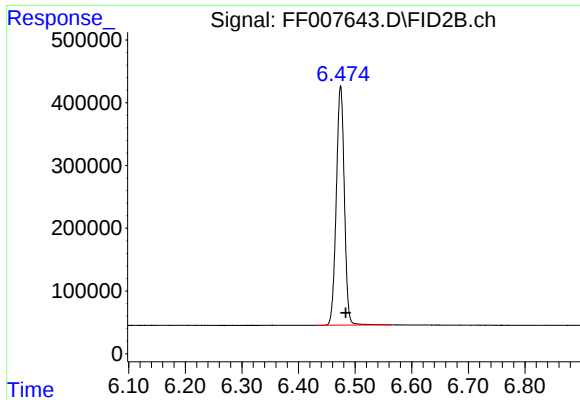

#3 N-DODECANE


R.T.: 6.474 min
Delta R.T.: -0.009 min
Response: 3774150
Conc: 23.20 ug/ml

Instrument :
FID_F
ClientSampleId :

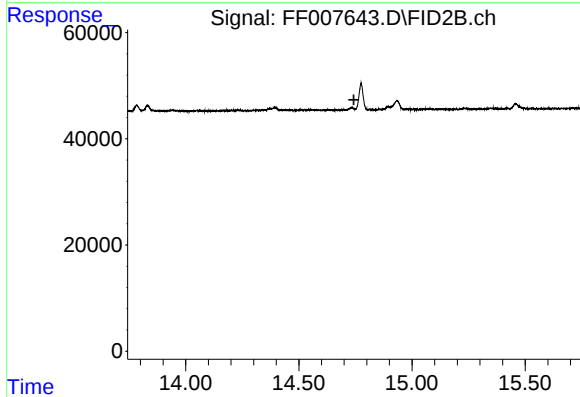


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.743 min
Response: 0
Conc: N.D.

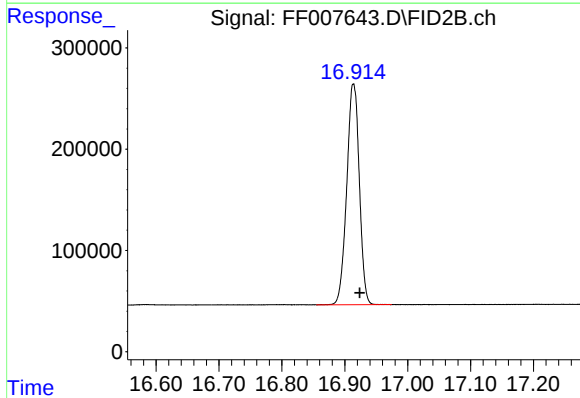


#12 N-OCTACOSANE

R.T.: 16.914 min
Delta R.T.: -0.010 min
Response: 3031172
Conc: 19.75 ug/ml

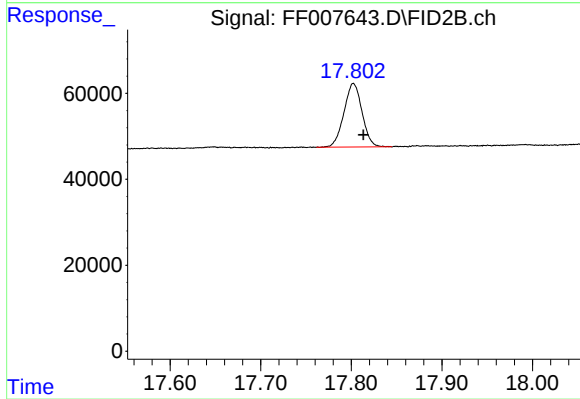

#13 N-TRIACONTANE


R.T.: 17.802 min
Delta R.T.: -0.011 min
Response: 205613
Conc: 1.39 ug/ml

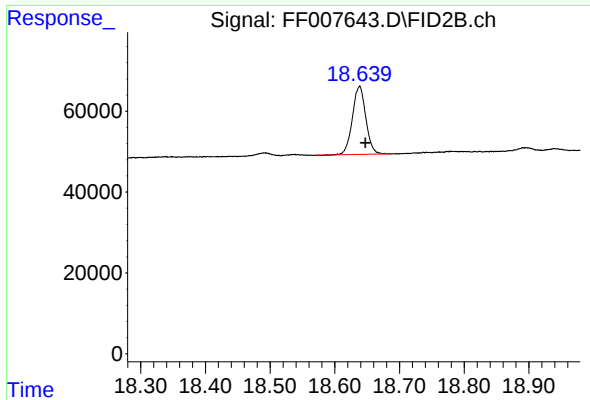

#14 N-DOTRIACONTANE


R.T.: 18.638 min
Delta R.T.: -0.009 min
Response: 243060
Conc: 1.75 ug/ml

Instrument :
FID_F
ClientSampleId :

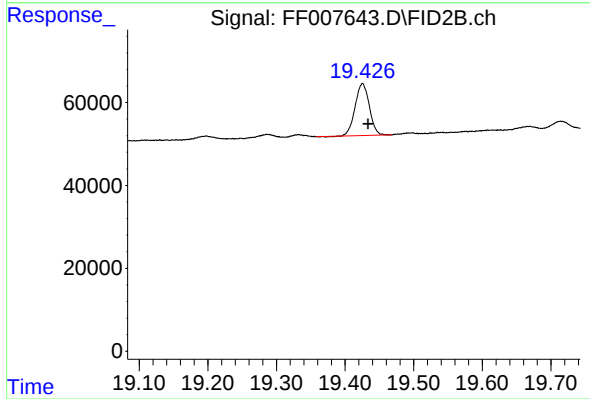

#15 N-TETRATRIACONTANE

R.T.: 19.425 min
Delta R.T.: -0.008 min
Response: 180942
Conc: 1.43 ug/ml

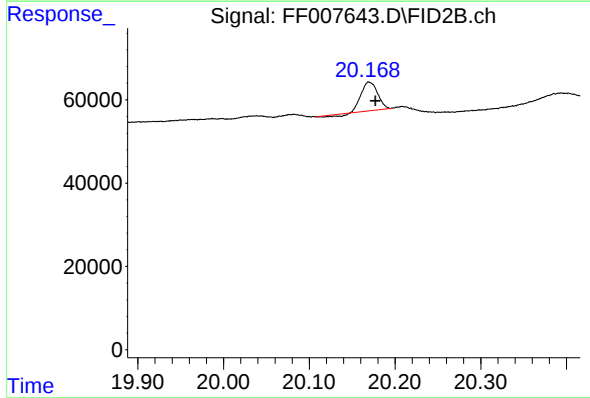

#16 N-HEXATRIACONTANE

R.T.: 20.170 min
Delta R.T.: -0.007 min
Response: 86900
Conc: 0.73 ug/ml