

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF092320\  
 Data File : FF007649.D  
 Signal(s) : FID2B.ch  
 Acq On : 23 Sep 2020 17:17  
 Operator : DD\AJ  
 Sample : L4113-01  
 Misc :  
 ALS Vial : 60 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Sep 24 00:56:42 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF090120.M  
 Quant Title :  
 QLast Update : Wed Sep 02 11:29:30 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

|                             | Compound                 | R.T.    | Response | Conc Units   |
|-----------------------------|--------------------------|---------|----------|--------------|
| -----                       |                          |         |          |              |
| System Monitoring Compounds |                          |         |          |              |
| 9) S                        | TETRACOSANE-d50 (SURR... | 14.733  | 2035610  | 13.841 ug/ml |
| Target Compounds            |                          |         |          |              |
| 4)                          | N-TETRADECANE            | 8.235   | 105239   | 0.640 ug/ml  |
| 7)                          | N-EICOSANE               | 12.697f | 264518   | 1.573 ug/ml  |
| 10)                         | N-TETRACOSANE            | 14.921  | 213110   | 1.307 ug/ml  |
| 14)                         | N-DOTRIACONTANE          | 18.634  | 129615   | 0.934 ug/ml  |
| -----                       |                          |         |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF092320\  
Data File : FF007649.D  
Signal(s) : FID2B.ch  
Acq On : 23 Sep 2020 17:17  
Operator : DD\AJ  
Sample : L4113-01  
Misc :  
ALS Vial : 60 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Sep 24 00:56:42 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF090120.M  
Quant Title :  
QLast Update : Wed Sep 02 11:29:30 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

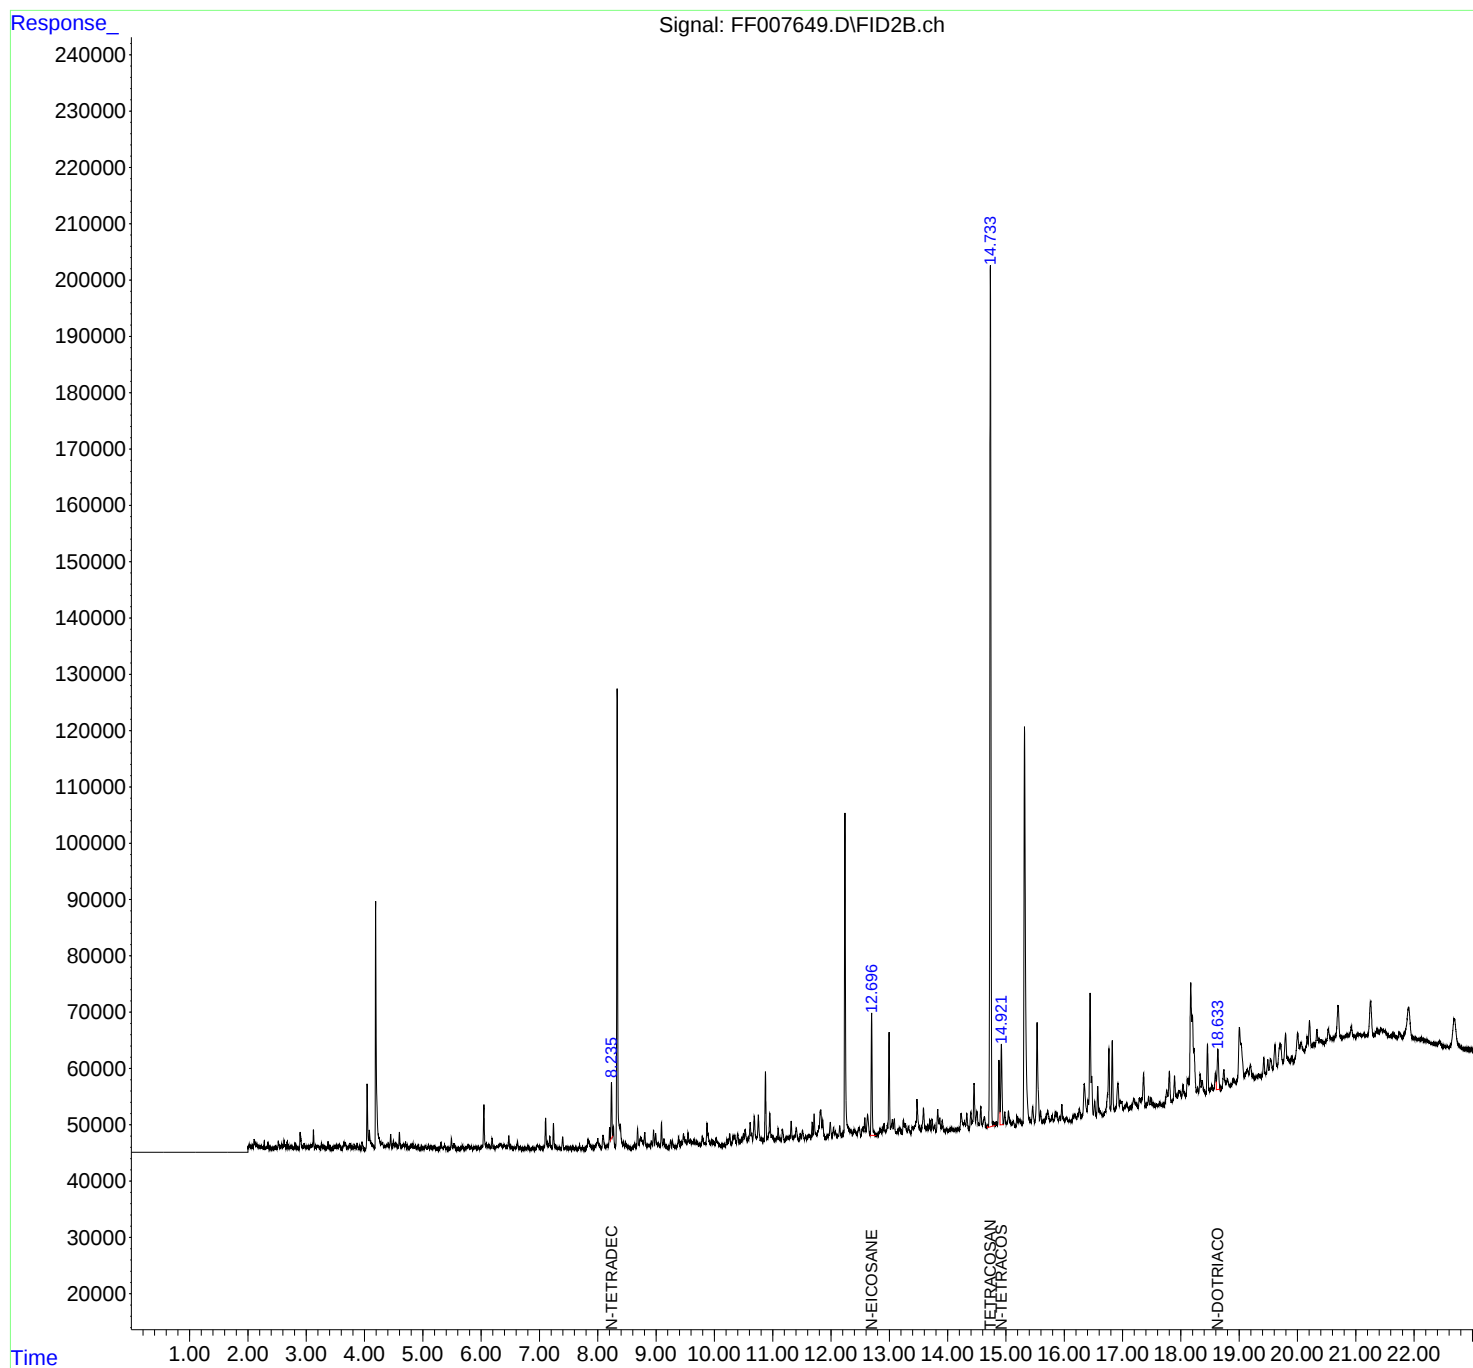


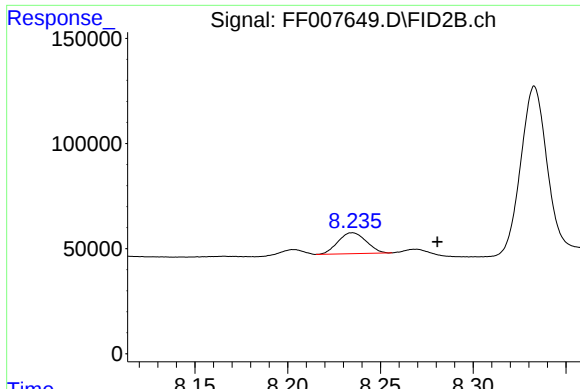

#4 N-TETRADECANE


R.T.: 8.235 min  
Delta R.T.: -0.046 min  
Response: 105239  
Conc: 0.64 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

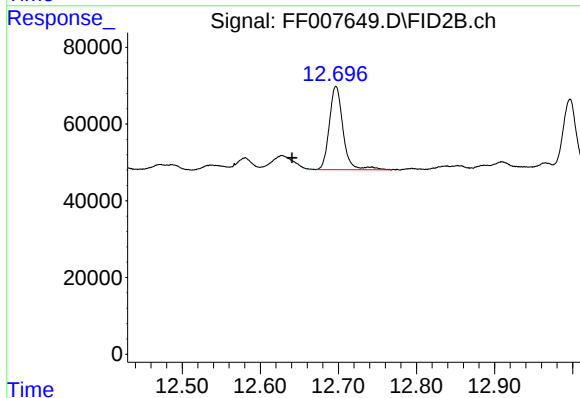


#7 N-EICOSANE

R.T.: 12.697 min  
Delta R.T.: 0.056 min  
Response: 264518  
Conc: 1.57 ug/ml

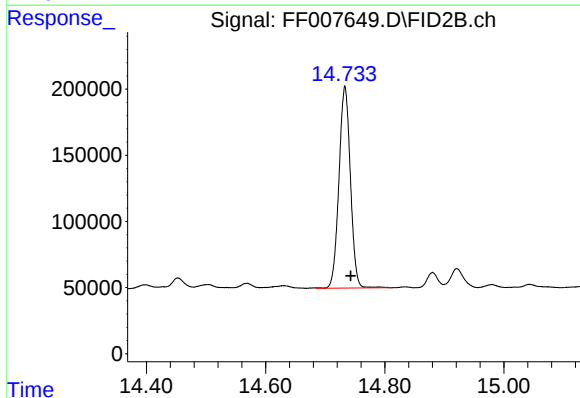


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.733 min  
Delta R.T.: -0.010 min  
Response: 2035610  
Conc: 13.84 ug/ml

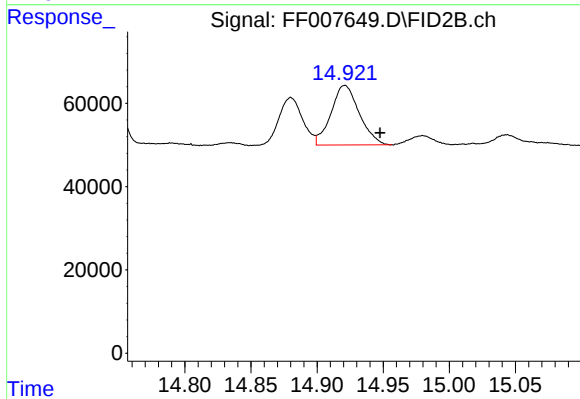

#10 N-TETRACOSANE

R.T.: 14.921 min  
Delta R.T.: -0.027 min  
Response: 213110  
Conc: 1.31 ug/ml

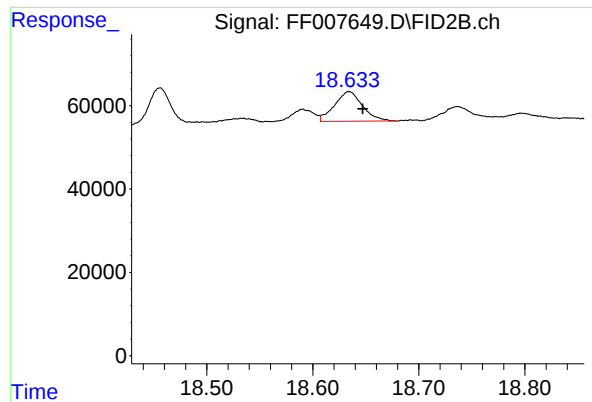

#14 N-DOTRIACONTANE

R.T.: 18.634 min  
Delta R.T.: -0.013 min  
Response: 129615  
Conc: 0.93 ug/ml

Instrument :  
FID\_F  
ClientSampleId :