

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092320\
 Data File : FF007650.D
 Signal(s) : FID2B.ch
 Acq On : 23 Sep 2020 17:48
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 24 00:56:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.734	2233001	15.183 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.802	94076	0.636 ug/ml
14) N-DOTRIACONTANE	18.637	121766	0.878 ug/ml
15) N-TETRATRIACONTANE	19.423	97738	0.774 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092320\
Data File : FF007650.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2020 17:48
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 24 00:56:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

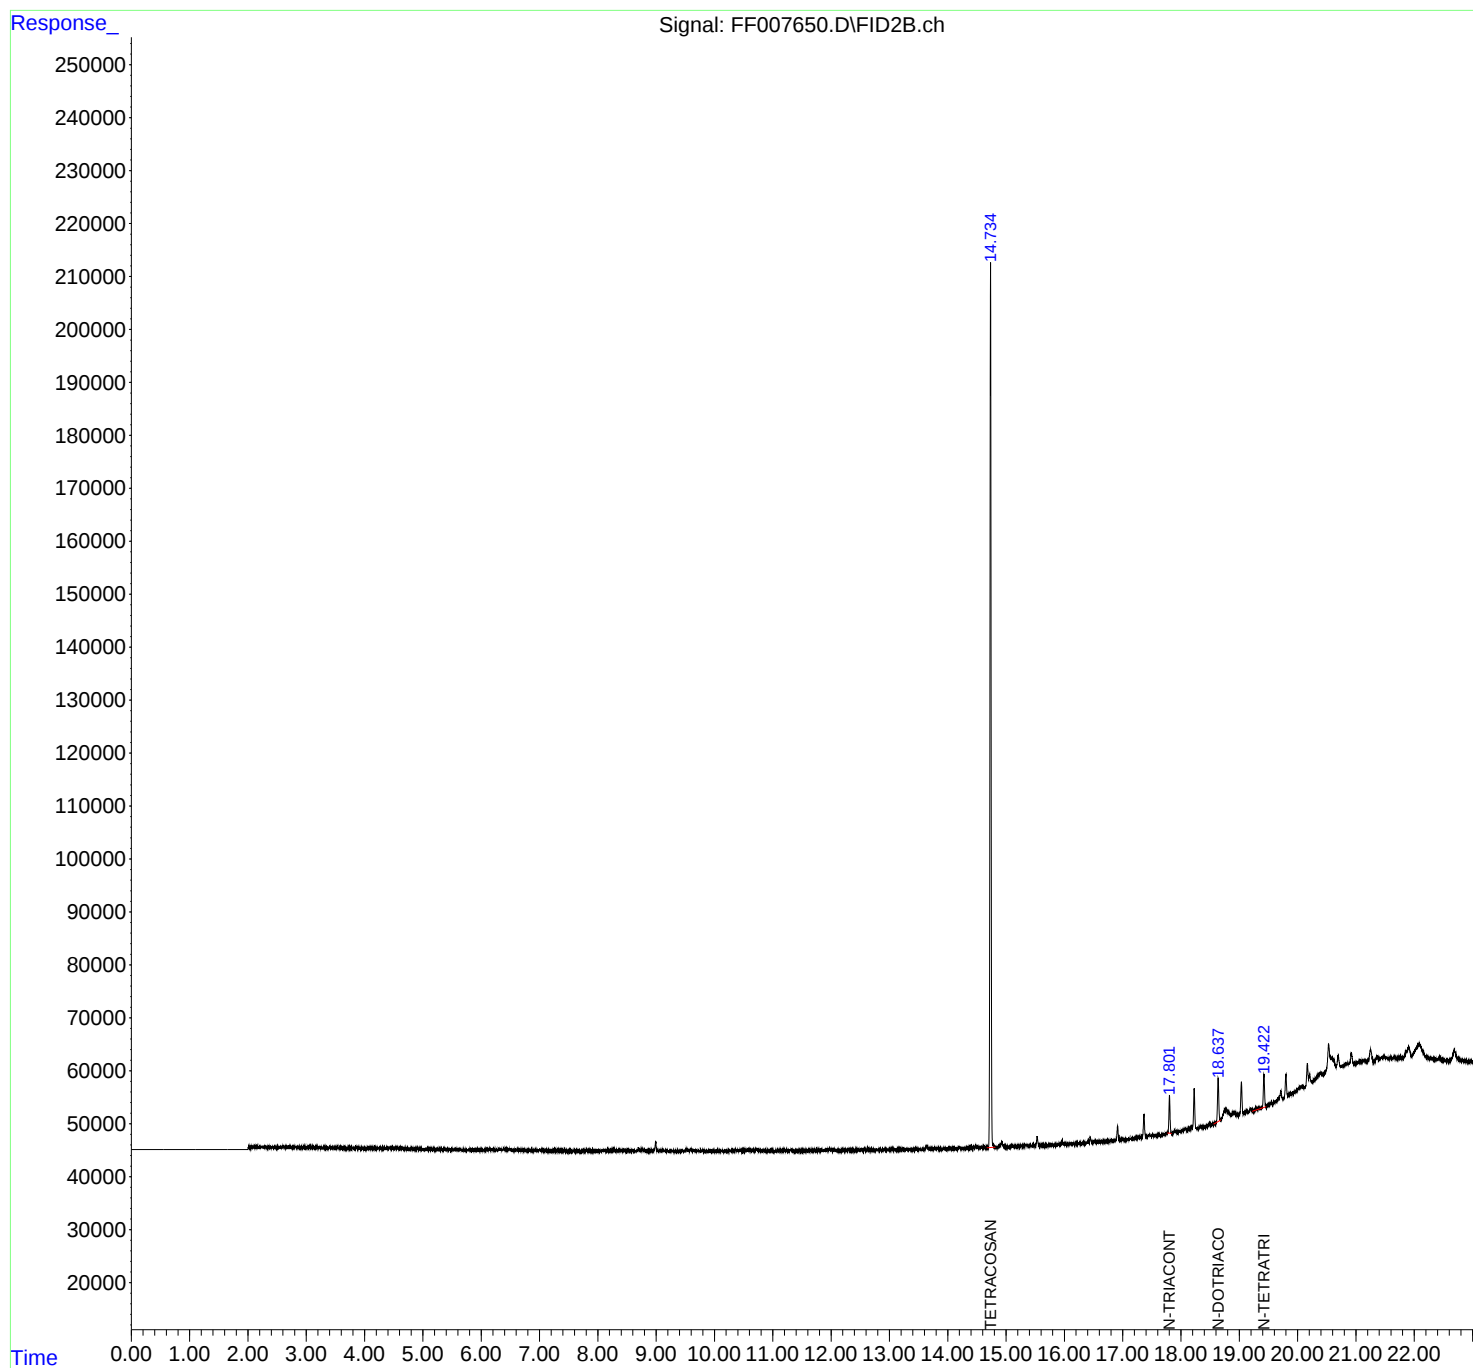


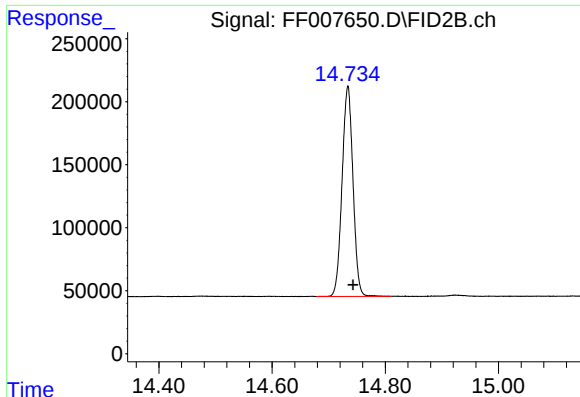

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.734 min
Delta R.T.: -0.009 min
Response: 2233001
Conc: 15.18 ug/ml

Instrument :
FID_F
ClientSampleId :

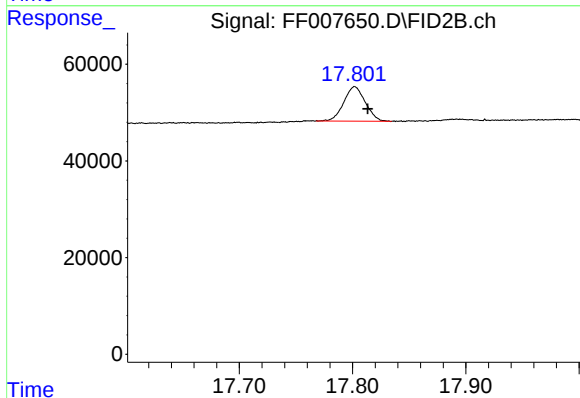


#13 N-TRIACONTANE

R.T.: 17.802 min
Delta R.T.: -0.011 min
Response: 94076
Conc: 0.64 ug/ml

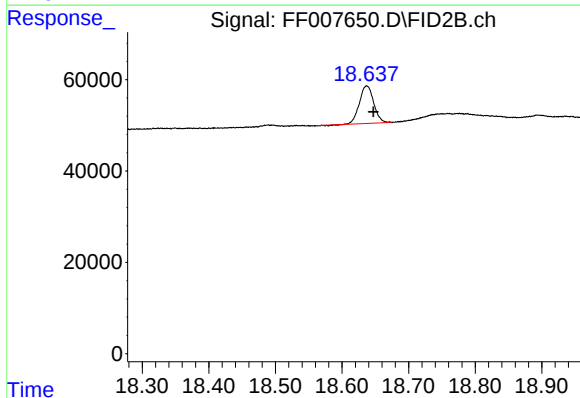

#14 N-DOTRIACONTANE

R.T.: 18.637 min
Delta R.T.: -0.010 min
Response: 121766
Conc: 0.88 ug/ml

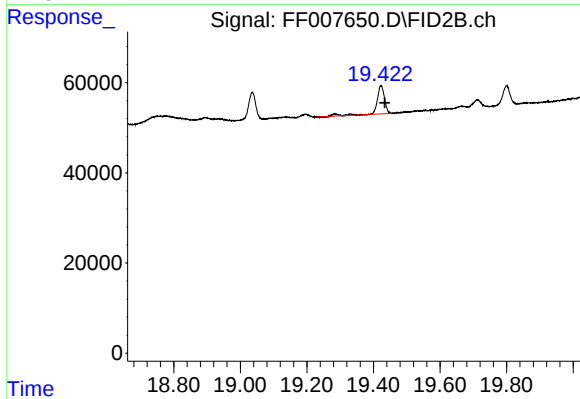

#15 N-TETRATRIACONTANE

R.T.: 19.423 min
Delta R.T.: -0.011 min
Response: 97738
Conc: 0.77 ug/ml