

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092320\
Data File : FF007646.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2020 15:44
Operator : DD\AJ
Sample : L4112-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KTS-SB-0102-0-92

Integration File: autoint1.e
Quant Time: Sep 24 00:55:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.733	1741210	11.839 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092320\
Data File : FF007646.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2020 15:44
Operator : DD\AJ
Sample : L4112-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KTS-SB-0102-0-92

Integration File: autoint1.e
Quant Time: Sep 24 00:55:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

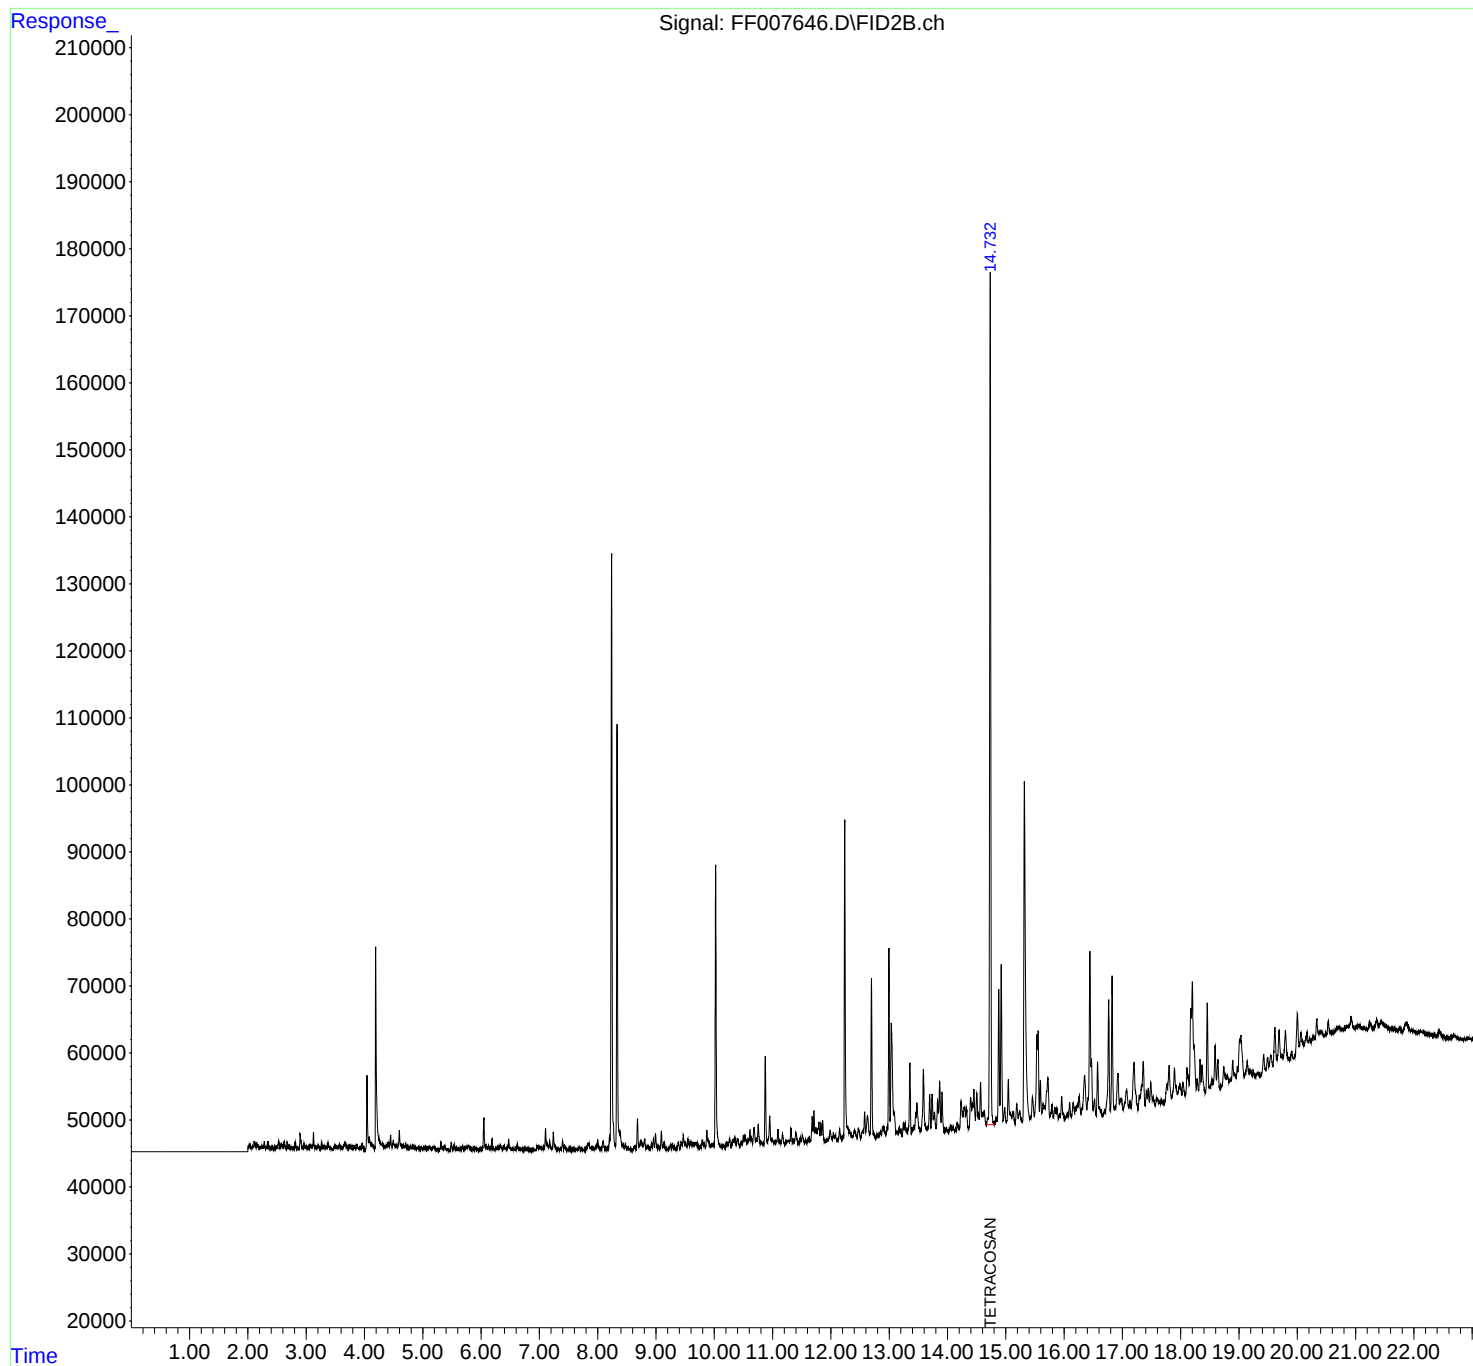

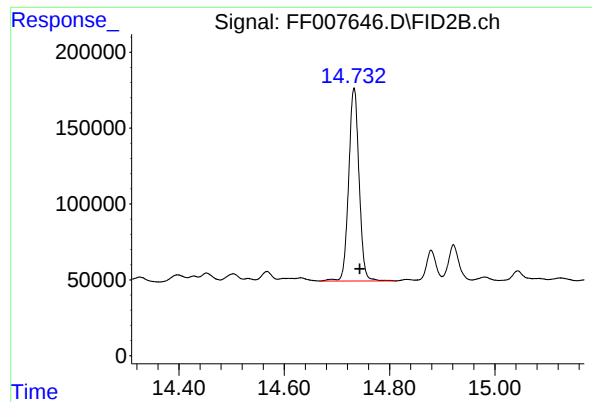

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.733 min
Delta R.T.: -0.011 min
Response: 1741210
Conc: 11.84 ug/ml

Instrument :
FID_F
ClientSampleId :
KTS-SB-0102-0-92