

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092321\
 Data File : FF008992.D
 Signal(s) : FID2B.ch
 Acq On : 23 Sep 2021 11:33
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 24 01:48:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
 Quant Title :
 QLast Update : Wed Sep 08 10:20:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.489	4722611	33.444 ug/ml
12)	N-OCTACOSANE	16.886	4084849	33.388 ug/ml
13)	N-TRIACONTANE	17.766	184598	1.579 ug/ml
14)	N-DOTRIACONTANE	18.597	235093	2.179 ug/ml
15)	N-TETRATRIACONTANE	19.377	176386	1.801 ug/ml
16)	N-HEXATRIACONTANE	20.116	103243	1.181 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092321\
Data File : FF008992.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2021 11:33
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 24 01:48:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

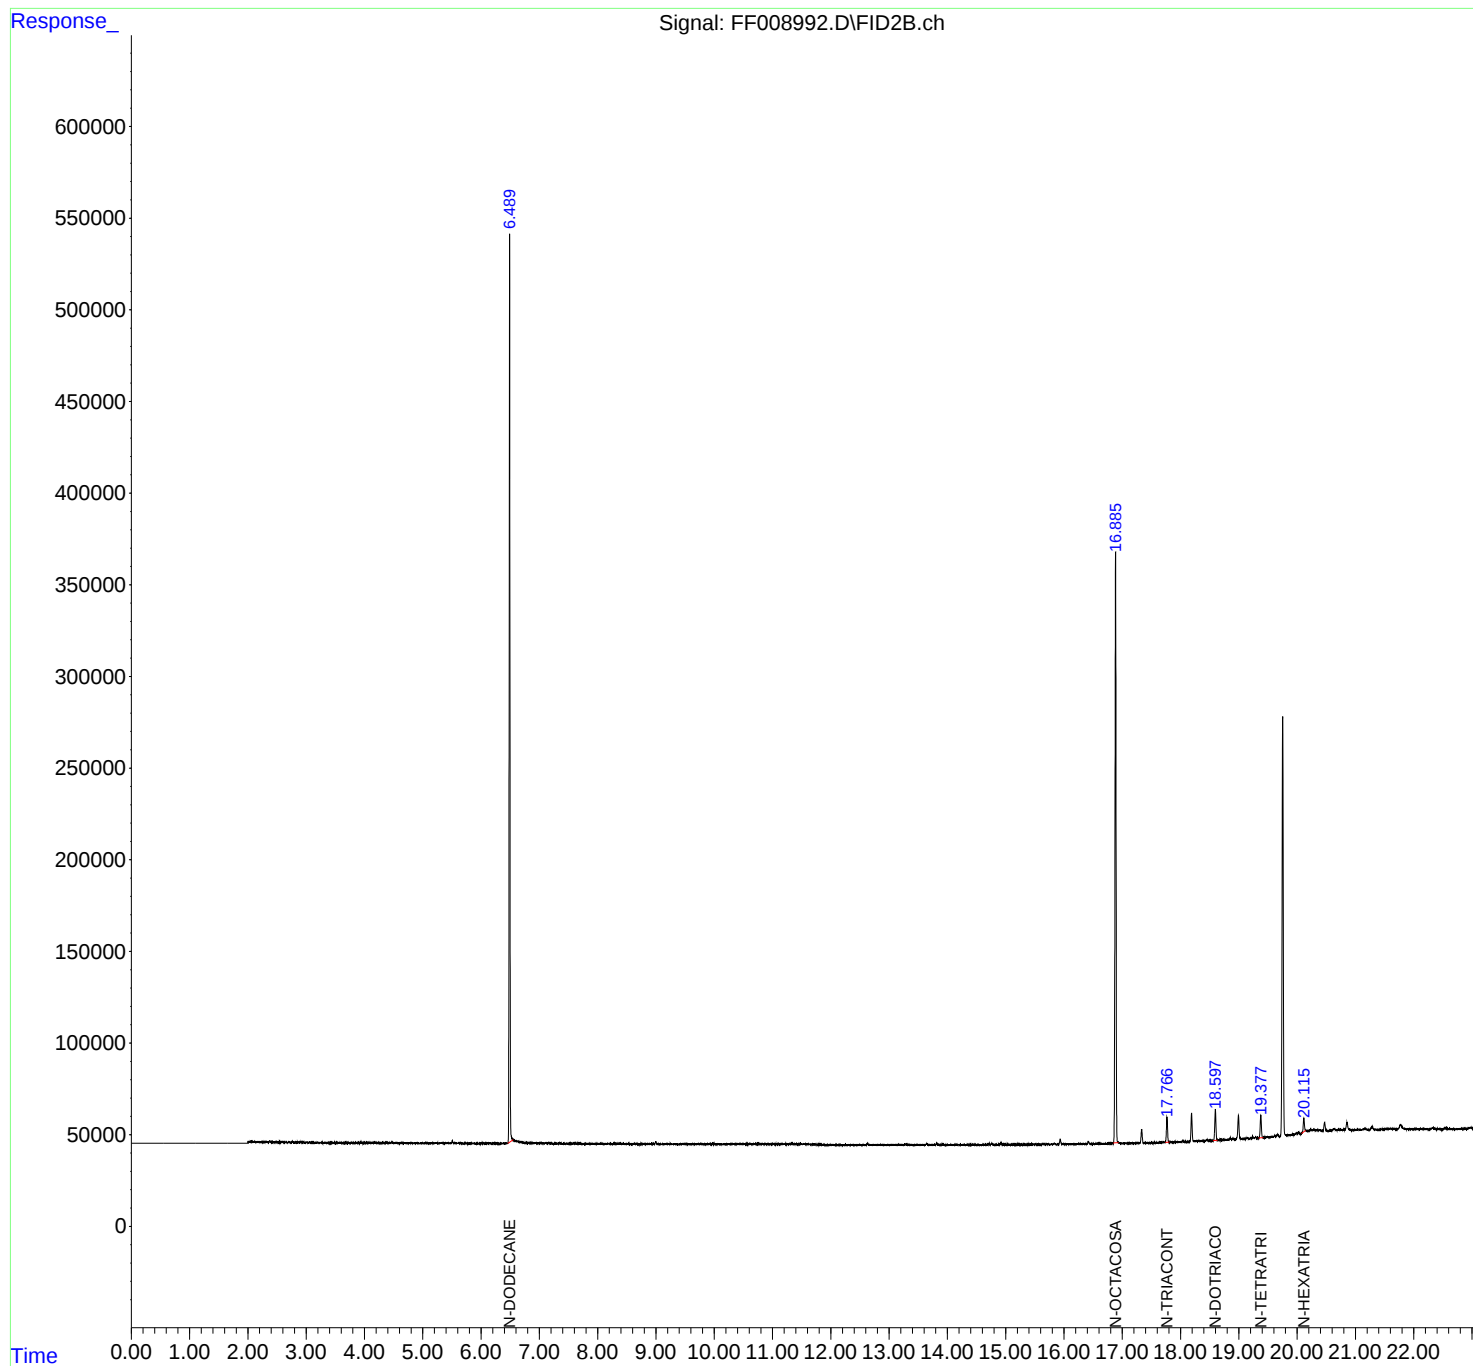


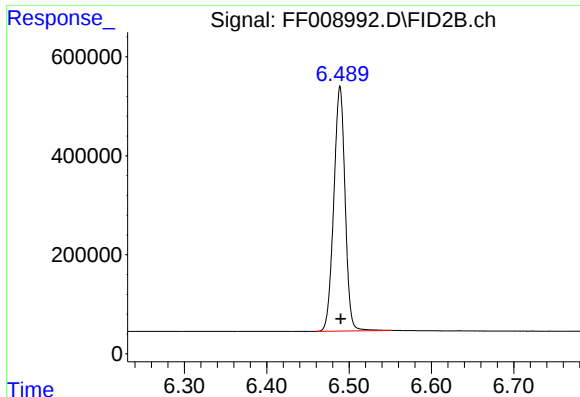

#3 N-DODECANE


R.T.: 6.489 min
Delta R.T.: 0.000 min
Response: 4722611
Conc: 33.44 ug/ml

Instrument :
FID_F
ClientSampleId :

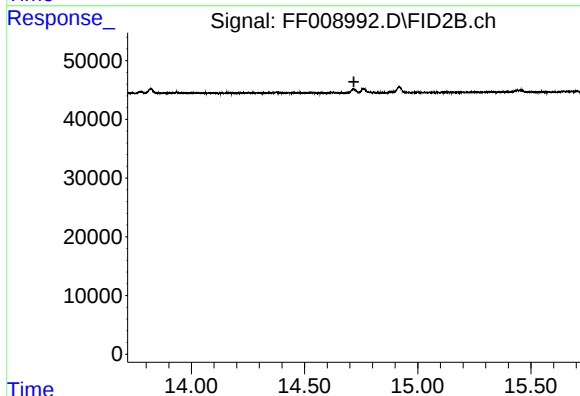


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.718 min
Response: 0
Conc: N.D.

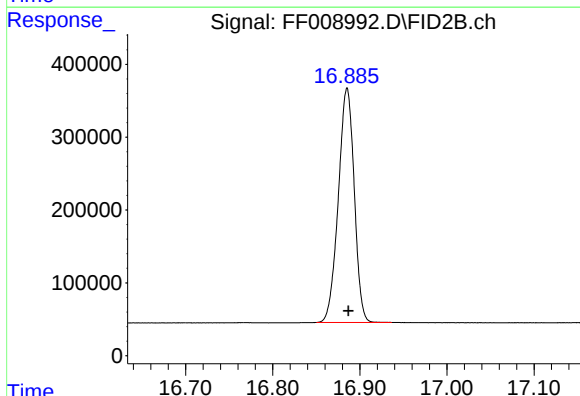


#12 N-OCTACOSANE

R.T.: 16.886 min
Delta R.T.: -0.001 min
Response: 4084849
Conc: 33.39 ug/ml

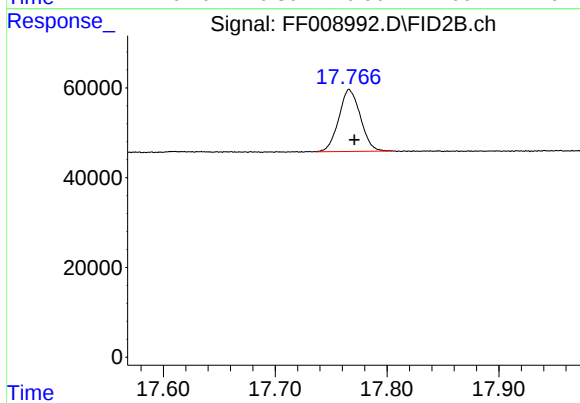

#13 N-TRIACONTANE


R.T.: 17.766 min
Delta R.T.: -0.005 min
Response: 184598
Conc: 1.58 ug/ml

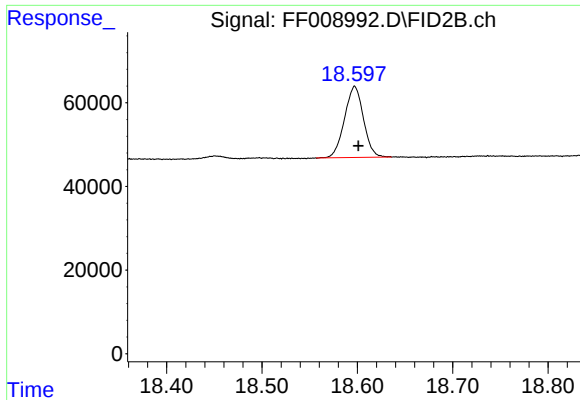

#14 N-DOTRIACONTANE


R.T.: 18.597 min
Delta R.T.: -0.004 min
Response: 235093
Conc: 2.18 ug/ml

Instrument :
FID_F
ClientSampleId :

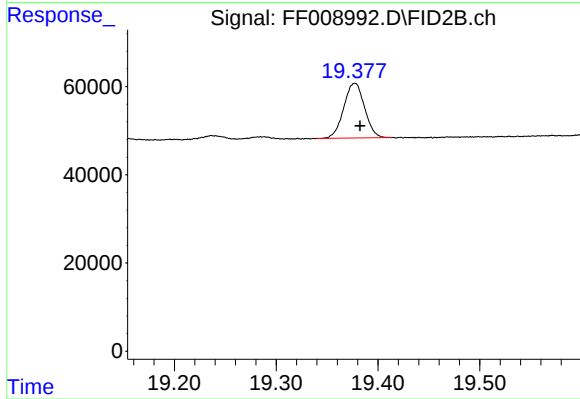

#15 N-TETRATRIACONTANE

R.T.: 19.377 min
Delta R.T.: -0.005 min
Response: 176386
Conc: 1.80 ug/ml

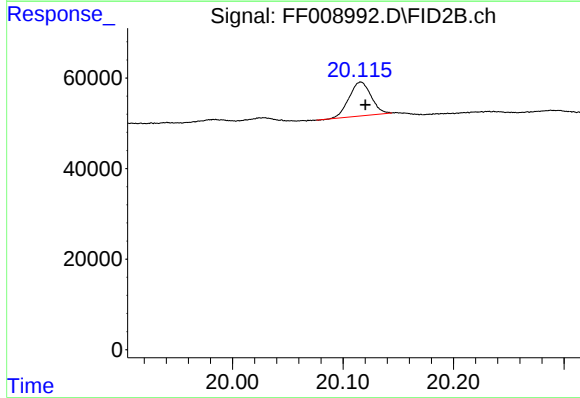

#16 N-HEXATRIACONTANE

R.T.: 20.116 min
Delta R.T.: -0.004 min
Response: 103243
Conc: 1.18 ug/ml