

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092321\
 Data File : FF008997.D
 Signal(s) : FID2B.ch
 Acq On : 23 Sep 2021 15:45
 Operator : DD\AJ
 Sample : M3861-08
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 24 01:49:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
 Quant Title :
 QLast Update : Wed Sep 08 10:20:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.719	2569965	21.877 ug/ml
Target Compounds			
6) N-OCTADECANE	11.334	134264	0.942 ug/ml
7) N-EICOSANE	12.620	166207	1.182 ug/ml
8) N-DOCOSANE	13.821	127300	0.937 ug/ml
10) N-TETRACOSANE	14.917	1991904	14.987 ug/ml
11) N-HEXACOSANE	15.937	85159	0.667 ug/ml
12) N-OCTACOSANE	16.883	195237	1.596 ug/ml
13) N-TRIACONTANE	17.771	241888	2.070 ug/ml
14) N-DOTRIACONTANE	18.594	206238	1.911 ug/ml
15) N-TETRATRIACONTANE	19.384	187602	1.915 ug/ml
16) N-HEXATRIACONTANE	20.113	180967	2.070 ug/ml
18) N-TETRACONTANE	21.768	247560	3.183 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092321\
Data File : FF008997.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2021 15:45
Operator : DD\AJ
Sample : M3861-08
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 24 01:49:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

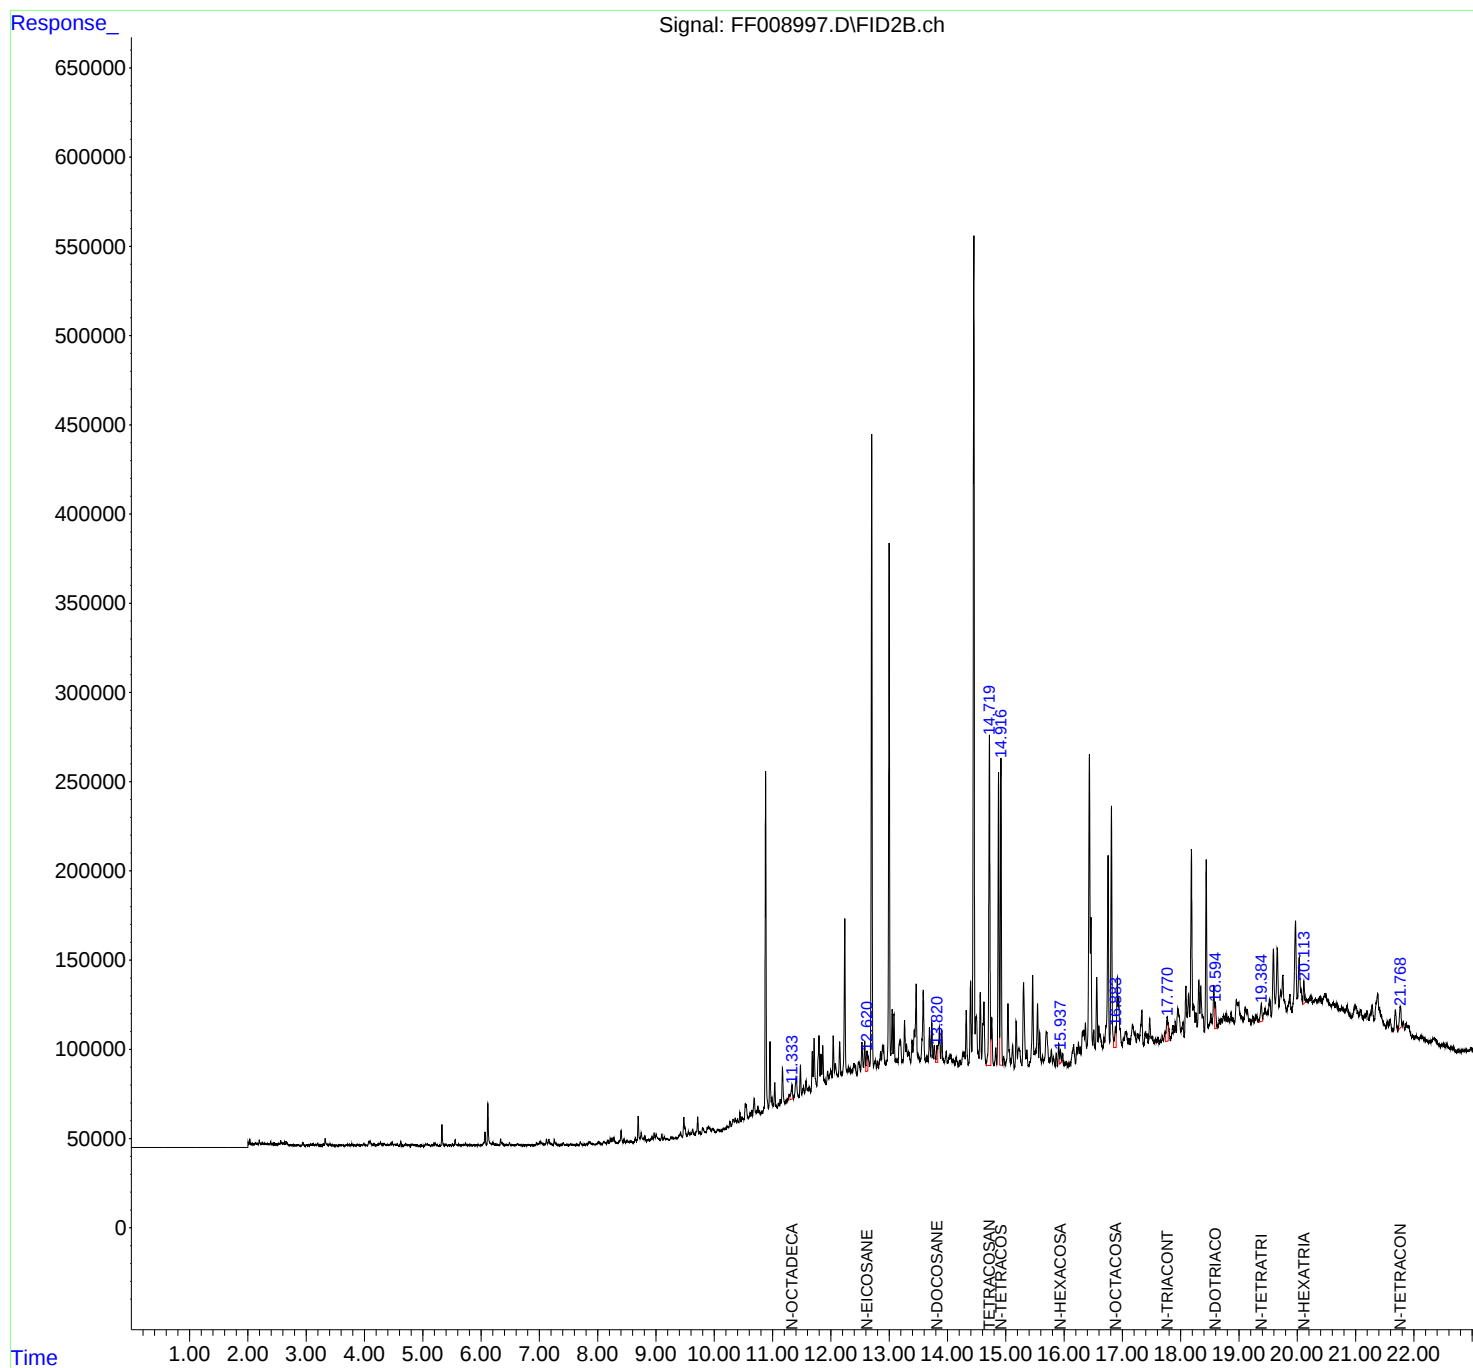


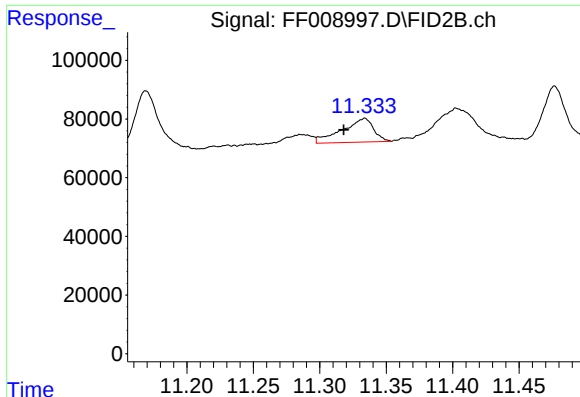

#6 N-OCTADECANE


R.T.: 11.334 min
Delta R.T.: 0.016 min
Response: 134264
Conc: 0.94 ug/ml

Instrument :
FID_F
ClientSampleId :

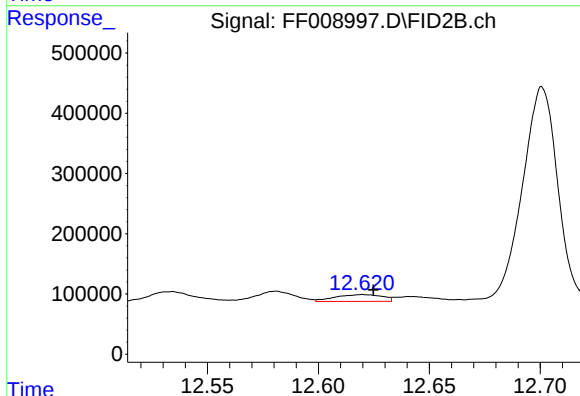


#7 N-EICOSANE

R.T.: 12.620 min
Delta R.T.: -0.005 min
Response: 166207
Conc: 1.18 ug/ml

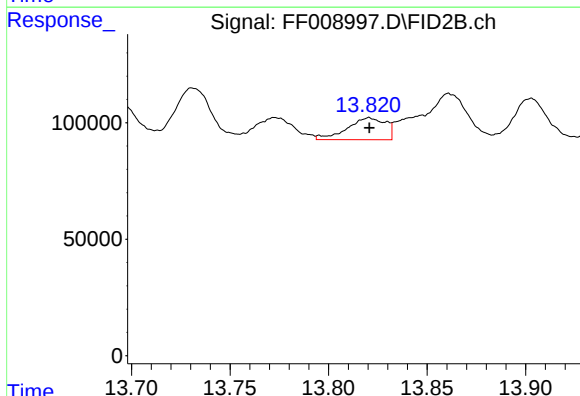


#8 N-DOCOSANE

R.T.: 13.821 min
Delta R.T.: 0.000 min
Response: 127300
Conc: 0.94 ug/ml

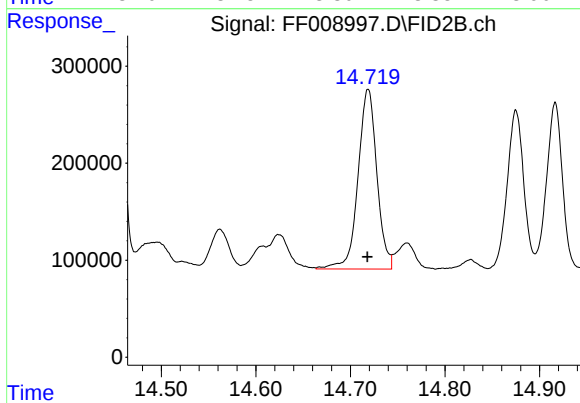

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.719 min
Delta R.T.: 0.000 min
Response: 2569965
Conc: 21.88 ug/ml

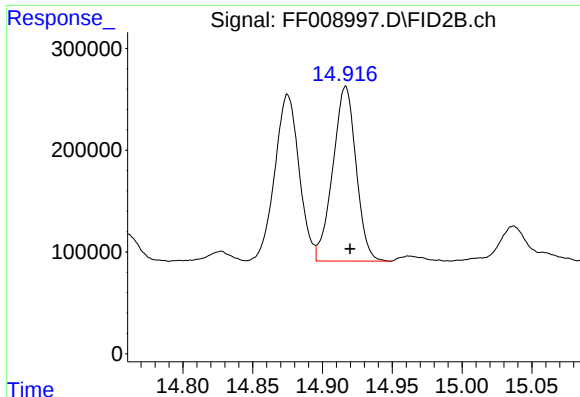

#10 N-TETRACOSANE


R.T.: 14.917 min
Delta R.T.: -0.003 min
Response: 1991904
Conc: 14.99 ug/ml

Instrument :
FID_F
ClientSampleId :

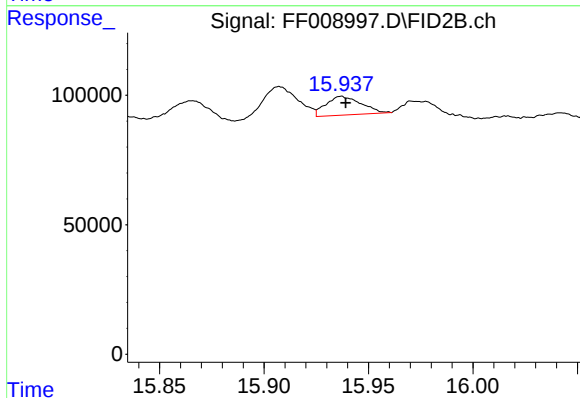


#11 N-HEXACOSANE

R.T.: 15.937 min
Delta R.T.: -0.002 min
Response: 85159
Conc: 0.67 ug/ml

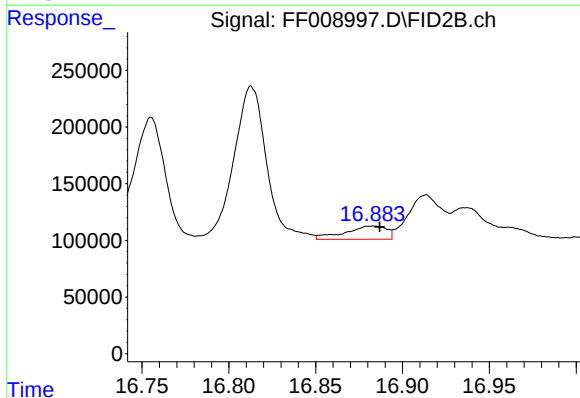


#12 N-OCTACOSANE

R.T.: 16.883 min
Delta R.T.: -0.004 min
Response: 195237
Conc: 1.60 ug/ml

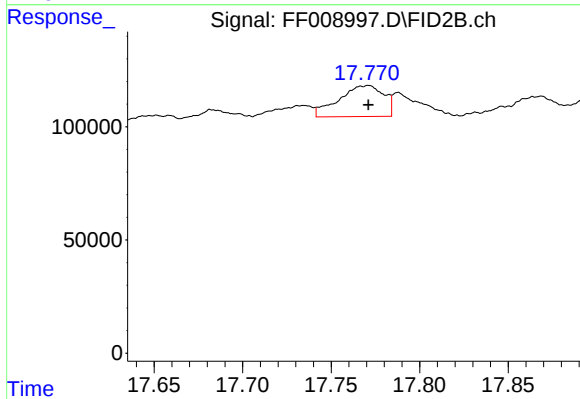

#13 N-TRIACONTANE


R.T.: 17.771 min
Delta R.T.: 0.000 min
Response: 241888
Conc: 2.07 ug/ml

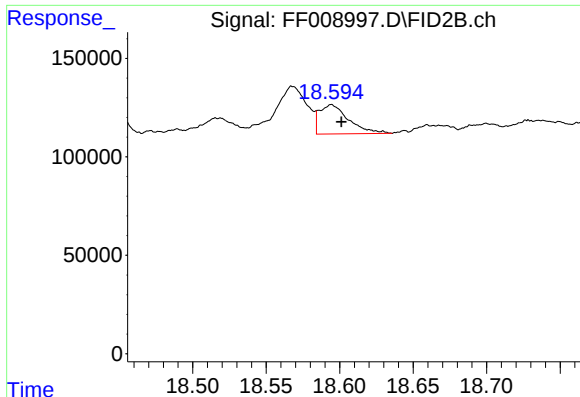

#14 N-DOTRIACONTANE


R.T.: 18.594 min
Delta R.T.: -0.007 min
Response: 206238
Conc: 1.91 ug/ml

Instrument :
FID_F
ClientSampleId :

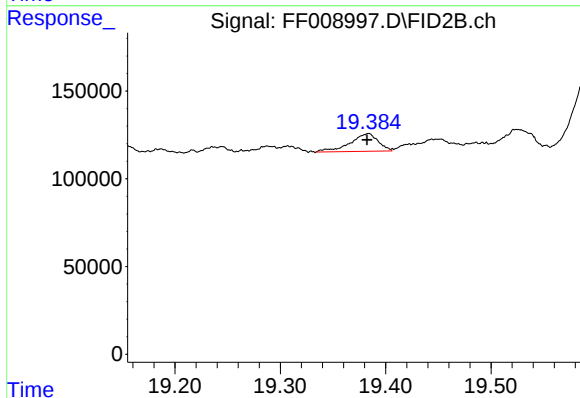


#15 N-TETRATRIACONTANE

R.T.: 19.384 min
Delta R.T.: 0.001 min
Response: 187602
Conc: 1.92 ug/ml

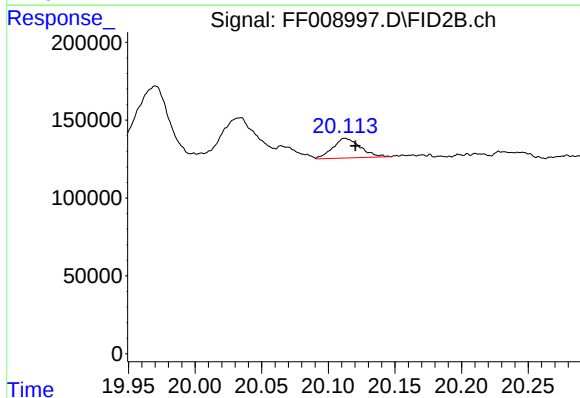

#16 N-HEXATRIACONTANE

R.T.: 20.113 min
Delta R.T.: -0.008 min
Response: 180967
Conc: 2.07 ug/ml

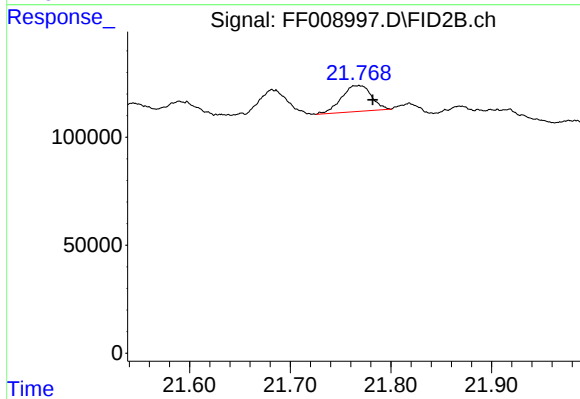

#18 N-TETRACONTANE

R.T.: 21.768 min
Delta R.T.: -0.014 min
Response: 247560
Conc: 3.18 ug/ml