

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092321\
Data File : FF008998.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2021 16:17
Operator : DD\AJ
Sample : M3861-09
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 24 01:49:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.717	1582047	13.467 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.916	187400	1.410 ug/ml
14) N-DOTRIACONTANE	18.596	159226	1.476 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092321\
Data File : FF008998.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2021 16:17
Operator : DD\AJ
Sample : M3861-09
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 24 01:49:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

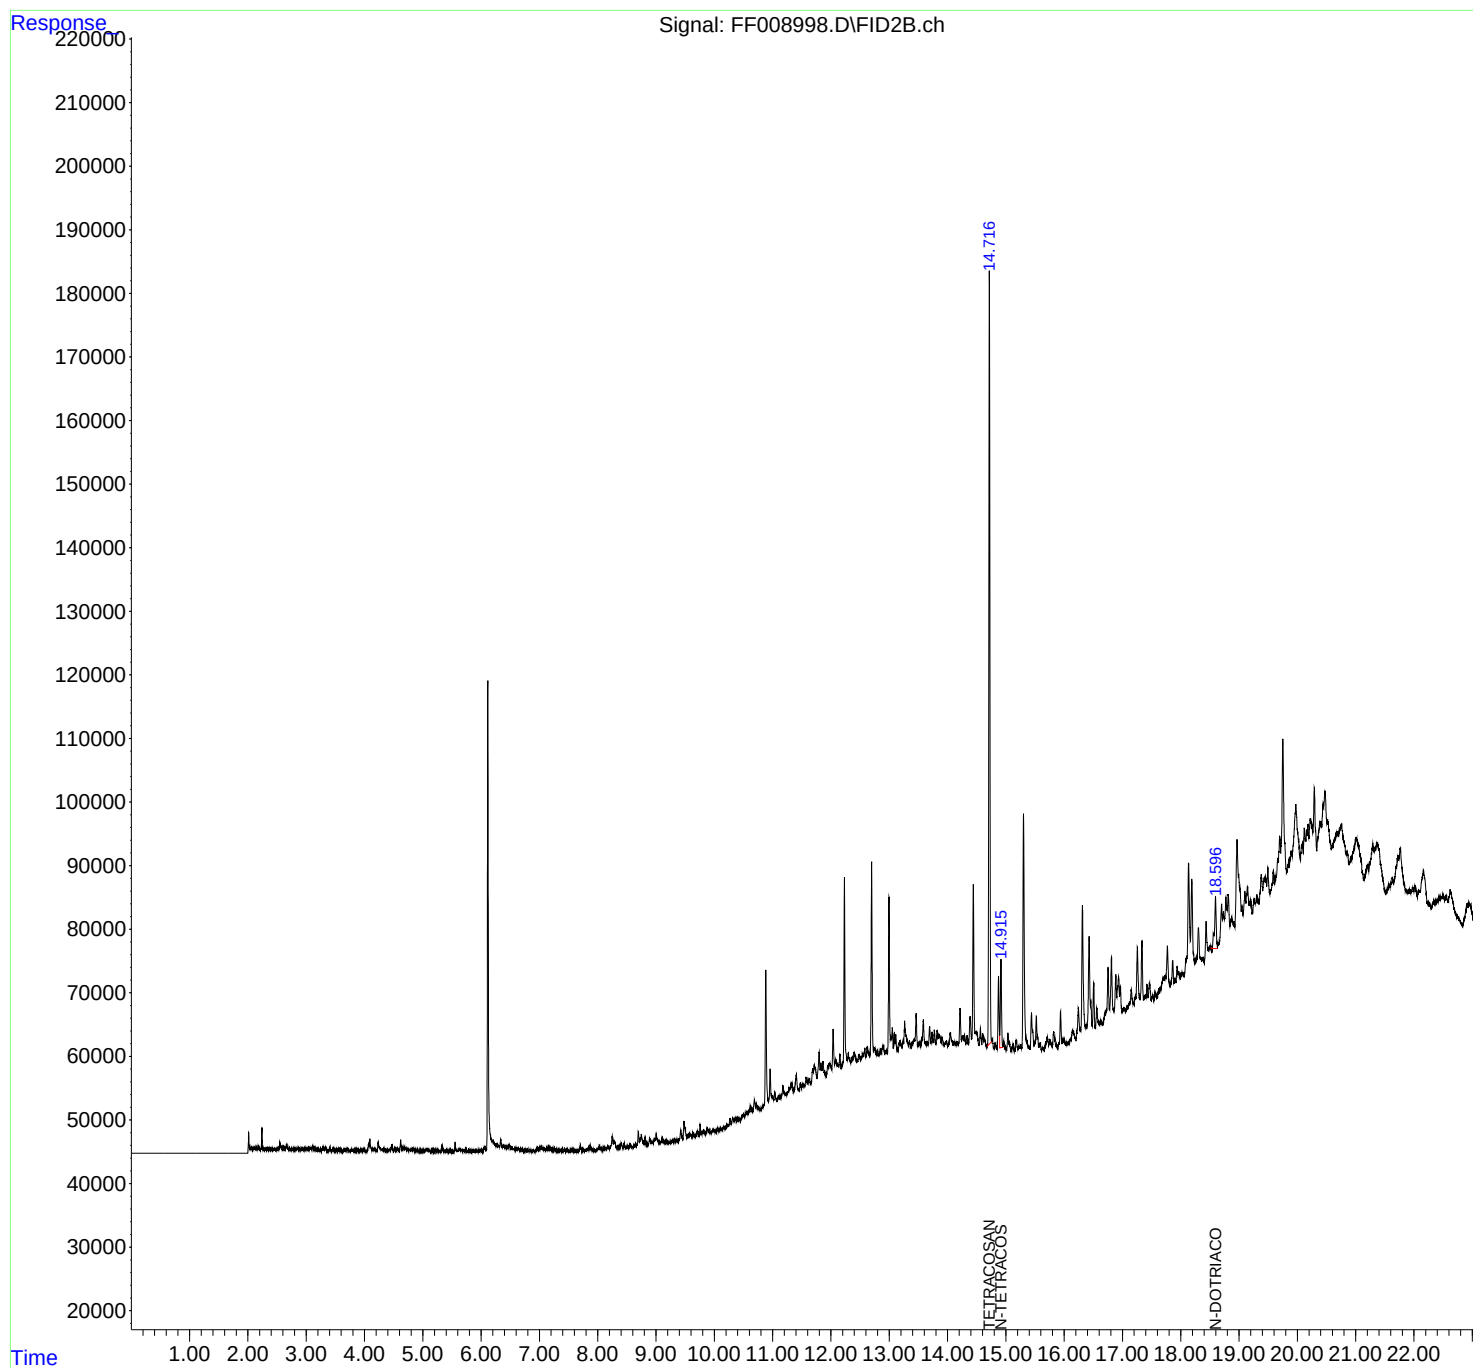


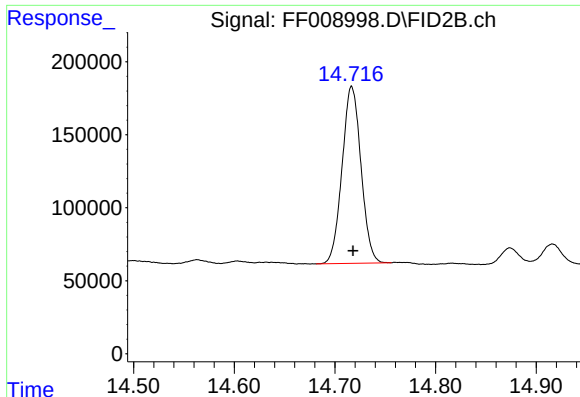

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.717 min
Delta R.T.: -0.001 min
Response: 1582047
Conc: 13.47 ug/ml

Instrument :
FID_F
ClientSampleId :

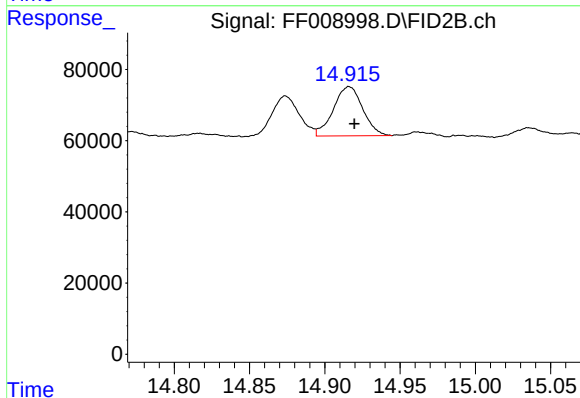

#10 N-TETRACOSANE

R.T.: 14.916 min
Delta R.T.: -0.004 min
Response: 187400
Conc: 1.41 ug/ml

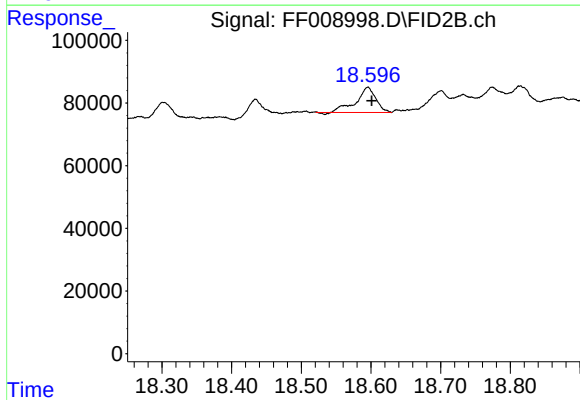

#14 N-DOTRIACONTANE

R.T.: 18.596 min
Delta R.T.: -0.005 min
Response: 159226
Conc: 1.48 ug/ml