

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092321\
Data File : FF009005.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2021 20:30
Operator : DD\AJ
Sample : M3861-08 5X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 24 01:50:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.715	235812	2.007 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.912	193933	1.459 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092321\
Data File : FF009005.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2021 20:30
Operator : DD\AJ
Sample : M3861-08 5X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 24 01:50:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

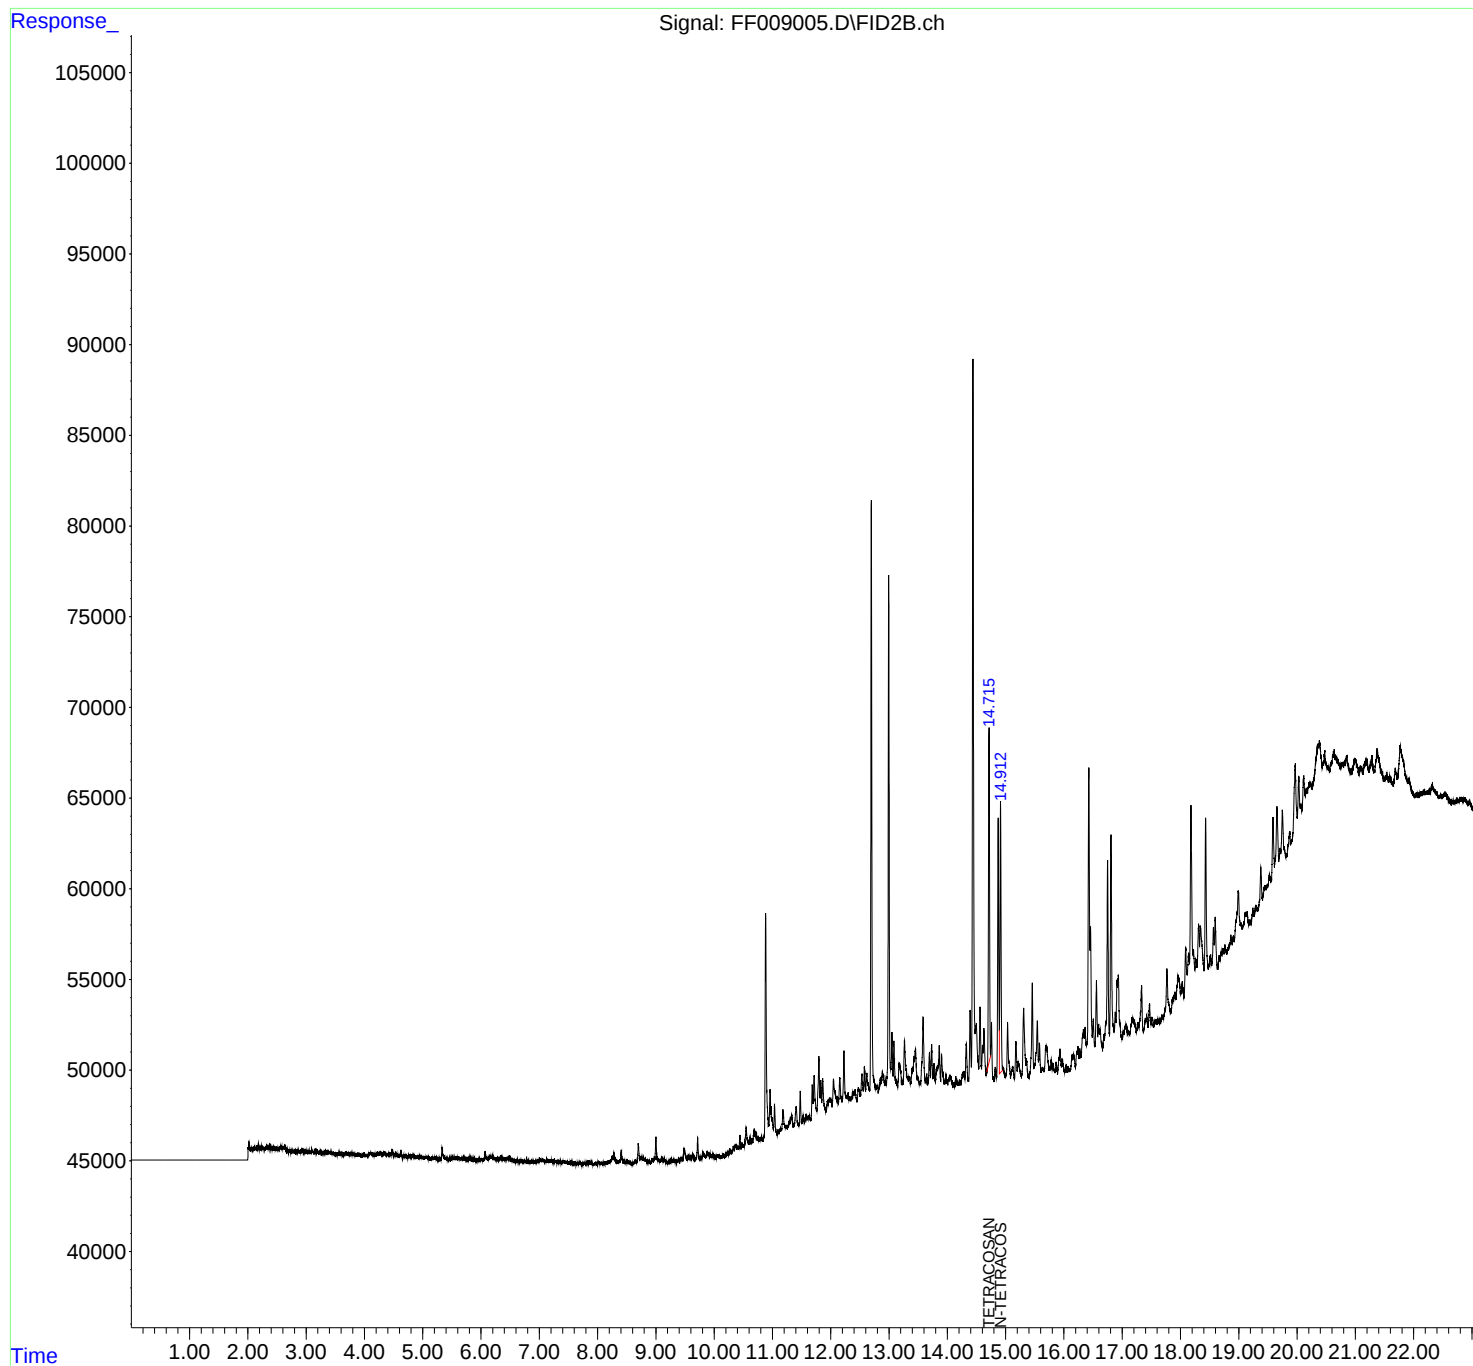


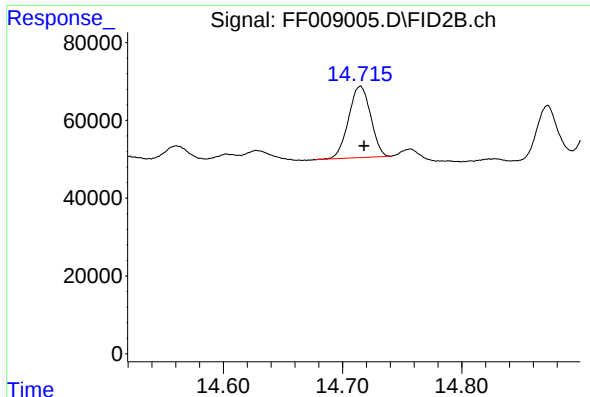

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.715 min
Delta R.T.: -0.003 min
Response: 235812
Conc: 2.01 ug/ml

Instrument :
FID_F
ClientSampleId :

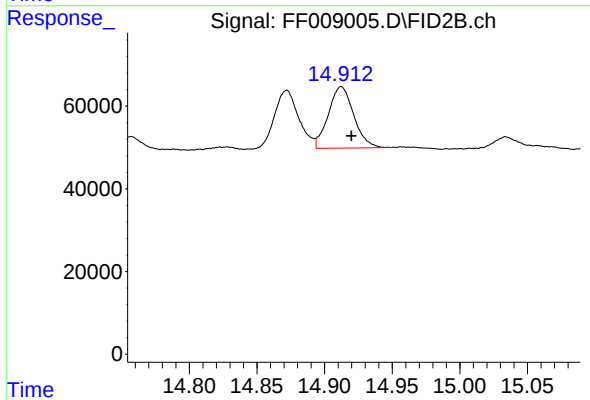

#10 N-TETRACOSANE

R.T.: 14.912 min
Delta R.T.: -0.007 min
Response: 193933
Conc: 1.46 ug/ml