

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092321\
Data File : FF008993.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2021 13:40
Operator : DD\AJ
Sample : PB139303BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB139303BL

Integration File: autoint1.e
Quant Time: Sep 24 01:48:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	2149639	18.299 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092321\
Data File : FF008993.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2021 13:40
Operator : DD\AJ
Sample : PB139303BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB139303BL

Integration File: autoint1.e
Quant Time: Sep 24 01:48:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

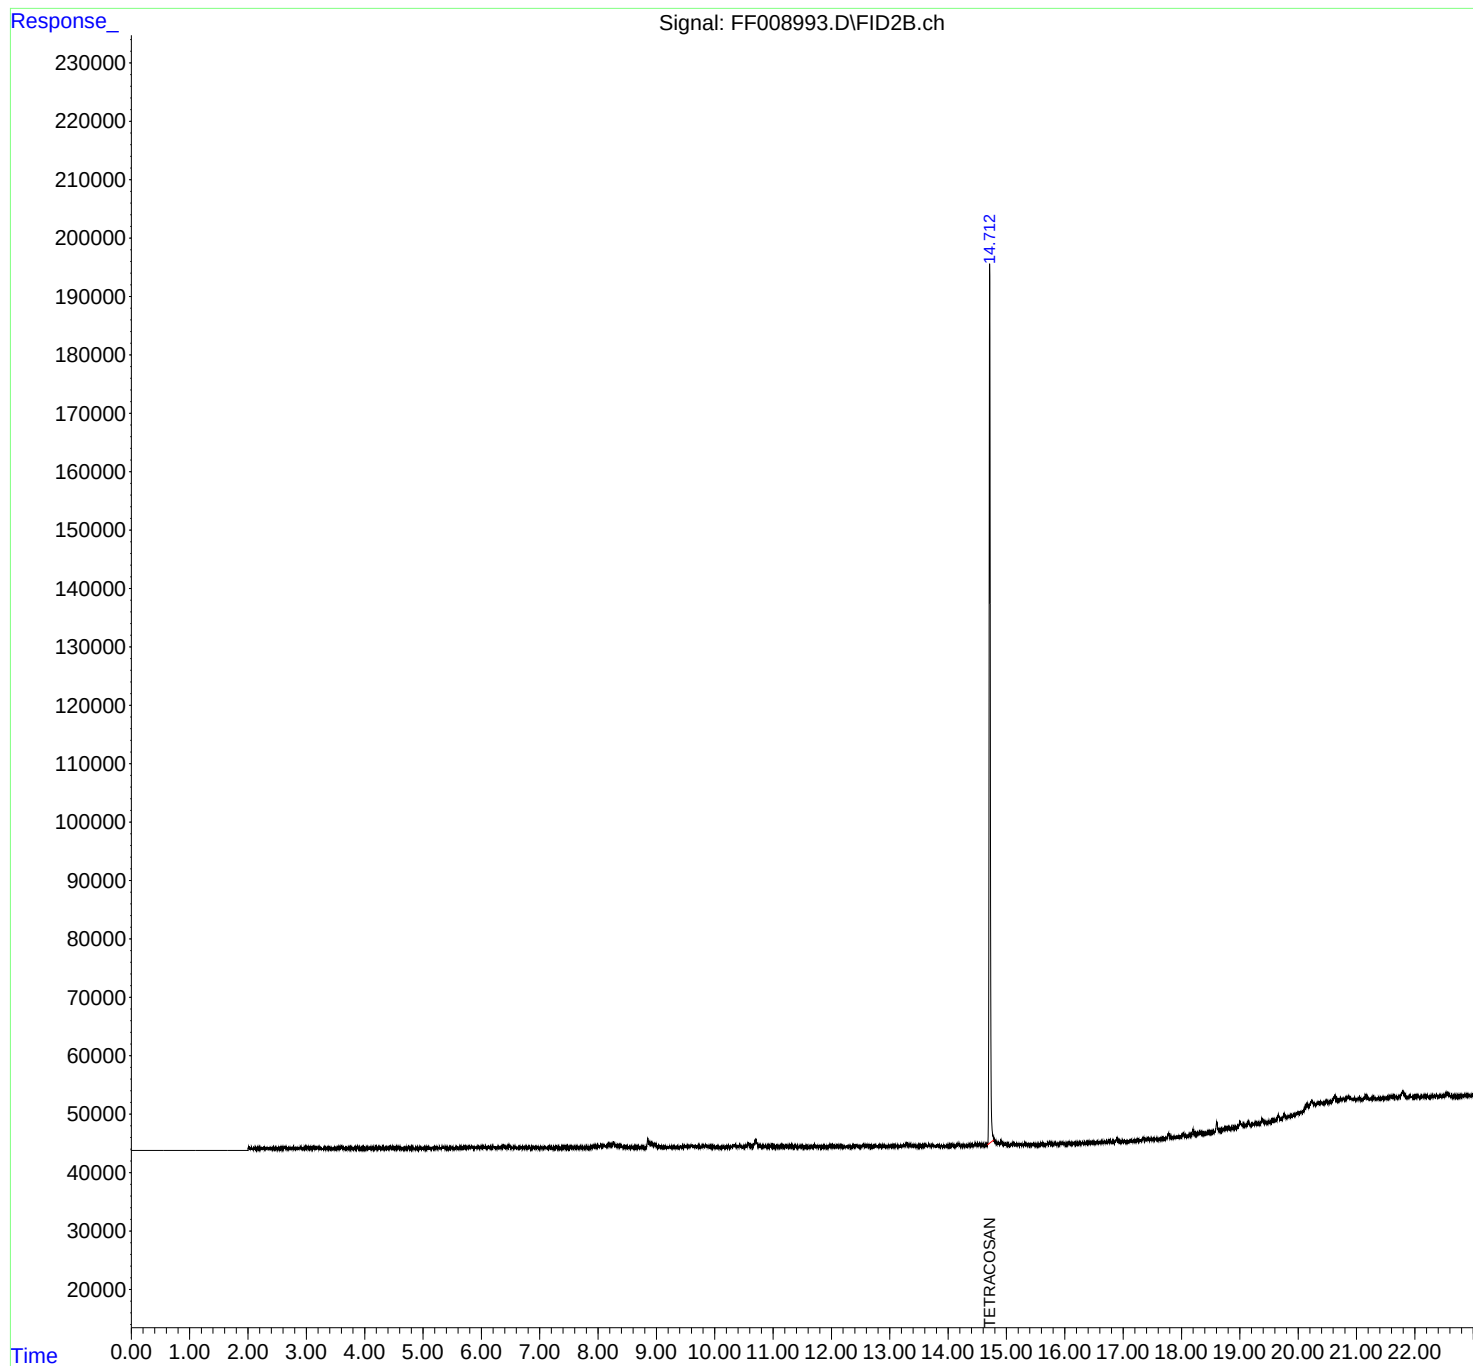

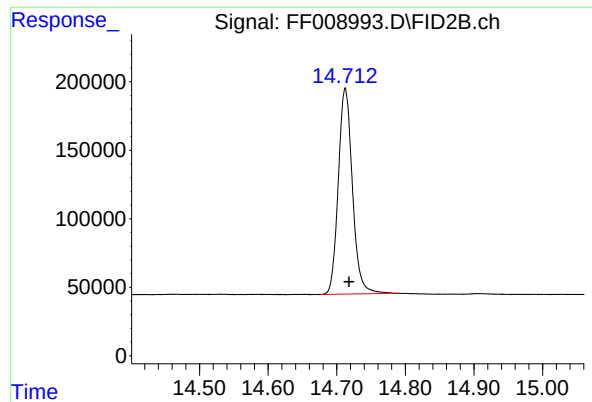

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.712 min
Delta R.T.: -0.006 min
Response: 2149639
Conc: 18.30 ug/ml

Instrument :
FID_F
ClientSampleId :
PB139303BL