

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092322\
 Data File : FF011520.D
 Signal(s) : FID2B.ch
 Acq On : 23 Sep 2022 15:25
 Operator : YP\AJ
 Sample : N4742-02MS
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-08-COMPMS

Integration File: Sample.e
 Quant Time: Sep 24 15:03:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.772	1192818	10.642 ug/ml
Target Compounds			
2) N-DECANE	4.338	2025754	15.613 ug/ml
3) N-DODECANE	6.507	2005555	15.315 ug/ml
4) N-TETRADECANE	8.331	1954005	14.876 ug/ml
5) N-HEXADECANE	9.934	1920884	14.481 ug/ml
6) N-OCTADECANE	11.372	1934758	14.555 ug/ml
7) N-EICOSANE	12.679	1877093	14.270 ug/ml
8) N-DOCOSANE	13.875	1840551	14.400 ug/ml
10) N-TETRACOSANE	14.976	1810819	14.222 ug/ml
11) N-HEXACOSANE	15.995	1785659	14.296 ug/ml
12) N-OCTACOSANE	16.943	1743403	14.233 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092322\
Data File : FF011520.D
Signal(s) : FID2B.ch
Acq On : 23 Sep 2022 15:25
Operator : YP\AJ
Sample : N4742-02MS
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-08-COMPMS

Integration File: Sample.e
Quant Time: Sep 24 15:03:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

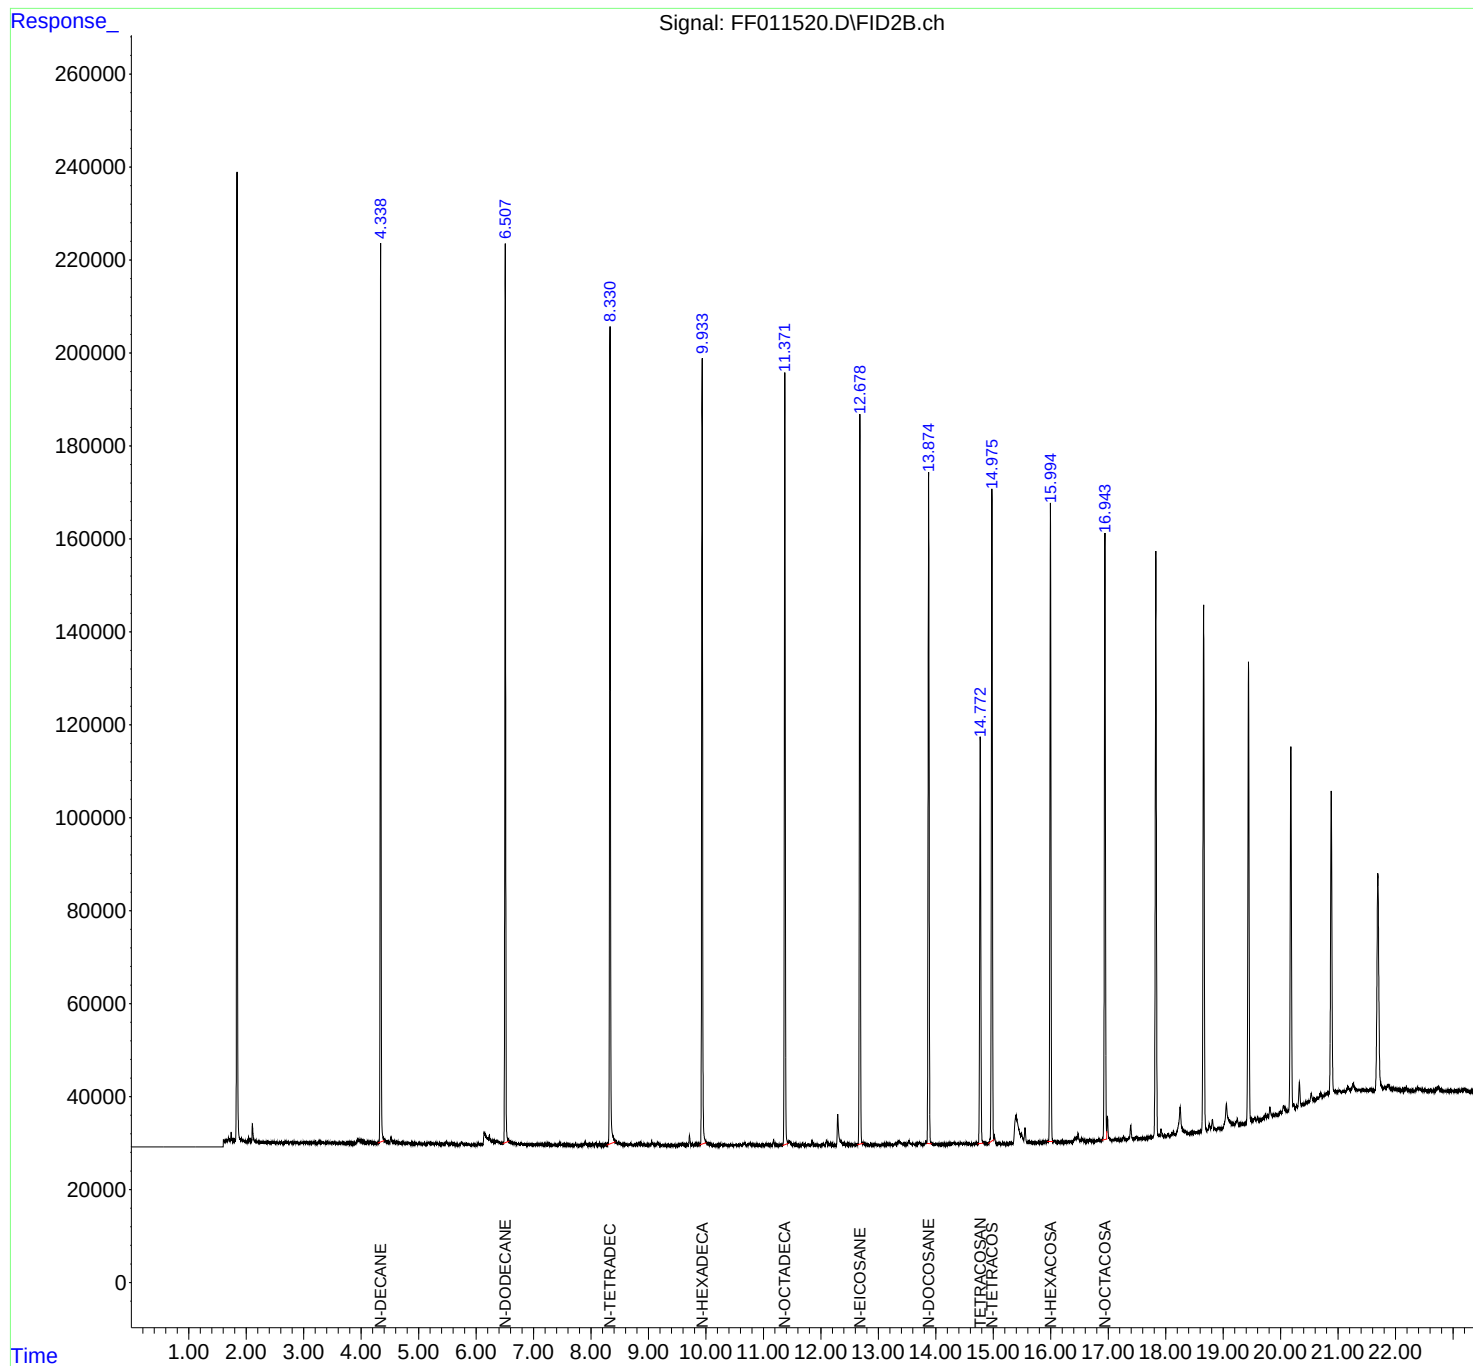


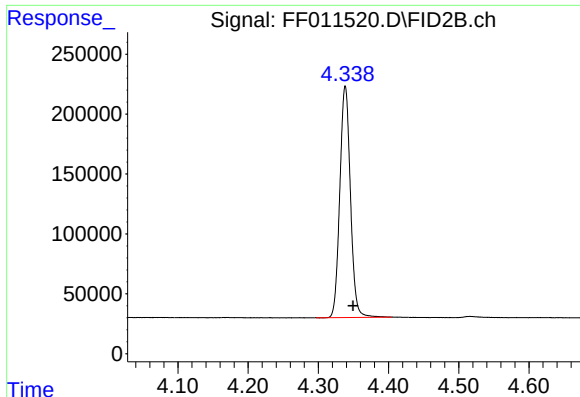

#2 N-DECANE


R.T.: 4.338 min
Delta R.T.: -0.011 min
Response: 2025754
Conc: 15.61 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-08-COMPMS

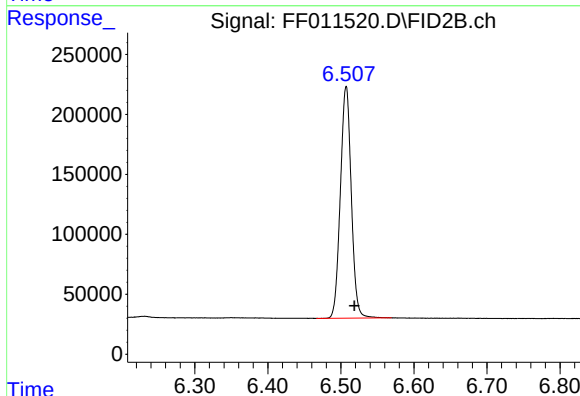


#3 N-DODECANE

R.T.: 6.507 min
Delta R.T.: -0.011 min
Response: 2005555
Conc: 15.32 ug/ml

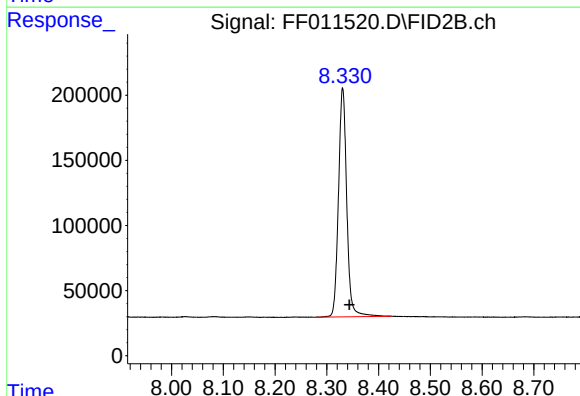


#4 N-TETRADECANE

R.T.: 8.331 min
Delta R.T.: -0.013 min
Response: 1954005
Conc: 14.88 ug/ml

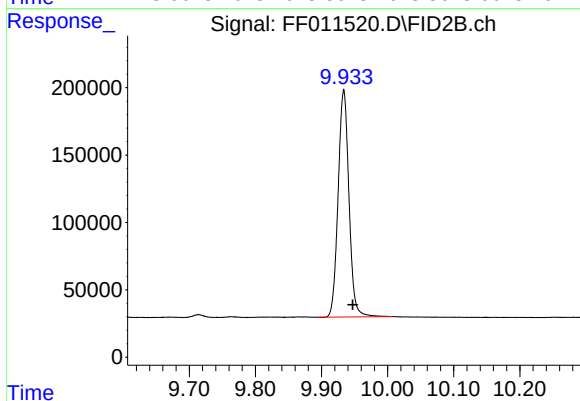

#5 N-HEXADECANE


R.T.: 9.934 min
Delta R.T.: -0.013 min
Response: 1920884
Conc: 14.48 ug/ml

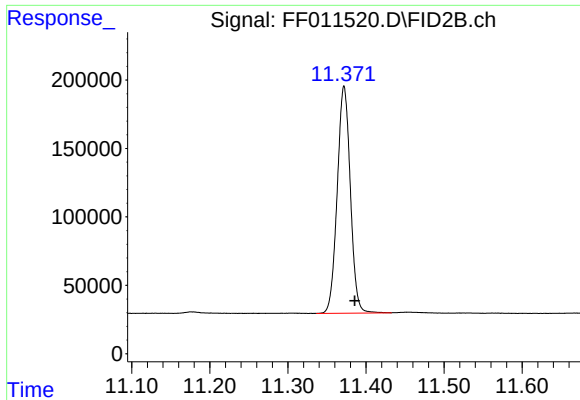

#6 N-OCTADECANE


R.T.: 11.372 min
Delta R.T.: -0.014 min
Response: 1934758
Conc: 14.55 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-08-COMPMS

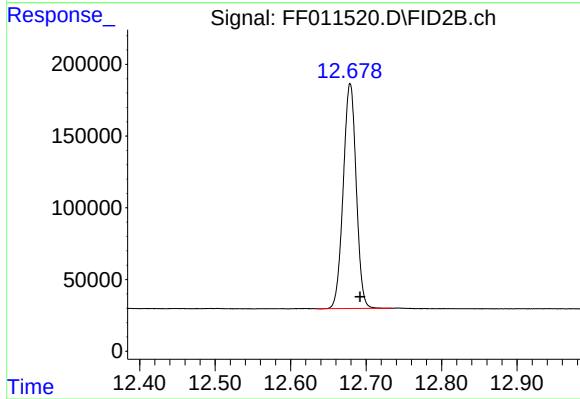


#7 N-EICOSANE

R.T.: 12.679 min
Delta R.T.: -0.013 min
Response: 1877093
Conc: 14.27 ug/ml

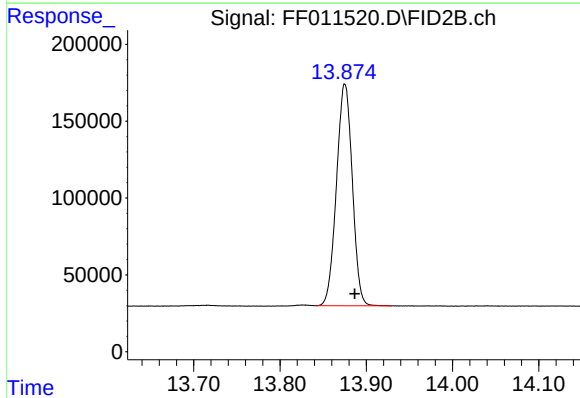


#8 N-DOCOSANE

R.T.: 13.875 min
Delta R.T.: -0.011 min
Response: 1840551
Conc: 14.40 ug/ml

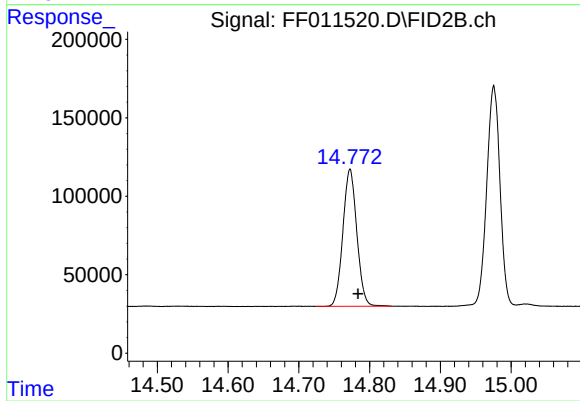

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.772 min
Delta R.T.: -0.011 min
Response: 1192818
Conc: 10.64 ug/ml

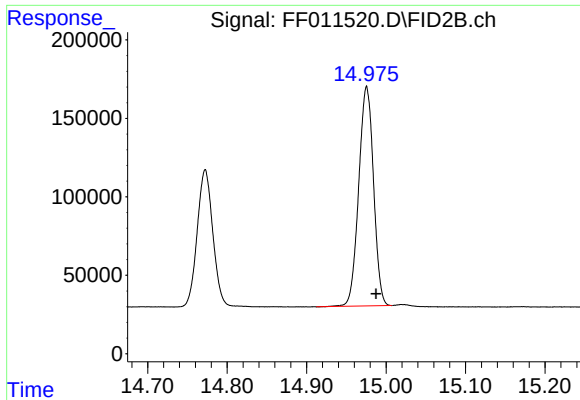

#10 N-TETRACOSANE


R.T.: 14.976 min
Delta R.T.: -0.012 min
Response: 1810819
Conc: 14.22 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-08-COMPMS

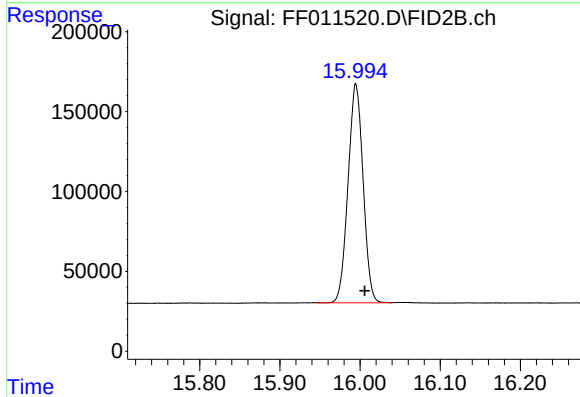

#11 N-HEXACOSANE

R.T.: 15.995 min
Delta R.T.: -0.011 min
Response: 1785659
Conc: 14.30 ug/ml

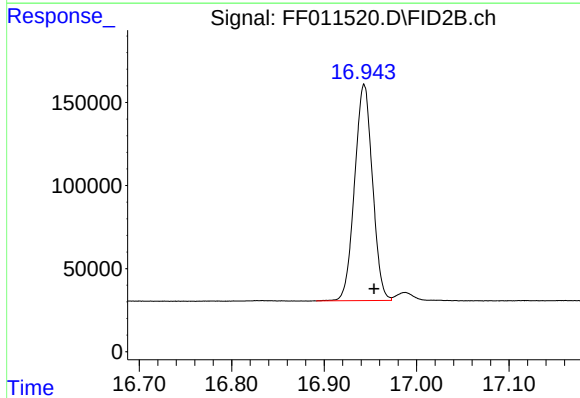

#12 N-OCTACOSANE

R.T.: 16.943 min
Delta R.T.: -0.011 min
Response: 1743403
Conc: 14.23 ug/ml