

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092418\
 Data File : FF002214.D
 Signal(s) : FID2B.ch
 Acq On : 25 Sep 2018 01:32
 Operator : AJ\SJ
 Sample : J5042-02 5X
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 25 05:04:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:20:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.268	487020	3.886 ug/ml
Target Compounds			
4) N-TETRADECANE	7.821	579129	4.371 ug/ml
7) N-EICOSANE	12.245f	1457522	10.226 ug/ml
10) N-TETRACOSANE	14.476	842794	5.939 ug/ml
12) N-OCTACOSANE	16.395	825106	5.751 ug/ml
13) N-TRIACONTANE	17.319	77719	0.536 ug/ml
14) N-DOTRIACONTANE	18.147	141746	1.005 ug/ml
15) N-TETRATRIACONTANE	18.931	90510	0.673 ug/ml
16) N-HEXATRIACONTANE	19.700	143765	1.154 ug/ml
17) N-OCTATRIACONTANE	20.373	119895	1.095 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092418\
Data File : FF002214.D
Signal(s) : FID2B.ch
Acq On : 25 Sep 2018 01:32
Operator : AJ\SJ
Sample : J5042-02 5X
Misc :
ALS Vial : 76 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 25 05:04:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

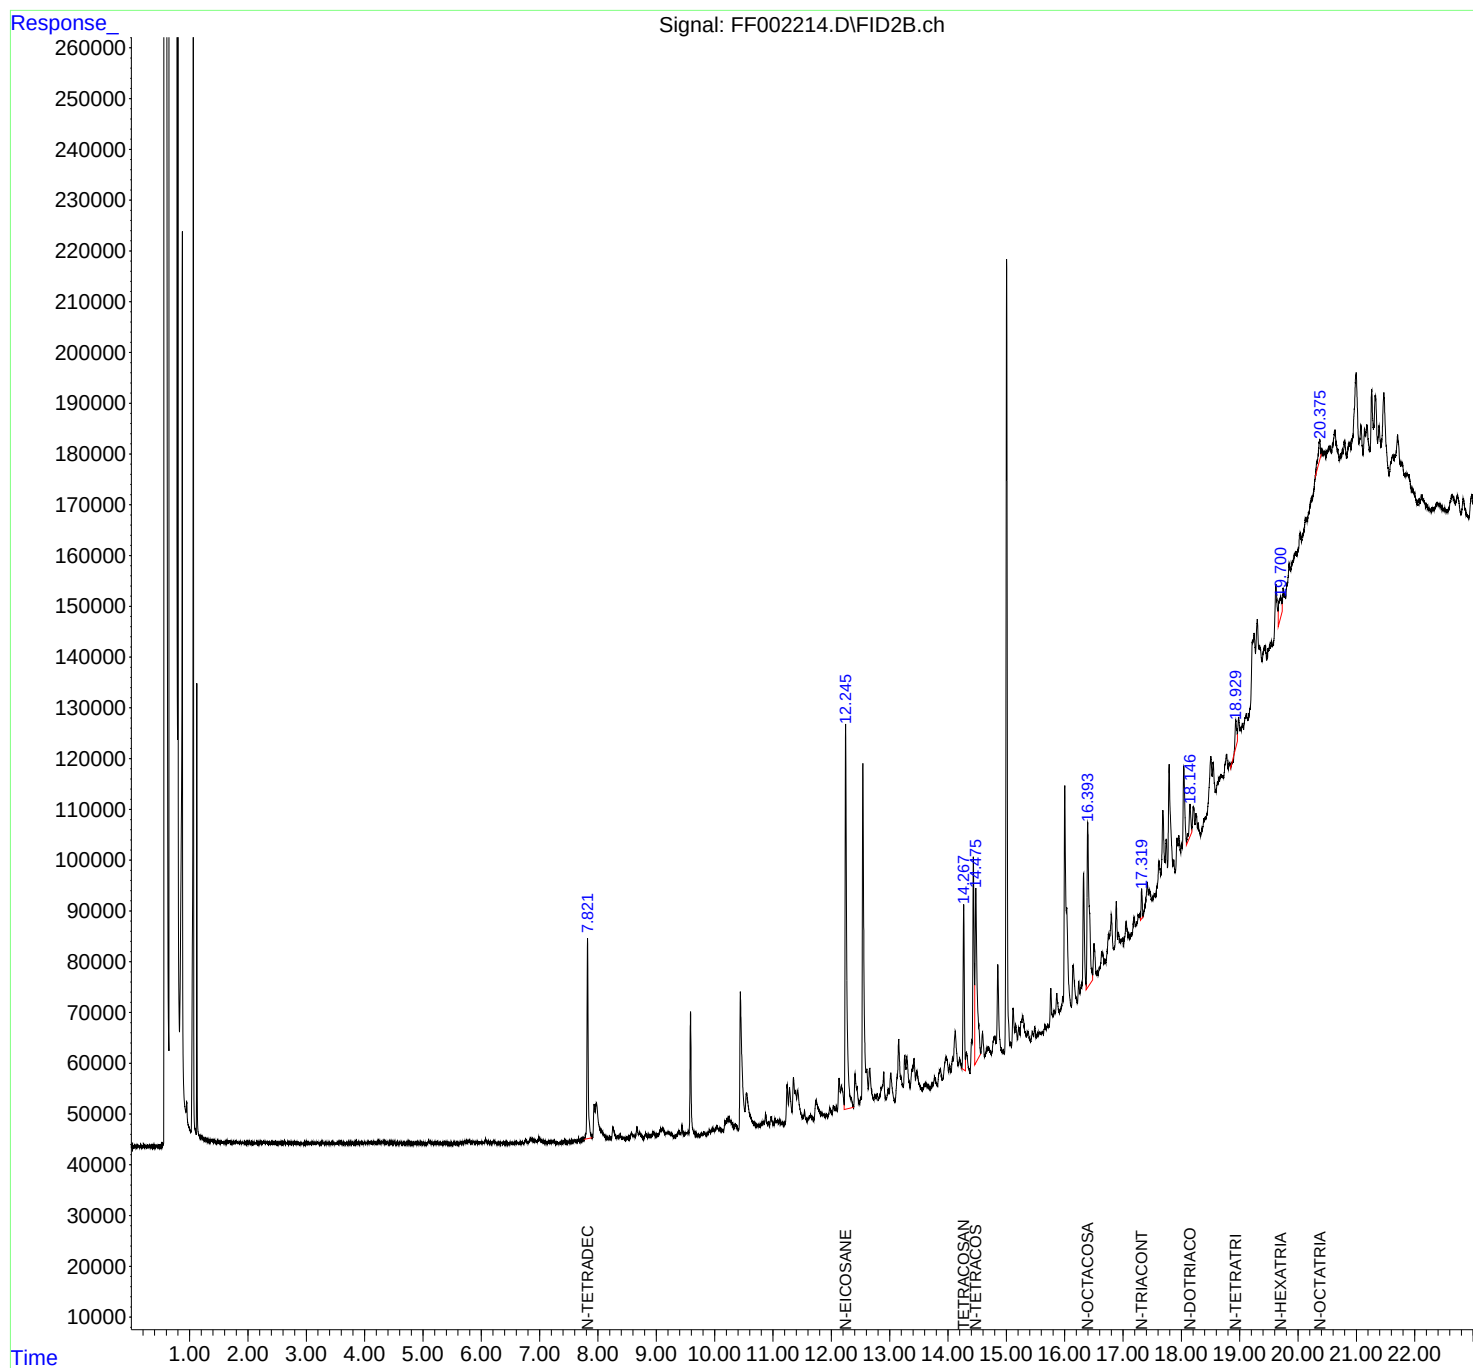

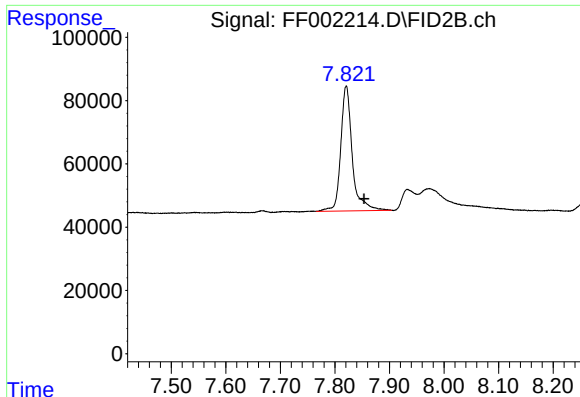


#4 N-TETRADECANE

R.T.: 7.821 min
Delta R.T.: -0.032 min
Response: 579129
Conc: 4.37 ug/ml

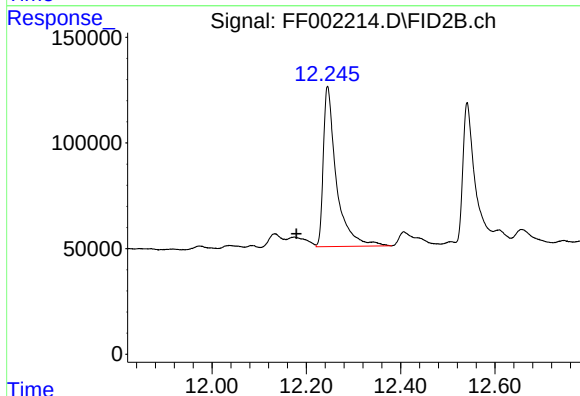


#7 N-EICOSANE

R.T.: 12.245 min
Delta R.T.: 0.066 min
Response: 1457522
Conc: 10.23 ug/ml

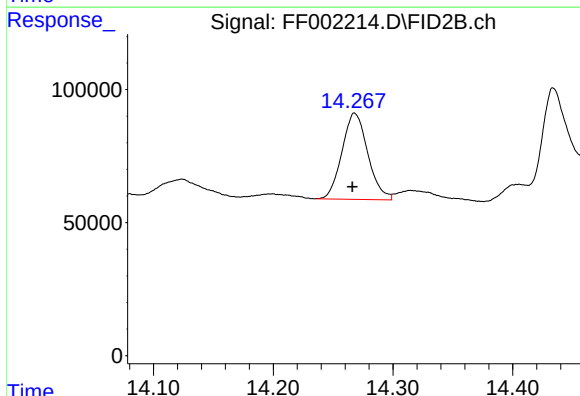


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.268 min
Delta R.T.: 0.002 min
Response: 487020
Conc: 3.89 ug/ml

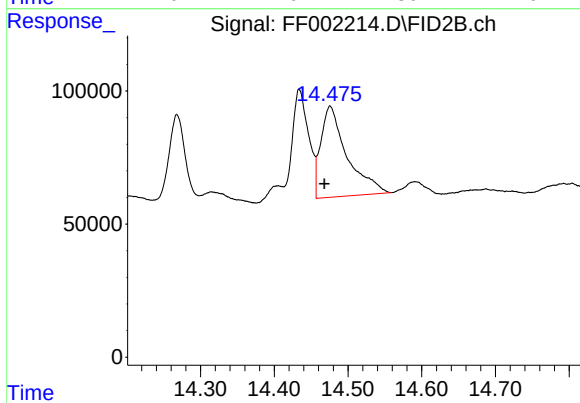


#10 N-TETRACOSANE

R.T.: 14.476 min
Delta R.T.: 0.008 min
Response: 842794
Conc: 5.94 ug/ml

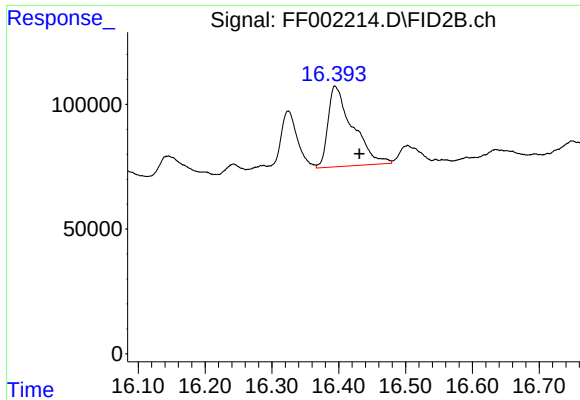


#12 N-OCTACOSANE

R.T.: 16.395 min
Delta R.T.: -0.036 min
Response: 825106
Conc: 5.75 ug/ml

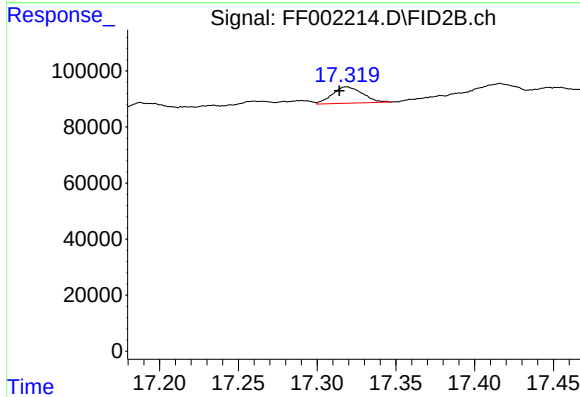


#13 N-TRIACONTANE

R.T.: 17.319 min
Delta R.T.: 0.004 min
Response: 77719
Conc: 0.54 ug/ml

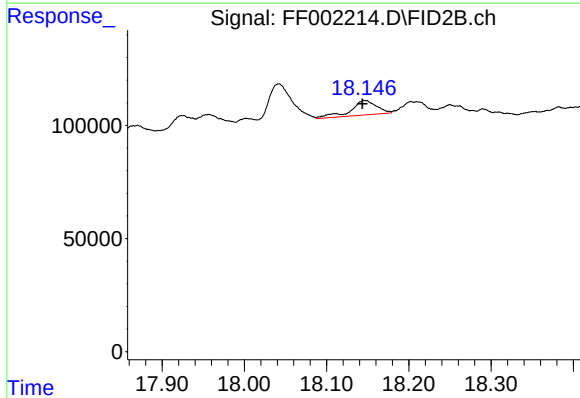


#14 N-DOTRIACONTANE

R.T.: 18.147 min
Delta R.T.: 0.003 min
Response: 141746
Conc: 1.01 ug/ml

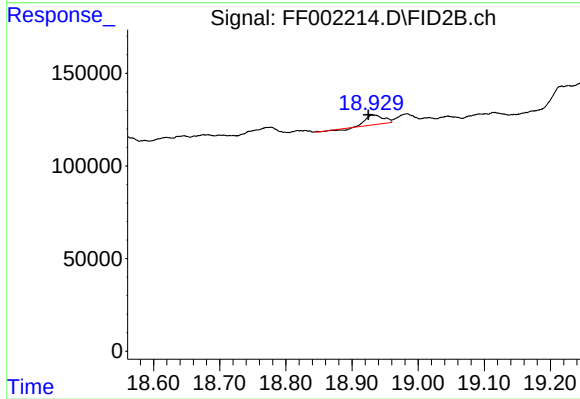


#15 N-TETRATRIACONTANE

R.T.: 18.931 min
Delta R.T.: 0.006 min
Response: 90510
Conc: 0.67 ug/ml

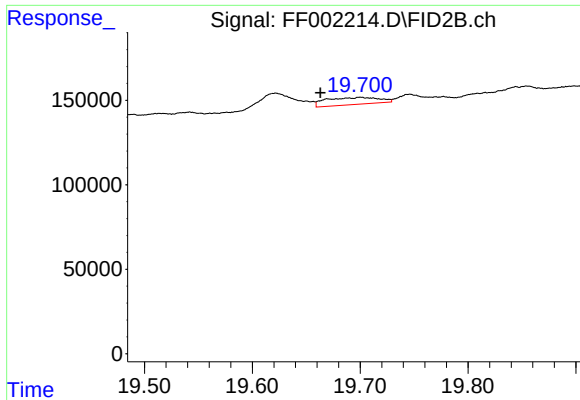

#16 N-HEXATRIACONTANE

R.T.: 19.700 min
Delta R.T.: 0.037 min
Response: 143765
Conc: 1.15 ug/ml

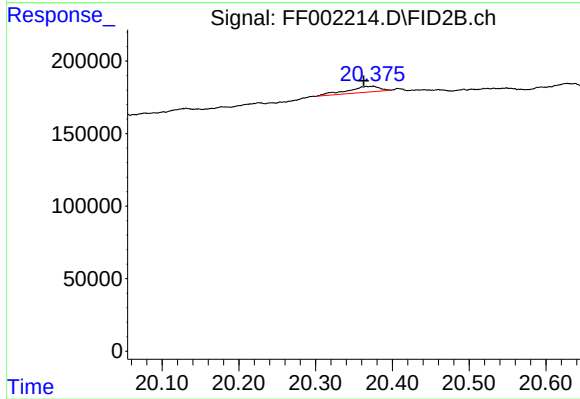

#17 N-OCTATRIACONTANE

R.T.: 20.373 min
Delta R.T.: 0.011 min
Response: 119895
Conc: 1.09 ug/ml