

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092418\
 Data File : FF002215.D
 Signal(s) : FID2B.ch
 Acq On : 25 Sep 2018 02:02
 Operator : AJ\SJ
 Sample : J5042-03 5X
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 25 05:04:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:20:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.267	463819	3.701 ug/ml
Target Compounds			
4) N-TETRADECANE	7.820	493178	3.722 ug/ml
7) N-EICOSANE	12.242f	2119597	14.871 ug/ml
10) N-TETRACOSANE	14.472	1250538	8.812 ug/ml
12) N-OCTACOSANE	16.390	1104046	7.695 ug/ml
13) N-TRIACONTANE	17.320	94188	0.650 ug/ml
14) N-DOTRIACONTANE	18.147	150603	1.068 ug/ml
15) N-TETRATRIACONTANE	18.933	61766	0.459 ug/ml
16) N-HEXATRIACONTANE	19.622	286440	2.300 ug/ml
17) N-OCTATRIACONTANE	20.371	119303	1.090 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092418\
Data File : FF002215.D
Signal(s) : FID2B.ch
Acq On : 25 Sep 2018 02:02
Operator : AJ\SJ
Sample : J5042-03 5X
Misc :
ALS Vial : 77 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 25 05:04:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

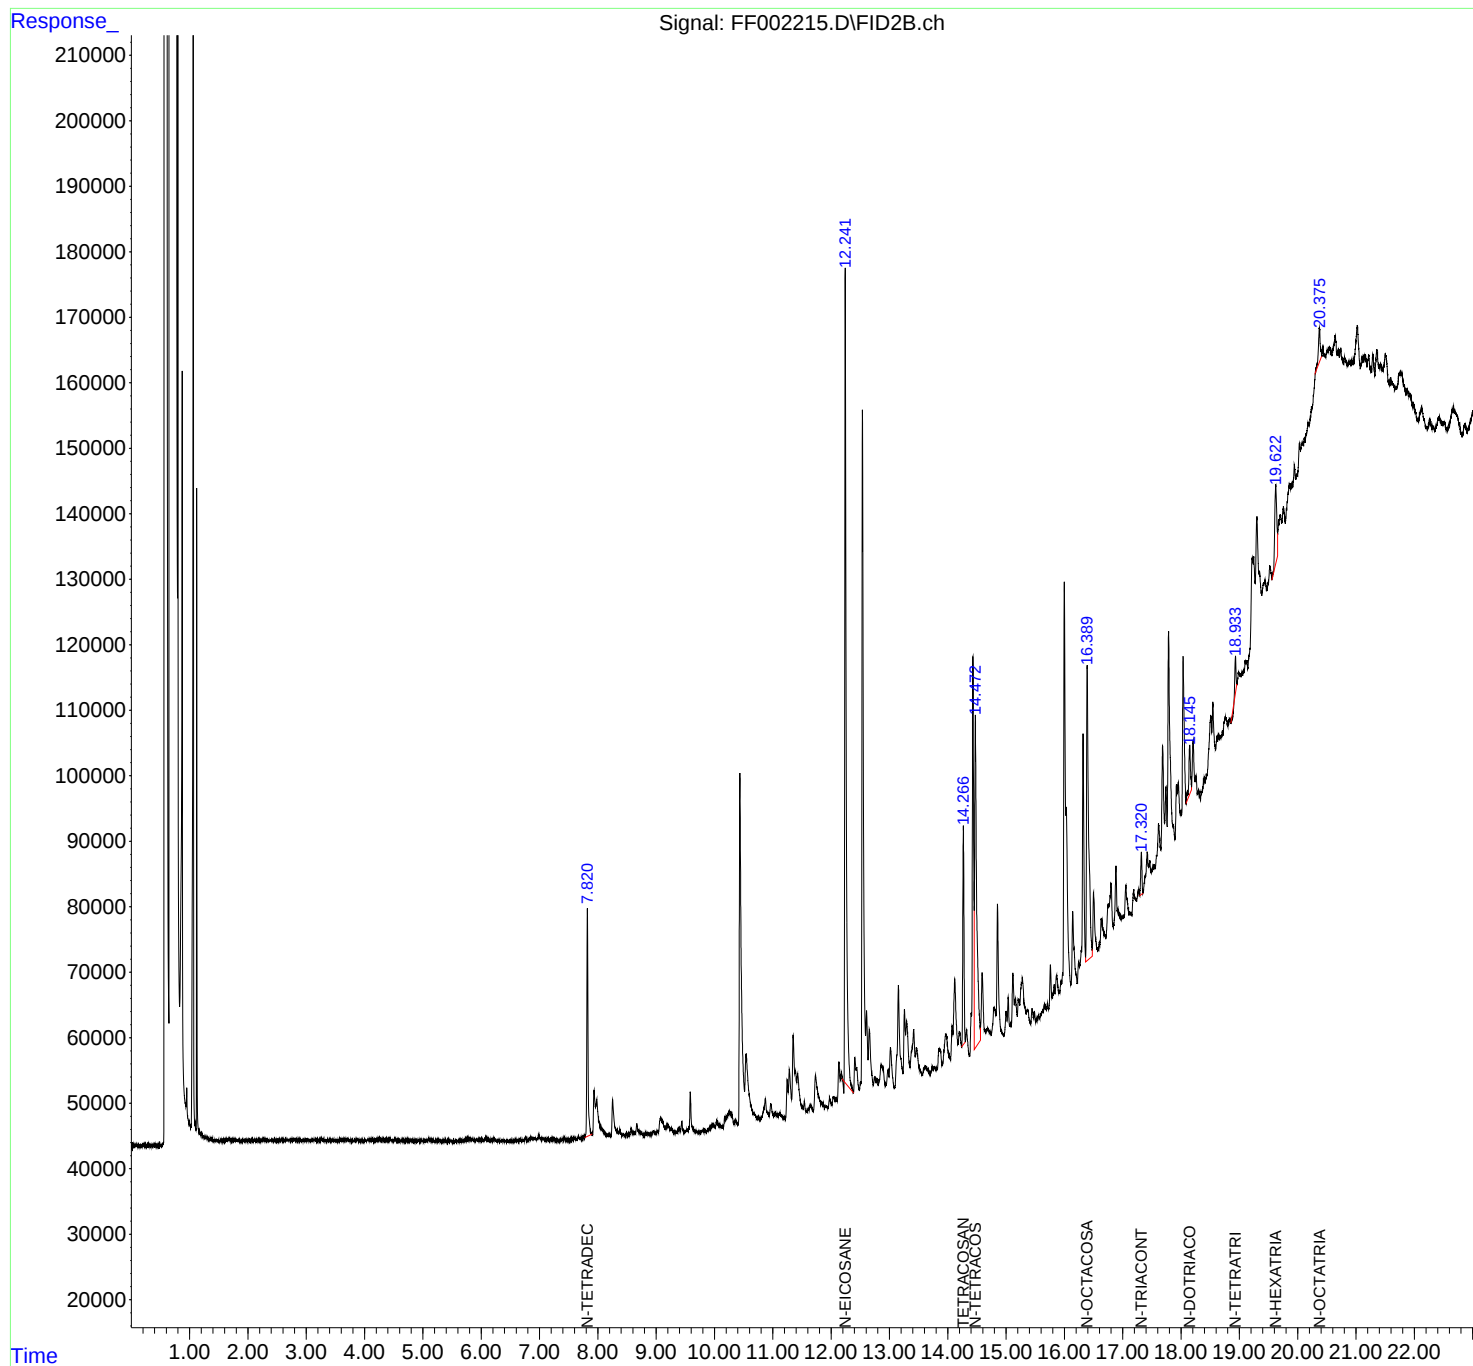

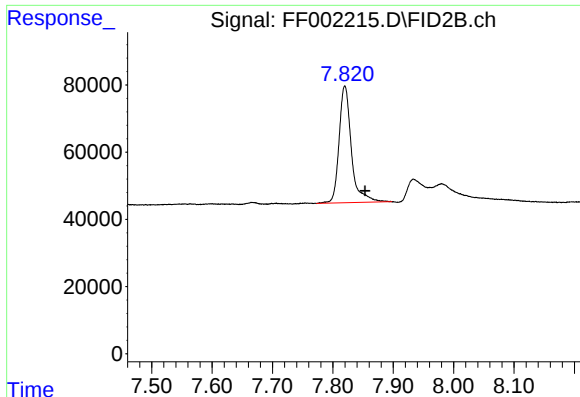


#4 N-TETRADECANE

R.T.: 7.820 min
Delta R.T.: -0.033 min
Response: 493178
Conc: 3.72 ug/ml

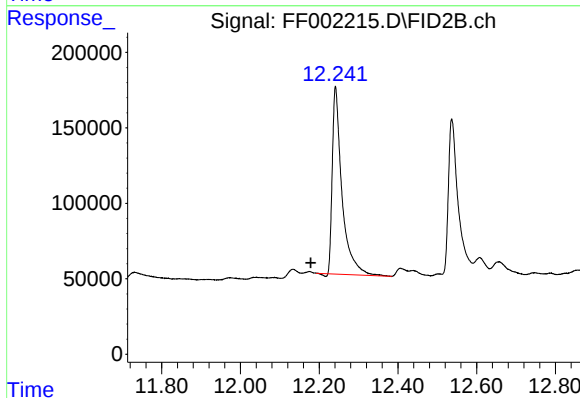


#7 N-EICOSANE

R.T.: 12.242 min
Delta R.T.: 0.063 min
Response: 2119597
Conc: 14.87 ug/ml

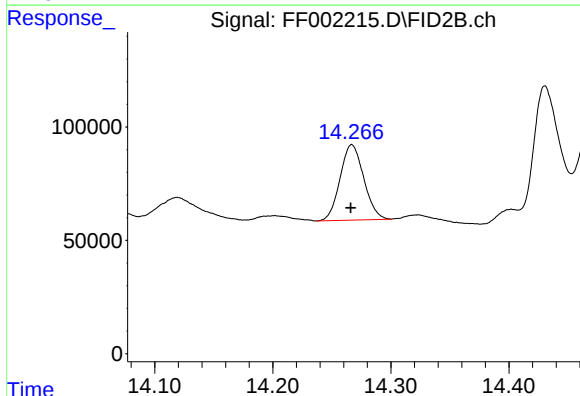


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.267 min
Delta R.T.: 0.001 min
Response: 463819
Conc: 3.70 ug/ml

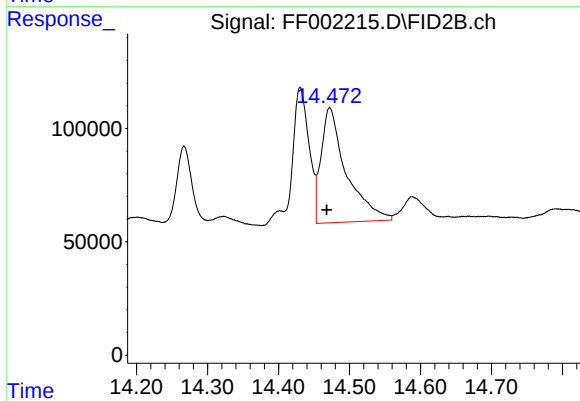


#10 N-TETRACOSANE

R.T.: 14.472 min
Delta R.T.: 0.004 min
Response: 1250538
Conc: 8.81 ug/ml

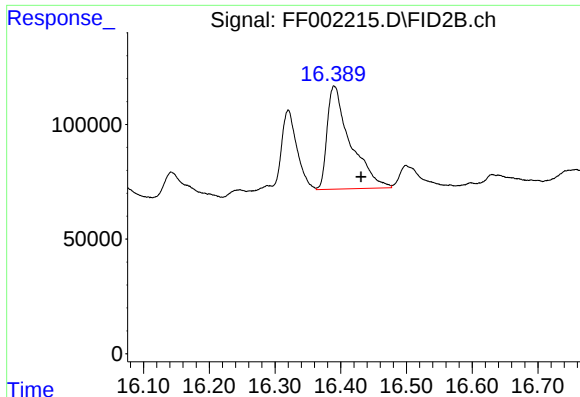


#12 N-OCTACOSANE

R.T.: 16.390 min
Delta R.T.: -0.041 min
Response: 1104046
Conc: 7.70 ug/ml

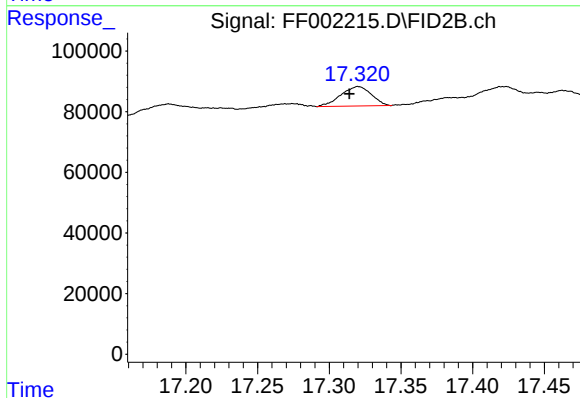


#13 N-TRIACONTANE

R.T.: 17.320 min
Delta R.T.: 0.006 min
Response: 94188
Conc: 0.65 ug/ml

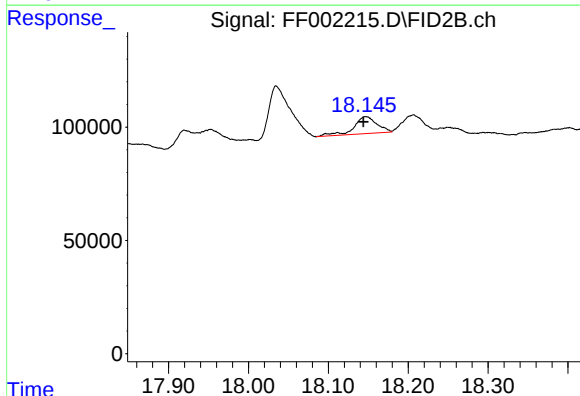


#14 N-DOTRIACONTANE

R.T.: 18.147 min
Delta R.T.: 0.003 min
Response: 150603
Conc: 1.07 ug/ml

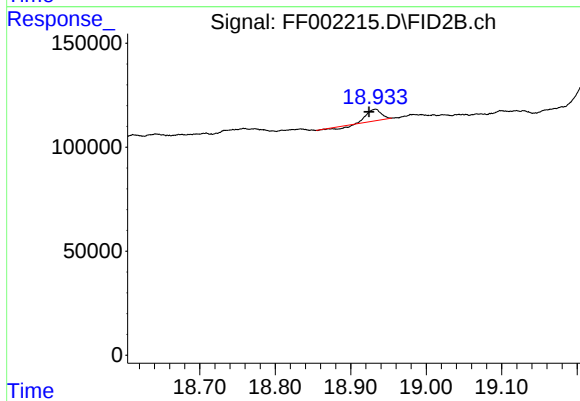


#15 N-TETRATRIACONTANE

R.T.: 18.933 min
Delta R.T.: 0.008 min
Response: 61766
Conc: 0.46 ug/ml

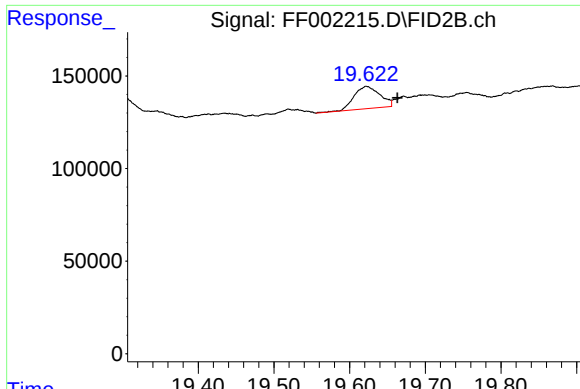

#16 N-HEXATRIACONTANE

R.T.: 19.622 min
Delta R.T.: -0.041 min
Response: 286440
Conc: 2.30 ug/ml

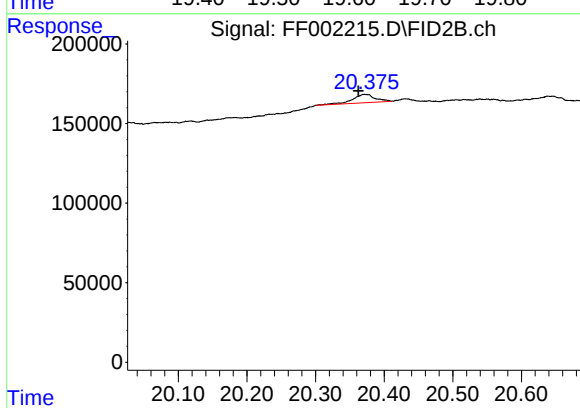

#17 N-OCTATRIACONTANE

R.T.: 20.371 min
Delta R.T.: 0.009 min
Response: 119303
Conc: 1.09 ug/ml