

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092418\
 Data File : FF002216.D
 Signal(s) : FID2B.ch
 Acq On : 25 Sep 2018 02:31
 Operator : AJ\SJ
 Sample : J5042-04 5X
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 25 05:04:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:20:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.267	254766	2.033 ug/ml
Target Compounds				
4)	N-TETRADECANE	7.802f	808429	6.101 ug/ml
5)	N-HEXADECANE	9.469	628386	4.588 ug/ml
6)	N-OCTADECANE	10.826f	247818	1.767 ug/ml
7)	N-EICOSANE	12.187	624325	4.380 ug/ml
8)	N-DOCOSANE	13.383	416864	2.926 ug/ml
10)	N-TETRACOSANE	14.466	2335225	16.456 ug/ml
12)	N-OCTACOSANE	16.382	2079471	14.494 ug/ml
13)	N-TRIACONTANE	17.323	56737	0.391 ug/ml
14)	N-DOTRIACONTANE	18.186	661222	4.690 ug/ml
16)	N-HEXATRIACONTANE	19.684	254786	2.046 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092418\
Data File : FF002216.D
Signal(s) : FID2B.ch
Acq On : 25 Sep 2018 02:31
Operator : AJ\SJ
Sample : J5042-04 5X
Misc :
ALS Vial : 78 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 25 05:04:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

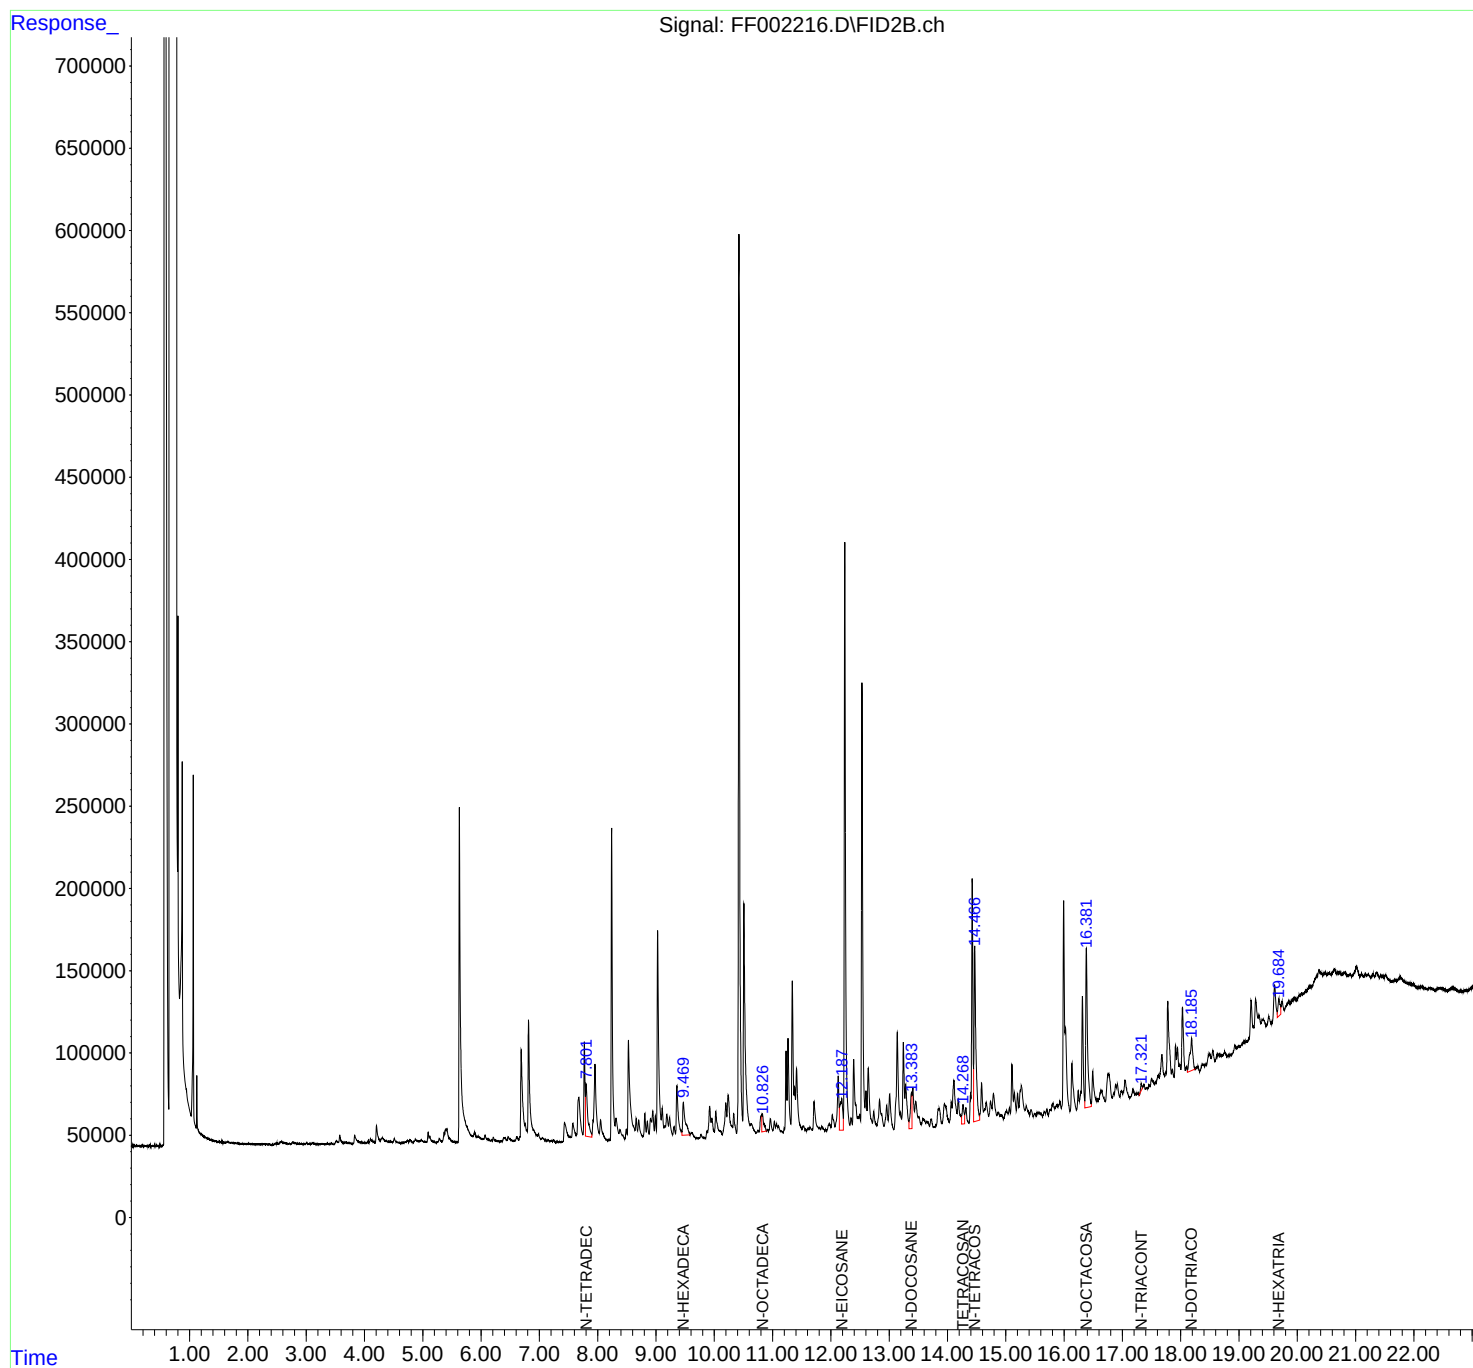

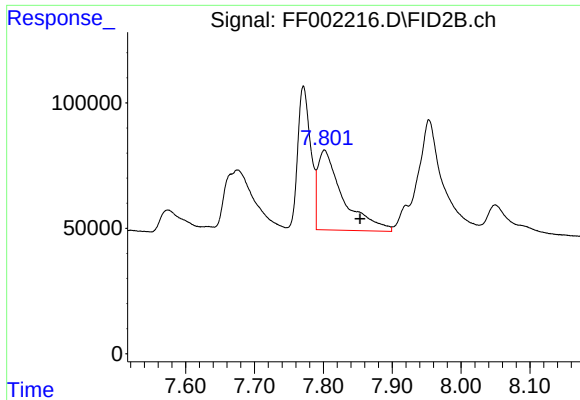


#4 N-TETRADECANE

R.T.: 7.802 min
Delta R.T.: -0.052 min
Response: 808429
Conc: 6.10 ug/ml

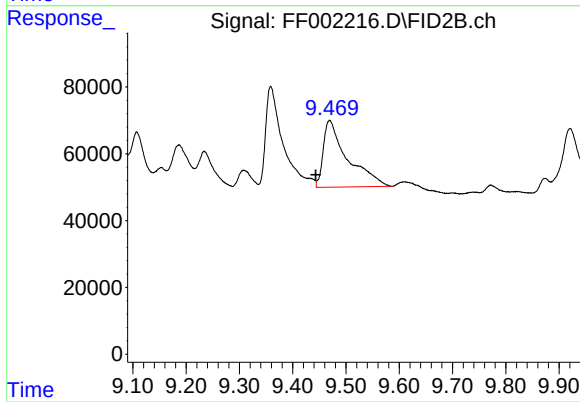


#5 N-HEXADECANE

R.T.: 9.469 min
Delta R.T.: 0.026 min
Response: 628386
Conc: 4.59 ug/ml

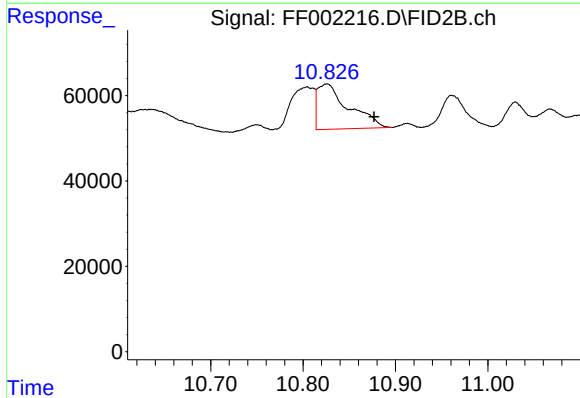


#6 N-OCTADECANE

R.T.: 10.826 min
Delta R.T.: -0.051 min
Response: 247818
Conc: 1.77 ug/ml

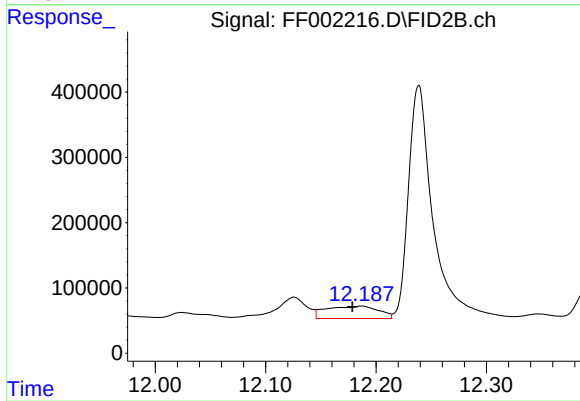


#7 N-EICOSANE

R.T.: 12.187 min
Delta R.T.: 0.008 min
Response: 624325
Conc: 4.38 ug/ml

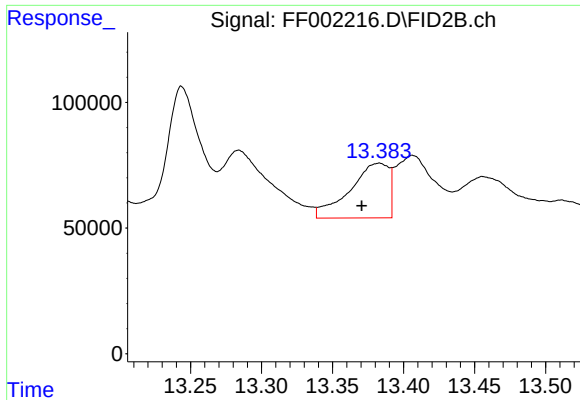


#8 N-DOCOSANE

R.T.: 13.383 min
Delta R.T.: 0.012 min
Response: 416864
Conc: 2.93 ug/ml

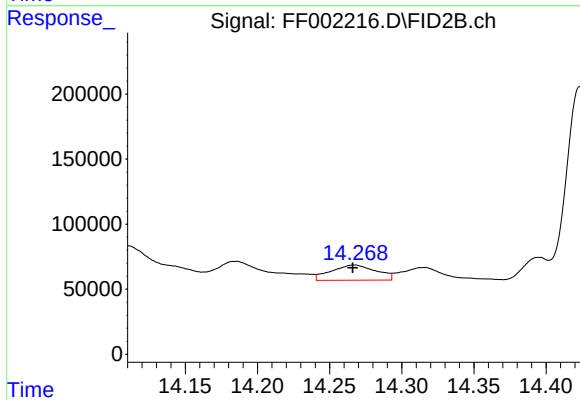


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.267 min
Delta R.T.: 0.001 min
Response: 254766
Conc: 2.03 ug/ml

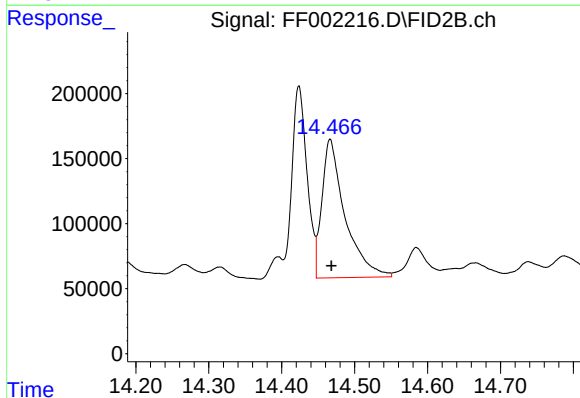


#10 N-TETRACOSANE

R.T.: 14.466 min
Delta R.T.: -0.002 min
Response: 2335225
Conc: 16.46 ug/ml

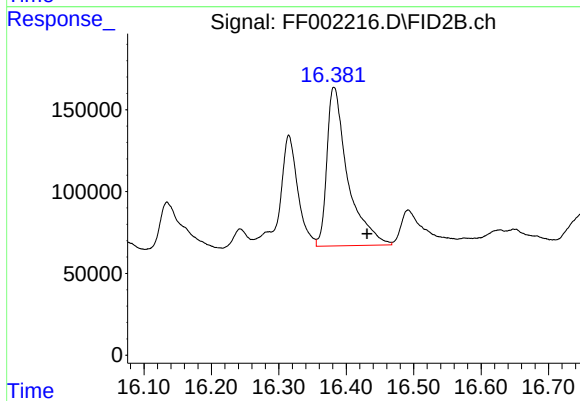


#12 N-OCTACOSANE

R.T.: 16.382 min
Delta R.T.: -0.049 min
Response: 2079471
Conc: 14.49 ug/ml

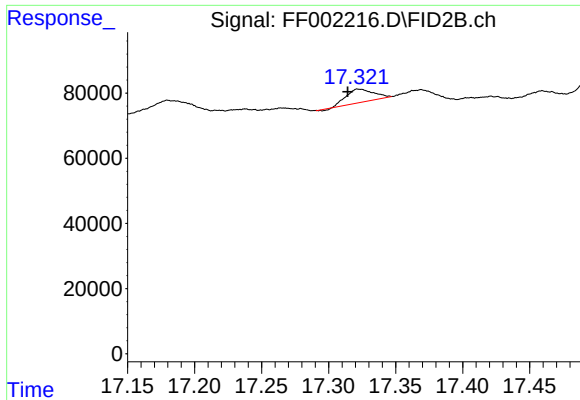


#13 N-TRIACONTANE

R.T.: 17.323 min
Delta R.T.: 0.008 min
Response: 56737
Conc: 0.39 ug/ml

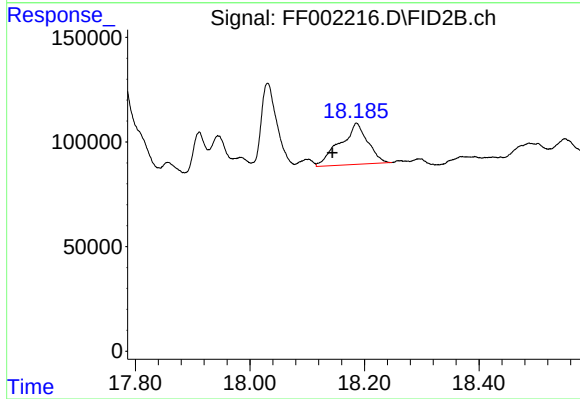

#14 N-DOTRIACONTANE

R.T.: 18.186 min
Delta R.T.: 0.042 min
Response: 661222
Conc: 4.69 ug/ml

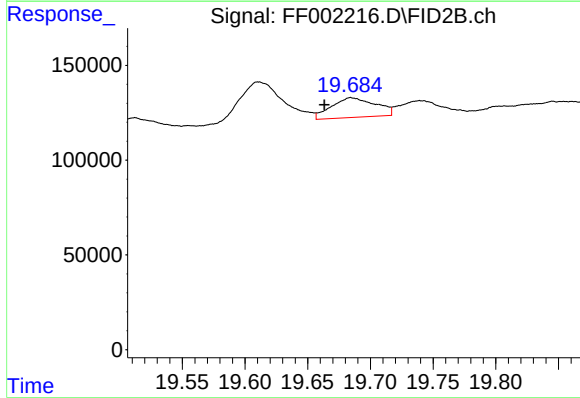

#16 N-HEXATRIACONTANE

R.T.: 19.684 min
Delta R.T.: 0.021 min
Response: 254786
Conc: 2.05 ug/ml