

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092418\
 Data File : FF002195.D
 Signal(s) : FID2B.ch
 Acq On : 24 Sep 2018 16:05
 Operator : AJ\SJ
 Sample : PB113132BS
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 25 05:00:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:20:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.266	2653163	21.168 ug/ml
Target Compounds			
2) N-DECANE	4.058	2938315	25.354 ug/ml
3) N-DODECANE	6.065	3275056	26.174 ug/ml
4) N-TETRADECANE	7.849	3454415	26.071 ug/ml
5) N-HEXADECANE	9.440	3550450	25.924 ug/ml
6) N-OCTADECANE	10.874	3613046	25.765 ug/ml
7) N-EICOSANE	12.177	3577869	25.101 ug/ml
8) N-DOCOSANE	13.370	3491414	24.506 ug/ml
10) N-TETRACOSANE	14.469	3408432	24.018 ug/ml
11) N-HEXACOSANE	15.486	3159342	22.213 ug/ml
12) N-OCTACOSANE	16.432	2982822	20.791 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092418\
Data File : FF002195.D
Signal(s) : FID2B.ch
Acq On : 24 Sep 2018 16:05
Operator : AJ\SJ
Sample : PB113132BS
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 25 05:00:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

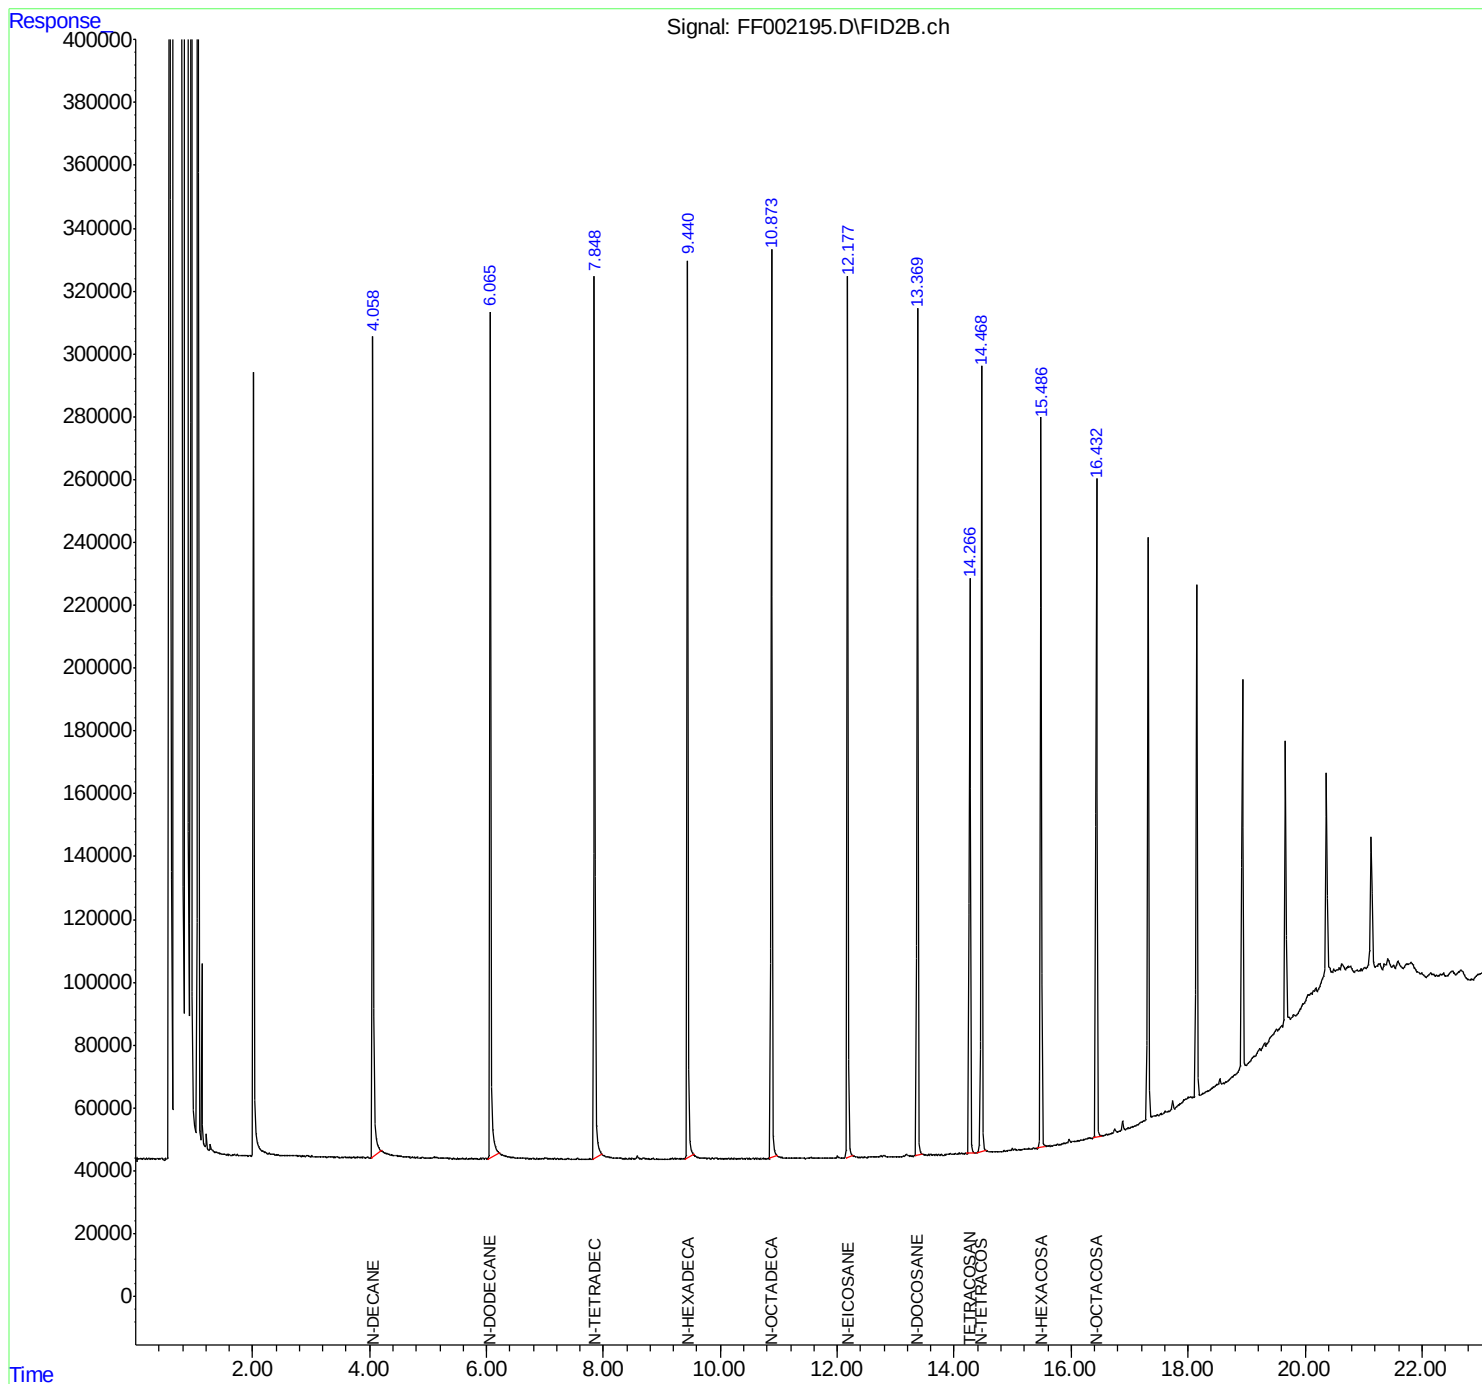

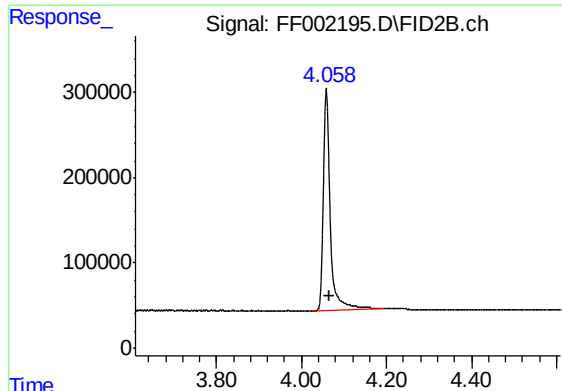


#2 N-DECANE

R.T.: 4.058 min
Delta R.T.: -0.008 min
Response: 2938315
Conc: 25.35 ug/ml

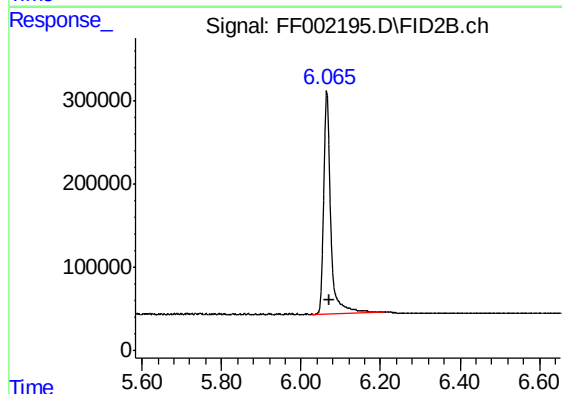


#3 N-DODECANE

R.T.: 6.065 min
Delta R.T.: -0.006 min
Response: 3275056
Conc: 26.17 ug/ml

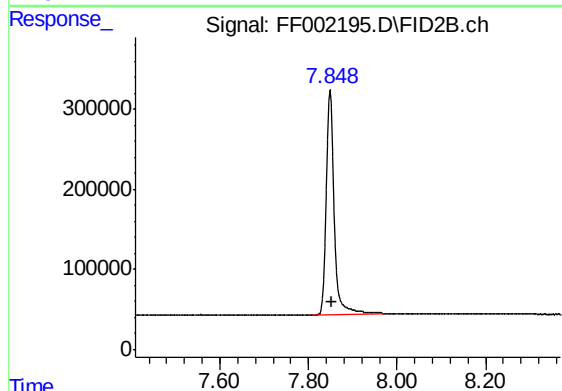


#4 N-TETRADECANE

R.T.: 7.849 min
Delta R.T.: -0.004 min
Response: 3454415
Conc: 26.07 ug/ml

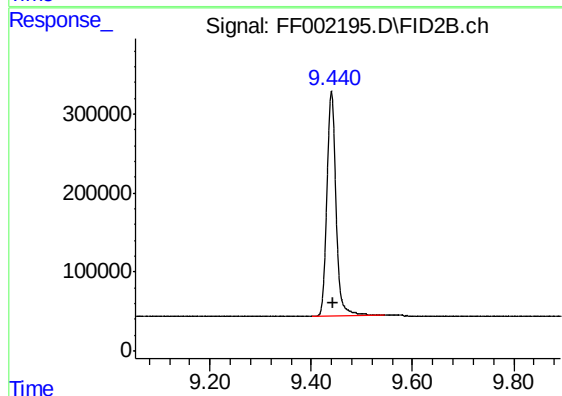


#5 N-HEXADECANE

R.T.: 9.440 min
Delta R.T.: -0.003 min
Response: 3550450
Conc: 25.92 ug/ml

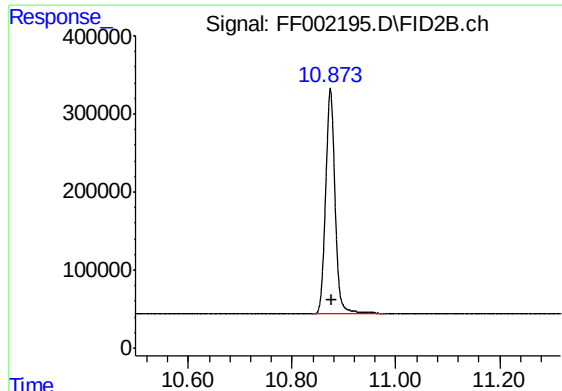


#6 N-OCTADECANE

R.T.: 10.874 min
Delta R.T.: -0.003 min
Response: 3613046
Conc: 25.76 ug/ml

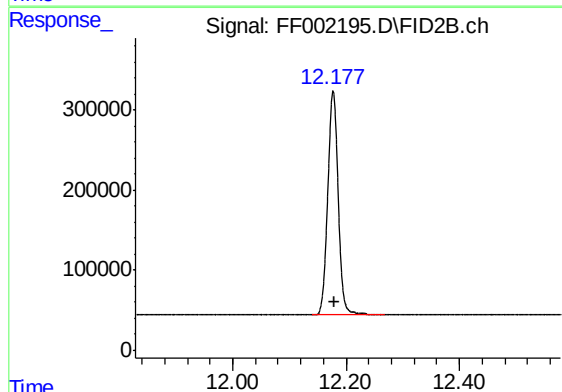


#7 N-EICOSANE

R.T.: 12.177 min
Delta R.T.: -0.002 min
Response: 3577869
Conc: 25.10 ug/ml

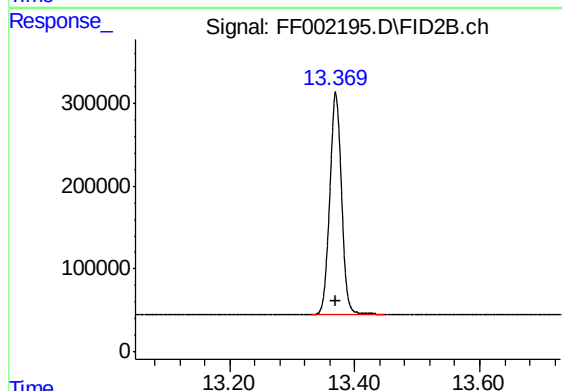


#8 N-DOCOSANE

R.T.: 13.370 min
Delta R.T.: 0.000 min
Response: 3491414
Conc: 24.51 ug/ml

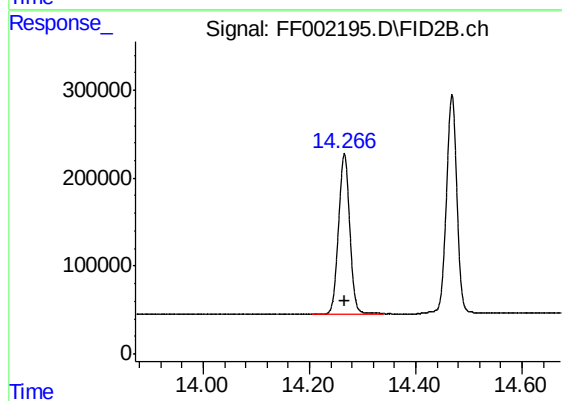


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.266 min
Delta R.T.: 0.000 min
Response: 2653163
Conc: 21.17 ug/ml

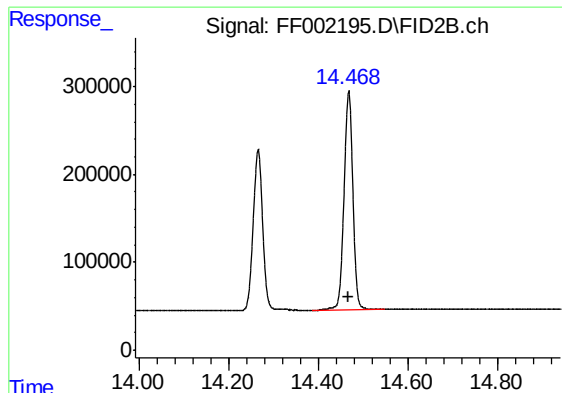


#10 N-TETRACOSANE

R.T.: 14.469 min
Delta R.T.: 0.000 min
Response: 3408432
Conc: 24.02 ug/ml

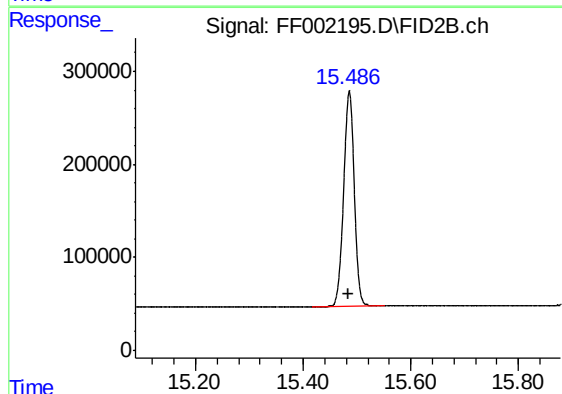

#11 N-HEXACOSANE

R.T.: 15.486 min
Delta R.T.: 0.000 min
Response: 3159342
Conc: 22.21 ug/ml

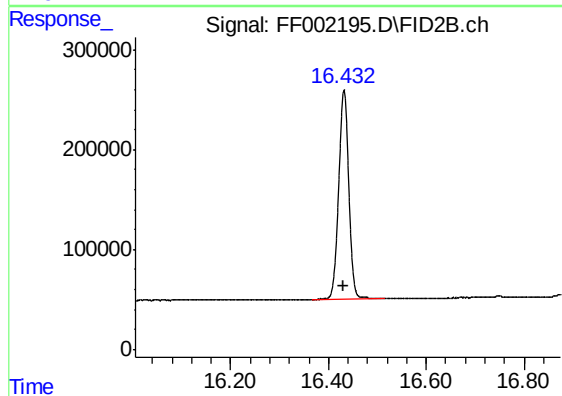

#12 N-OCTACOSANE

R.T.: 16.432 min
Delta R.T.: 0.001 min
Response: 2982822
Conc: 20.79 ug/ml