

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092420\
Data File : FF007660.D
Signal(s) : FID2B.ch
Acq On : 24 Sep 2020 14:50
Operator : DD\AJ
Sample : L3863-05 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 25 02:11:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.731	148986	1.013 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.333f	97262	0.591 ug/ml
13)	N-TRIACONTANE	17.803	129307	0.875 ug/ml
14)	N-DOTRIACONTANE	18.634	130621	0.941 ug/ml
15)	N-TETRATRIACONTANE	19.420	50152	0.397 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092420\
Data File : FF007660.D
Signal(s) : FID2B.ch
Acq On : 24 Sep 2020 14:50
Operator : DD\AJ
Sample : L3863-05 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 25 02:11:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

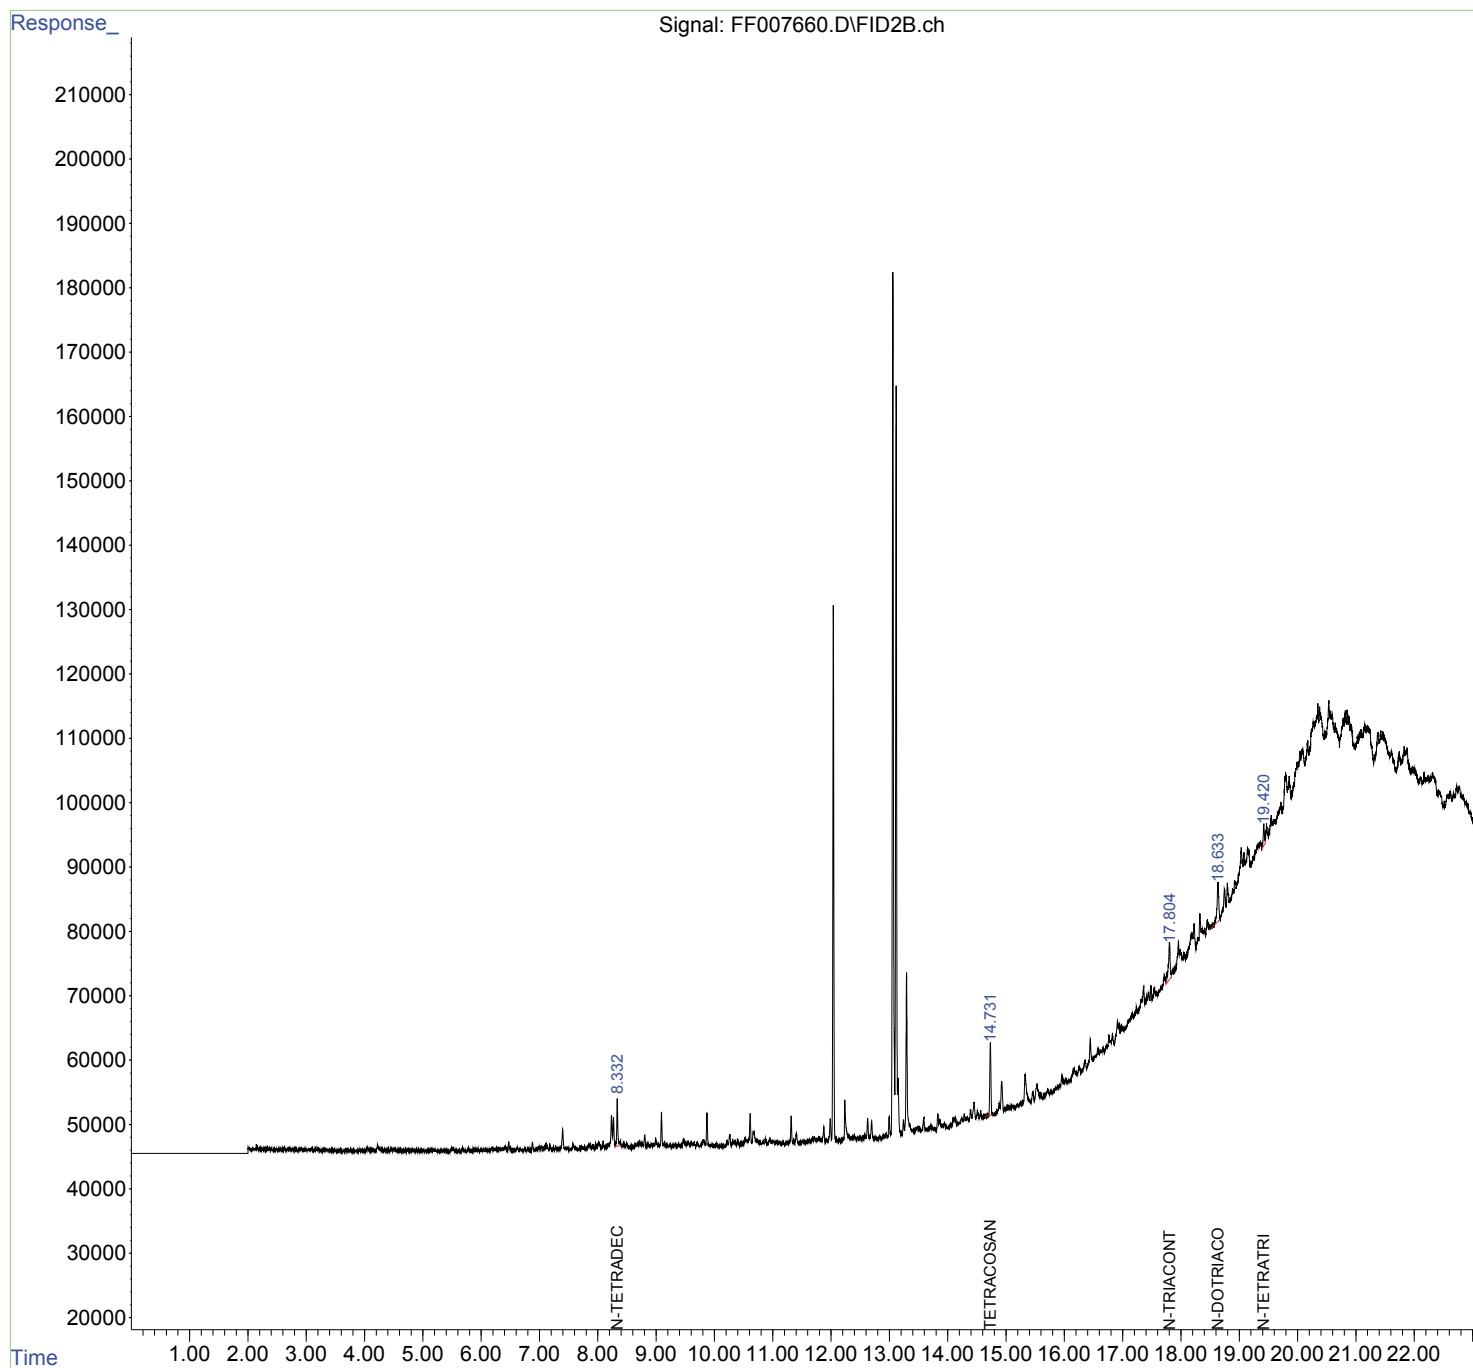

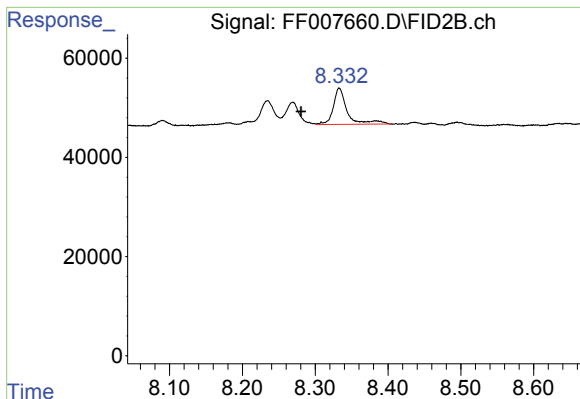


#4 N-TETRADECANE

R.T.: 8.333 min
Delta R.T.: 0.053 min
Response: 97262
Conc: 0.59 ug/ml

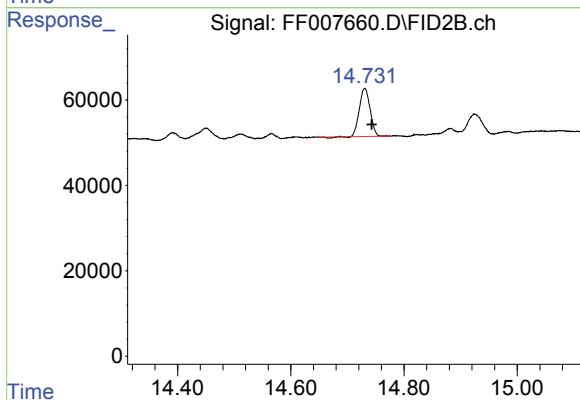


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.731 min
Delta R.T.: -0.012 min
Response: 148986
Conc: 1.01 ug/ml

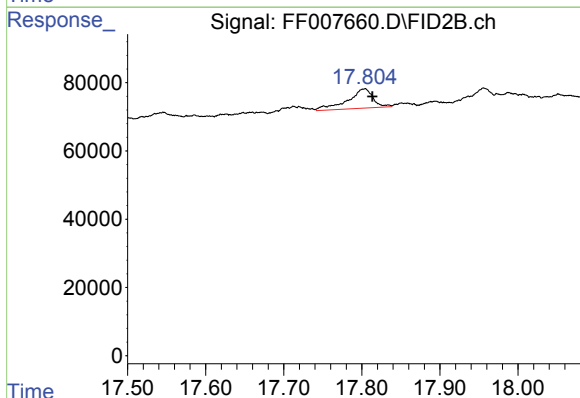


#13 N-TRIACONTANE

R.T.: 17.803 min
Delta R.T.: -0.010 min
Response: 129307
Conc: 0.87 ug/ml

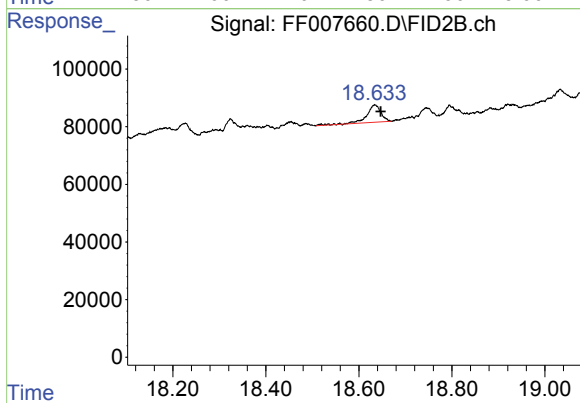

#14 N-DOTRIACONTANE

R.T.: 18.634 min
Delta R.T.: -0.013 min
Response: 130621
Conc: 0.94 ug/ml

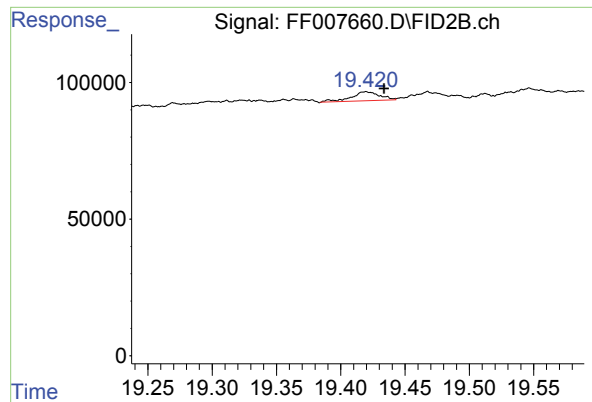

#15 N-TETRATRIACONTANE

R.T.: 19.420 min
Delta R.T.: -0.014 min
Response: 50152
Conc: 0.40 ug/ml