

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092421\
 Data File : FF009008.D
 Signal(s) : FID2B.ch
 Acq On : 24 Sep 2021 09:22
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 24 22:46:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
 Quant Title :
 QLast Update : Wed Sep 08 10:20:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.768	174971	1.497 ug/ml
14) N-DOTRIACONTANE	18.597	227596	2.109 ug/ml
15) N-TETRATRIACONTANE	19.378	170650	1.742 ug/ml
16) N-HEXATRIACONTANE	20.116	100530	1.150 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092421\
Data File : FF009008.D
Signal(s) : FID2B.ch
Acq On : 24 Sep 2021 09:22
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 24 22:46:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

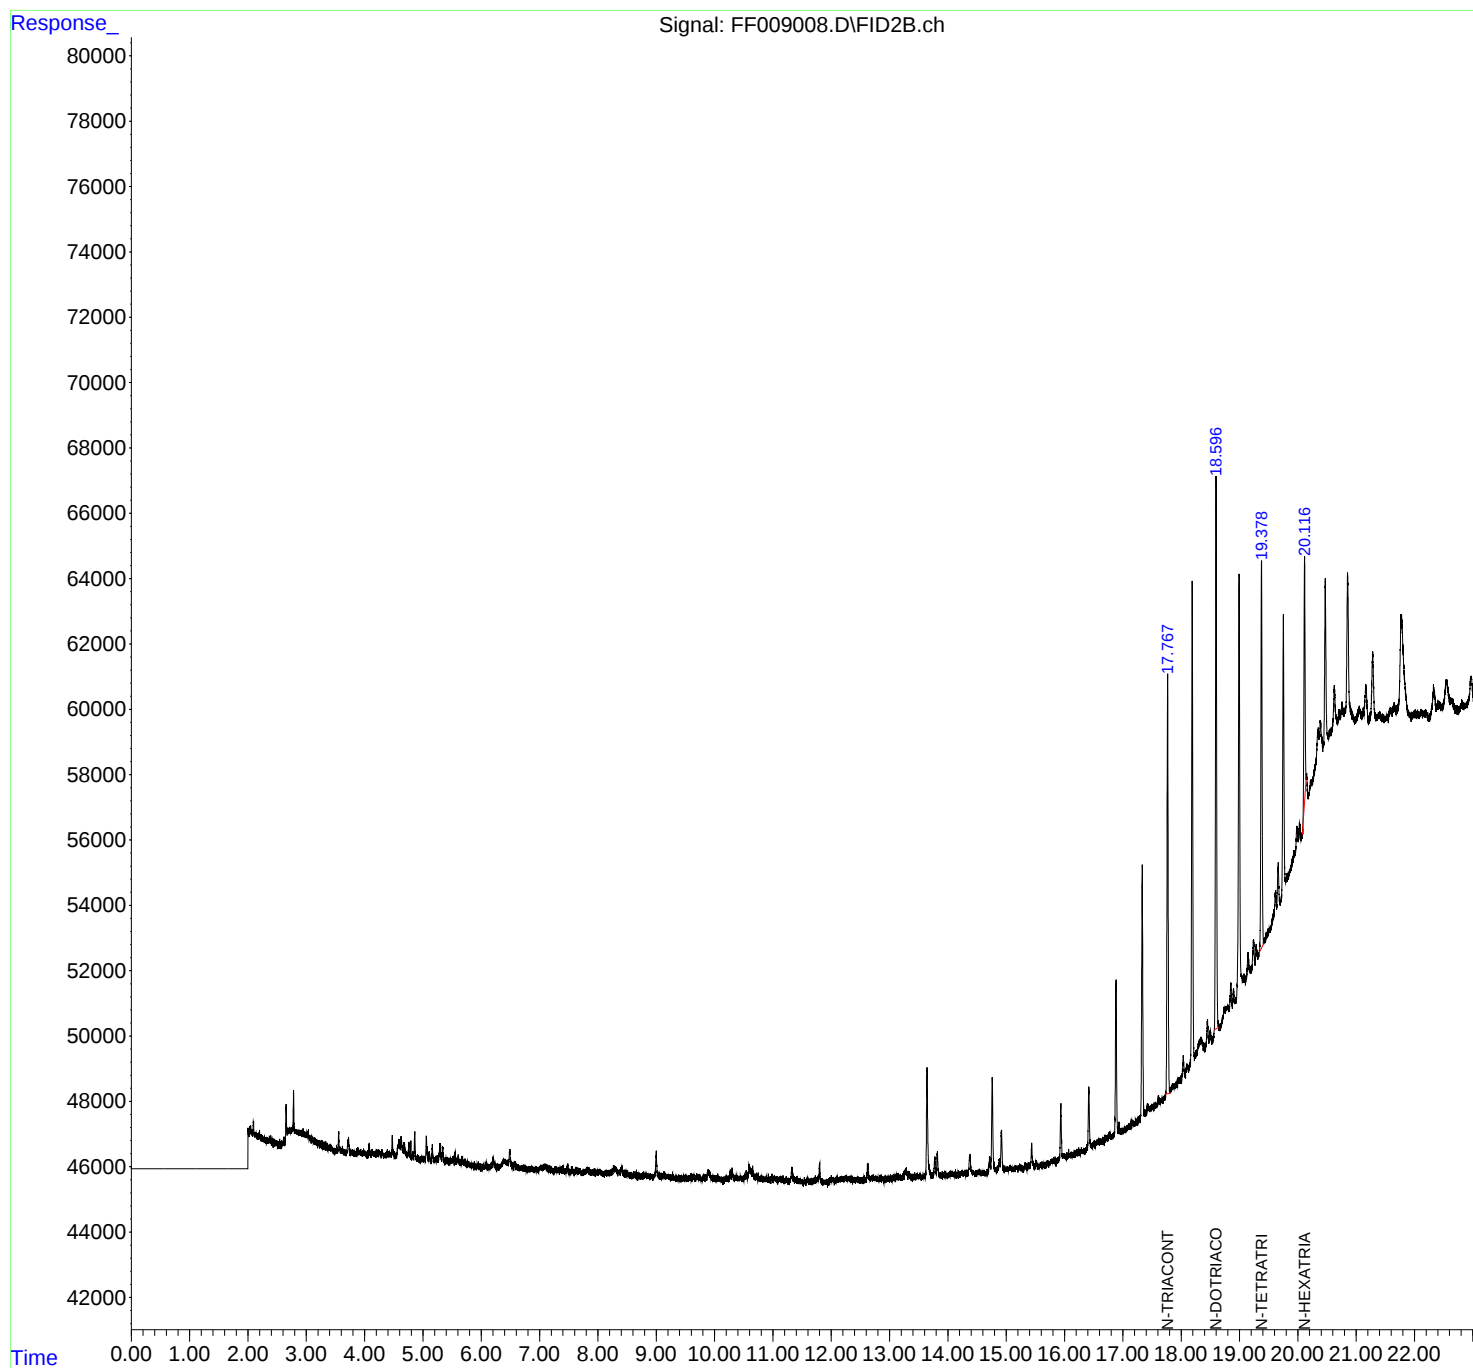


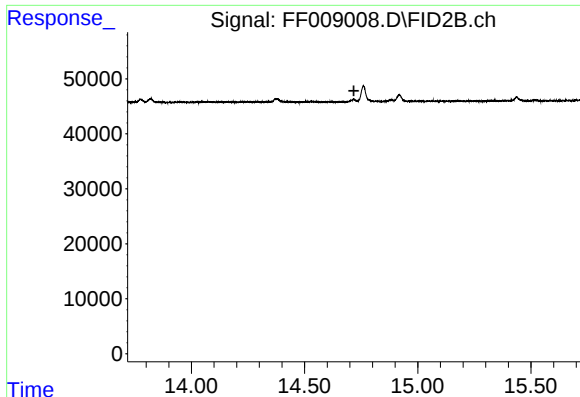

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.718 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

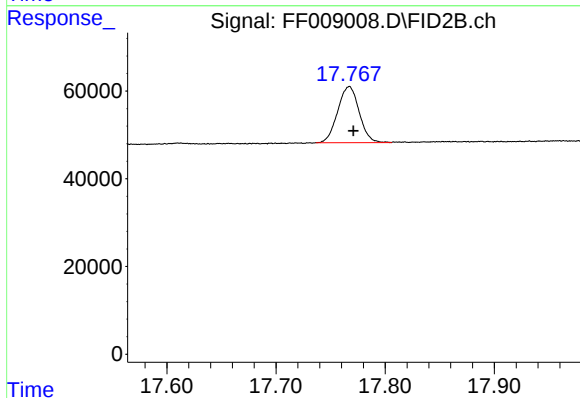


#13 N-TRIACONTANE

R.T.: 17.768 min
Delta R.T.: -0.003 min
Response: 174971
Conc: 1.50 ug/ml

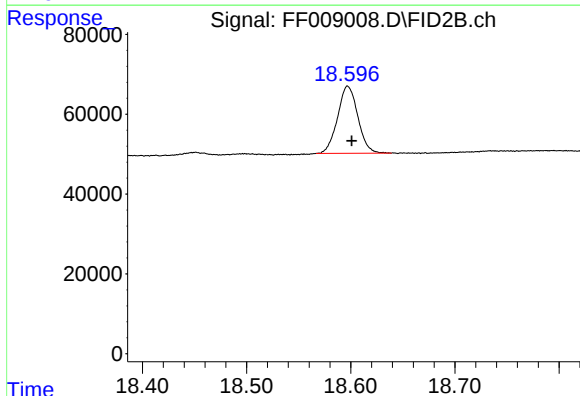


#14 N-DOTRIACONTANE

R.T.: 18.597 min
Delta R.T.: -0.004 min
Response: 227596
Conc: 2.11 ug/ml

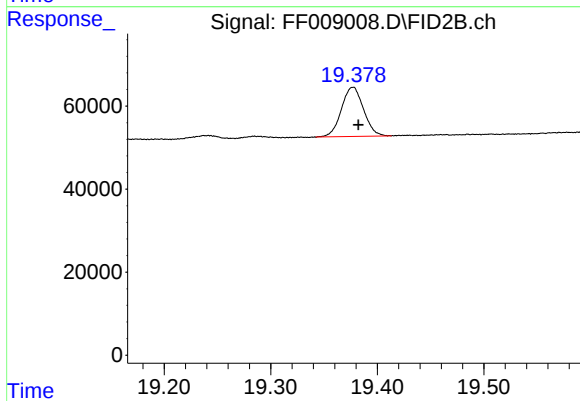

#15 N-TETRATRIACONTANE

R.T.: 19.378 min
Delta R.T.: -0.004 min
Response: 170650
Conc: 1.74 ug/ml

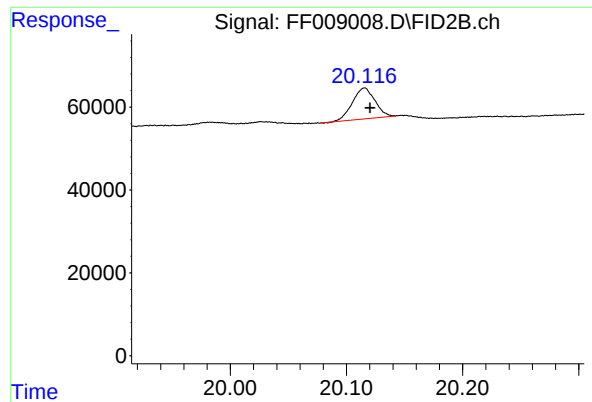

#16 N-HEXATRIACONTANE

R.T.: 20.116 min
Delta R.T.: -0.005 min
Response: 100530
Conc: 1.15 ug/ml

Instrument :
FID_F
ClientSampleId :