

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092421\
 Data File : FF009020.D
 Signal(s) : FID2B.ch
 Acq On : 24 Sep 2021 17:13
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 24 22:49:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
 Quant Title :
 QLast Update : Wed Sep 08 10:20:54 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13)	N-TRIACONTANE	17.775	128312	1.098 ug/ml
14)	N-DOTRIACONTANE	18.604	185194	1.716 ug/ml
15)	N-TETRATRIACONTANE	19.388	318376	3.250 ug/ml
16)	N-HEXATRIACONTANE	20.127	130834	1.497 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092421\
Data File : FF009020.D
Signal(s) : FID2B.ch
Acq On : 24 Sep 2021 17:13
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 24 22:49:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

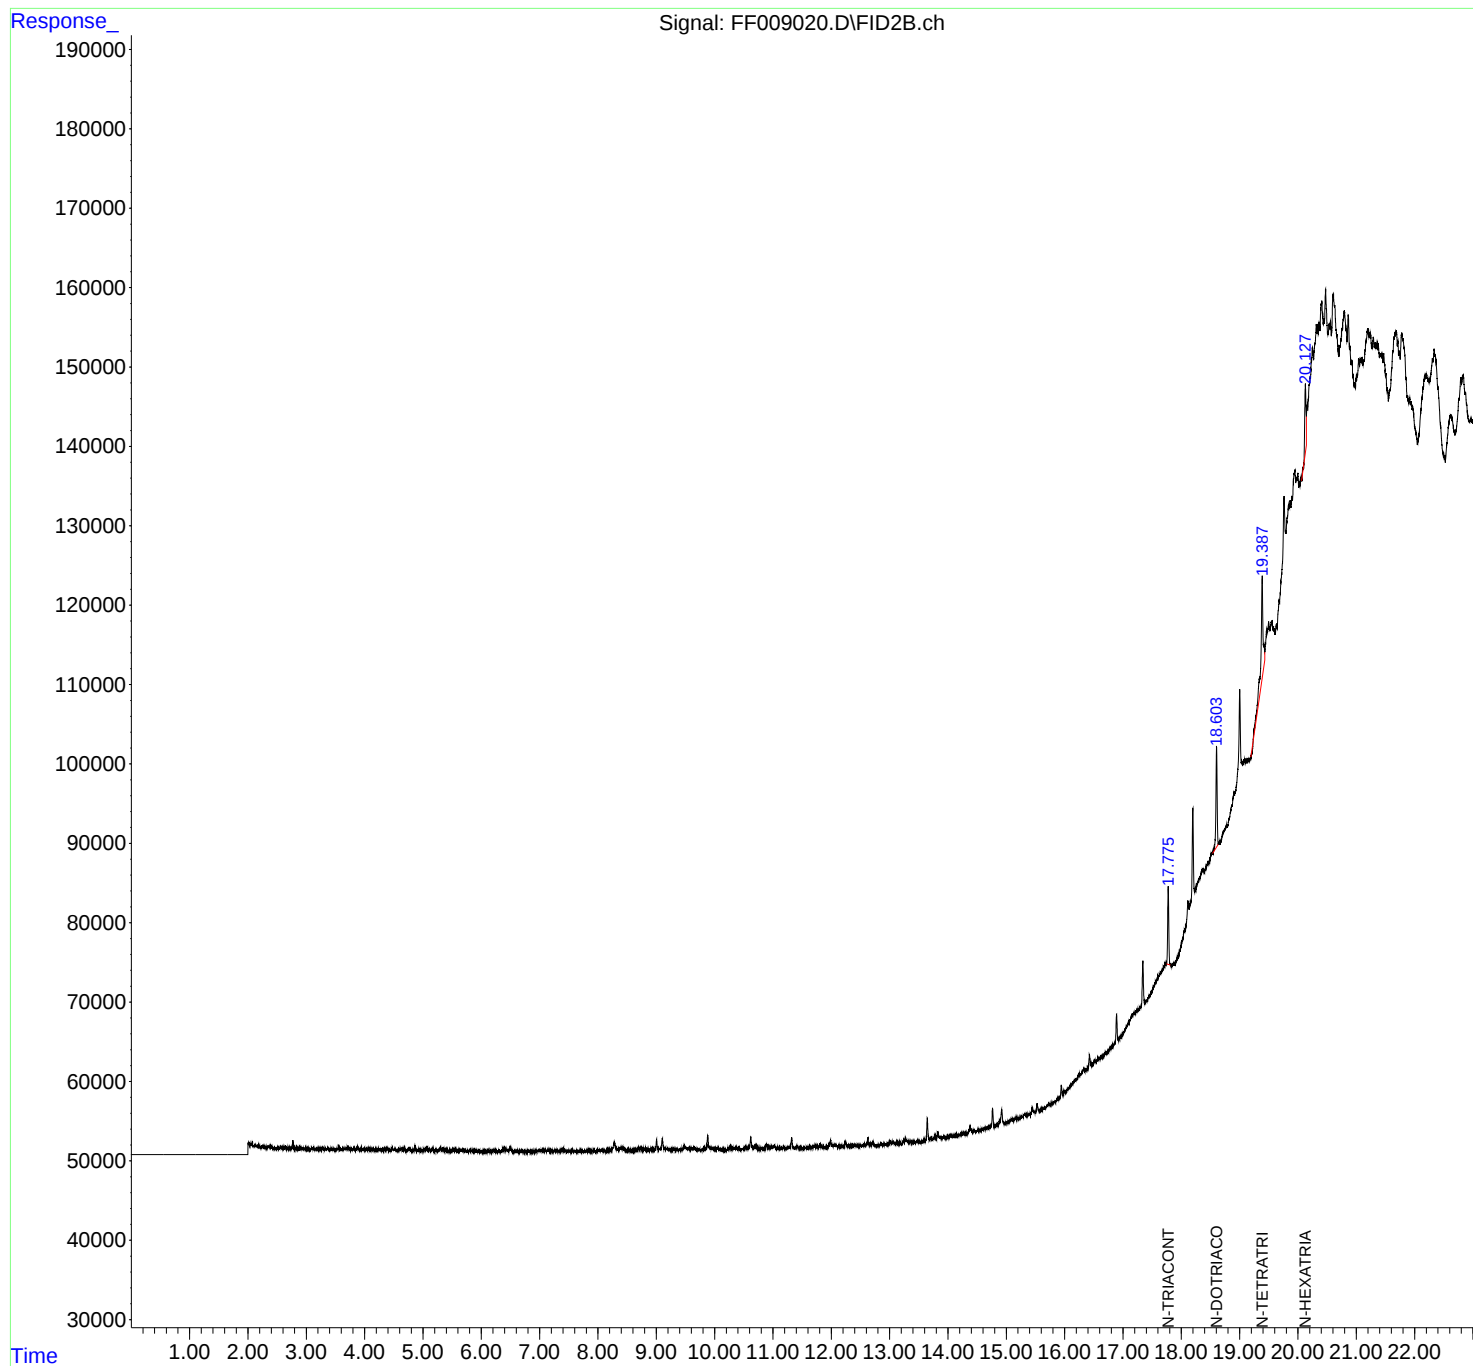


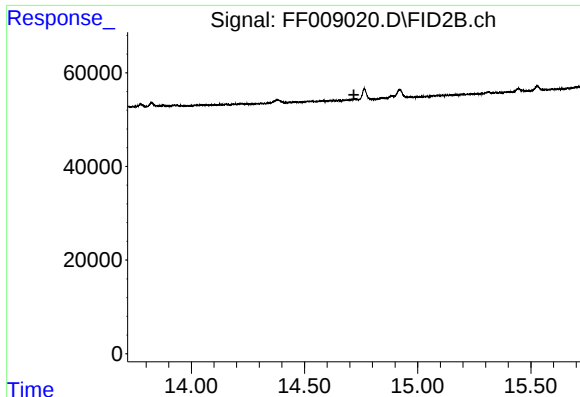

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.718 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

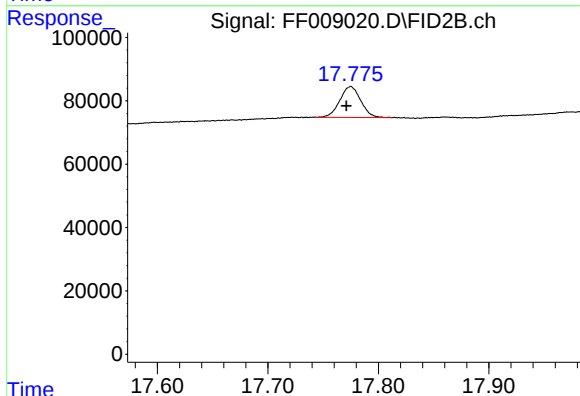


#13 N-TRIACONTANE

R.T.: 17.775 min
Delta R.T.: 0.004 min
Response: 128312
Conc: 1.10 ug/ml

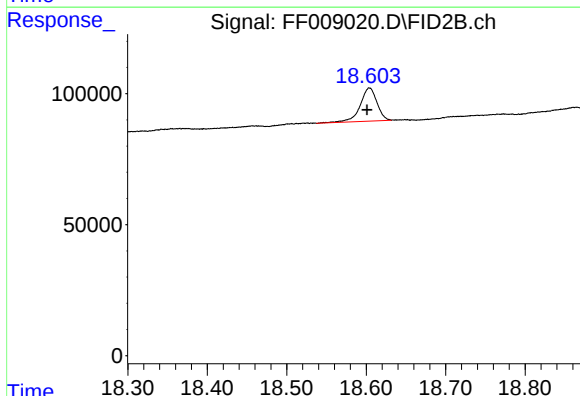


#14 N-DOTRIACONTANE

R.T.: 18.604 min
Delta R.T.: 0.003 min
Response: 185194
Conc: 1.72 ug/ml

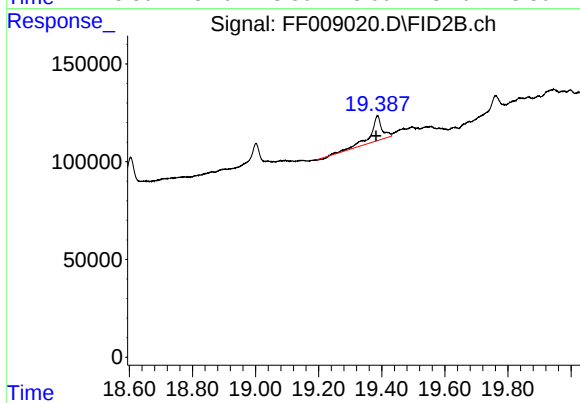

#15 N-TETRATRIACONTANE

R.T.: 19.388 min
Delta R.T.: 0.005 min
Response: 318376
Conc: 3.25 ug/ml

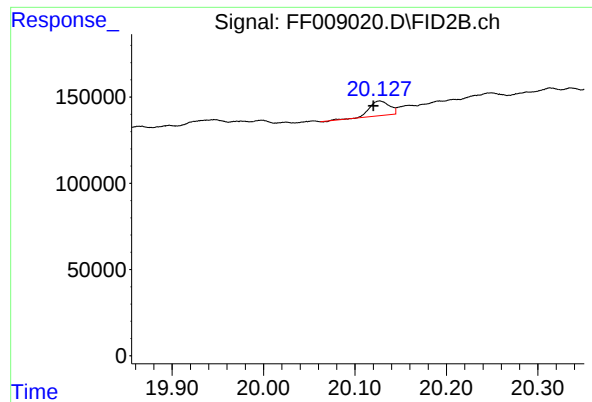

#16 N-HEXATRIACONTANE

R.T.: 20.127 min
Delta R.T.: 0.007 min
Response: 130834
Conc: 1.50 ug/ml

Instrument :
FID_F
ClientSampleId :