

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF092421\  
 Data File : FF009014.D  
 Signal(s) : FID2B.ch  
 Acq On : 24 Sep 2021 14:05  
 Operator : DD\AJ  
 Sample : M3872-01  
 Misc :  
 ALS Vial : 57 Sample Multiplier: 1

**Instrument :**  
 FID\_F  
**ClientSampleId :**  
 SP-LPA-01

**Manual Integrations**  
**APPROVED**  
 mohammad  
 9/27/2021 2:33:27 PM

Integration File: autoint1.e  
 Quant Time: Sep 24 22:48:06 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF090721.M  
 Quant Title :  
 QLast Update : Wed Sep 08 10:20:54 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.718	2147363	18.280 ug/mlm
Target Compounds			
-----			

(f)=RT Delta > 1/2 Window (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF092421\  
 Data File : FF009014.D  
 Signal(s) : FID2B.ch  
 Acq On : 24 Sep 2021 14:05  
 Operator : DD\AJ  
 Sample : M3872-01  
 Misc :  
 ALS Vial : 57 Sample Multiplier: 1


Instrument :  
 FID\_F  
 ClientSampleId :  
 SP-LPA-01


Manual Integrations  
 APPROVED

mohammad  
 9/27/2021 2:33:27 PM

Integration File: autoint1.e  
 Quant Time: Sep 24 22:48:06 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF090721.M  
 Quant Title :  
 QLast Update : Wed Sep 08 10:20:54 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

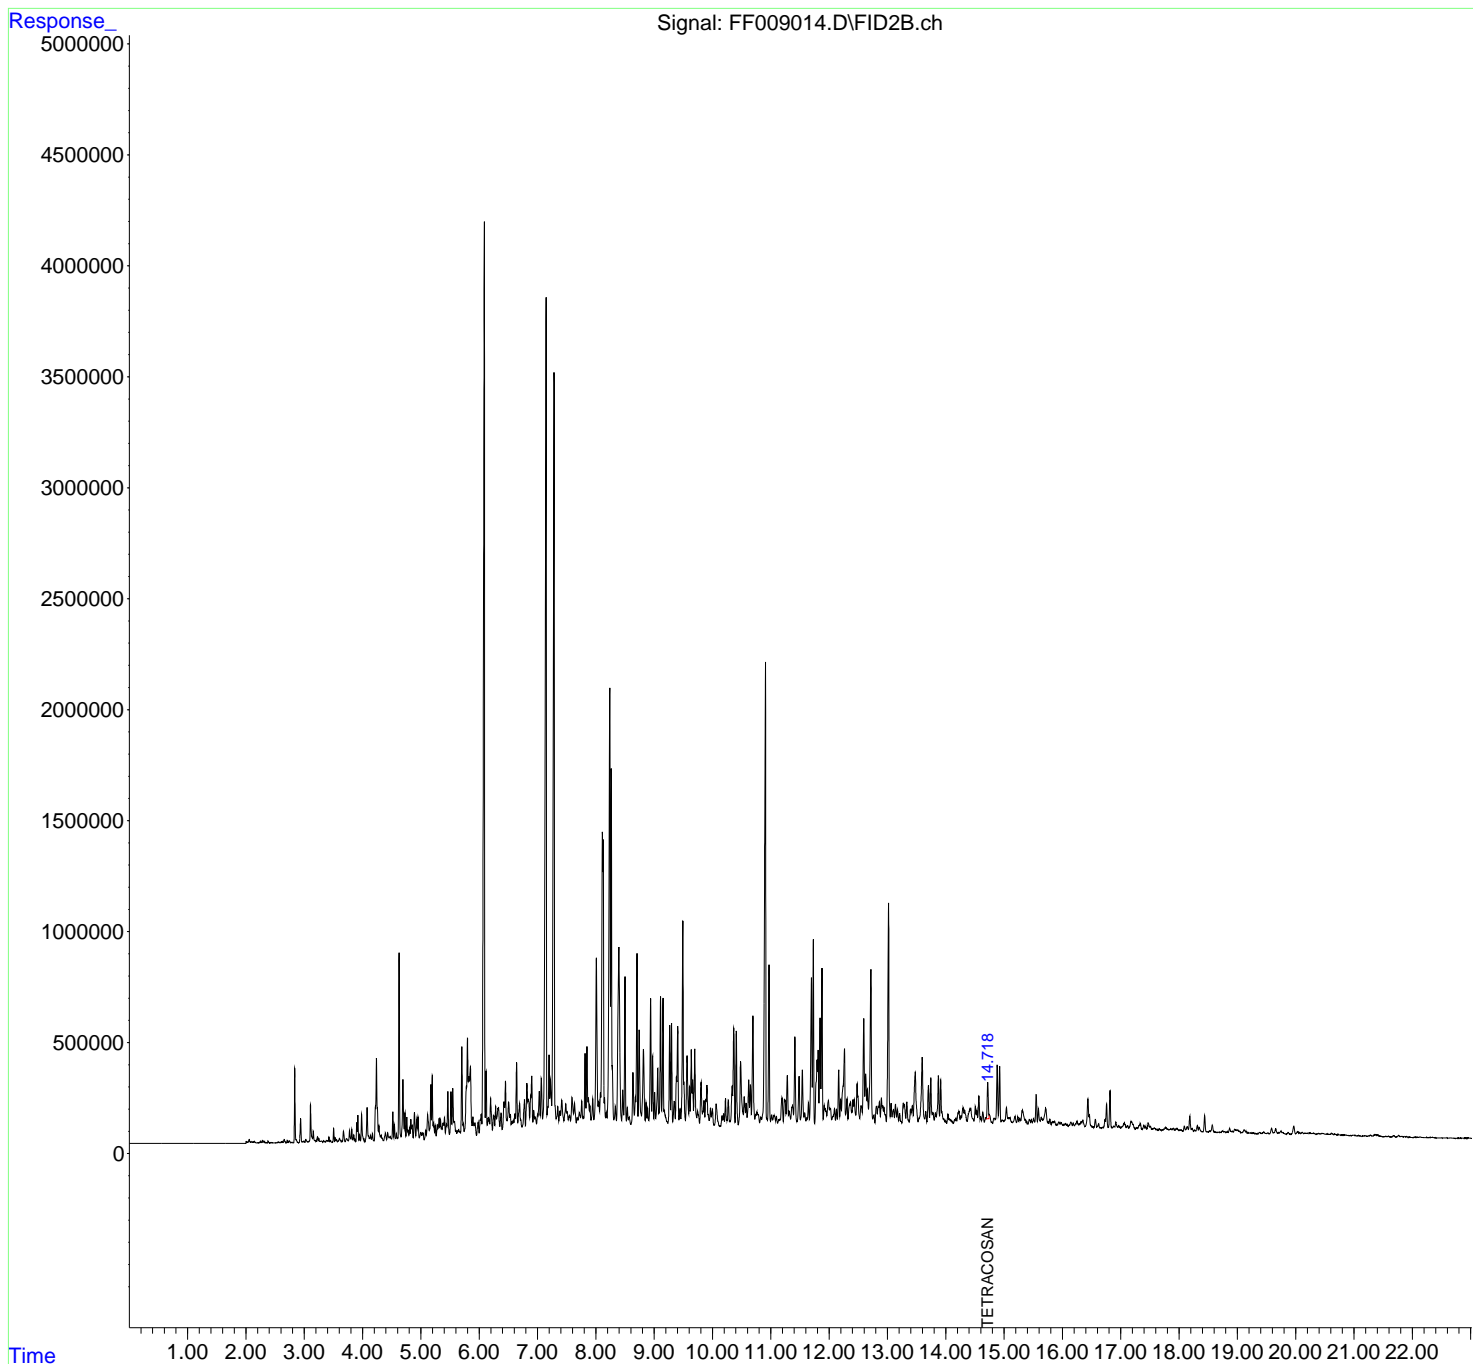

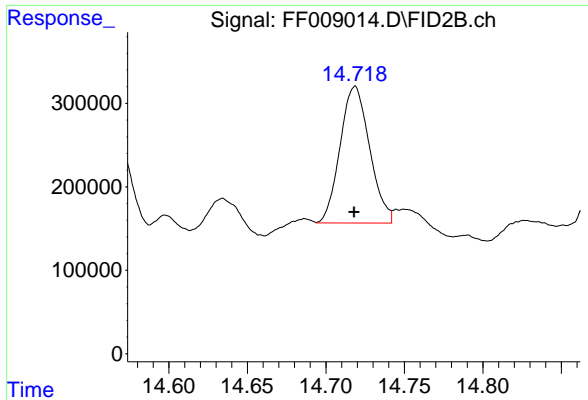

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.718 min  
Delta R.T.: 0.000 min  
Response: 2147363  
Conc: 18.28 ug/ml m

Instrument :  
FID\_F  
ClientSampled :  
SP-LPA-01

Manual Integrations  
APPROVED

mohammad  
9/27/2021 2:33:27 PM