

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092518\
Data File : FF002224.D
Signal(s) : FID2B.ch
Acq On : 25 Sep 2018 13:14
Operator : AJ\SJ
Sample : J4770-17 25X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 26 03:38:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
5)	N-HEXADECANE	9.440	117469	0.858 ug/ml
6)	N-OCTADECANE	10.873	157724	1.125 ug/ml
7)	N-EICOSANE	12.176	185770	1.303 ug/ml
8)	N-DOCOSANE	13.370	225136	1.580 ug/ml
10)	N-TETRACOSANE	14.469	418779	2.951 ug/ml
11)	N-HEXACOSANE	15.486	385403	2.710 ug/ml
12)	N-OCTACOSANE	16.434	304177	2.120 ug/ml
13)	N-TRIACONTANE	17.319	315235	2.174 ug/ml
14)	N-DOTRIACONTANE	18.149	279510	1.983 ug/ml
15)	N-TETRATRIACONTANE	18.931	186323	1.386 ug/ml
16)	N-HEXATRIACONTANE	19.673	66049	0.530 ug/ml
17)	N-OCTATRIACONTANE	20.375	94909	0.867 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092518\
Data File : FF002224.D
Signal(s) : FID2B.ch
Acq On : 25 Sep 2018 13:14
Operator : AJ\SJ
Sample : J4770-17 25X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 26 03:38:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

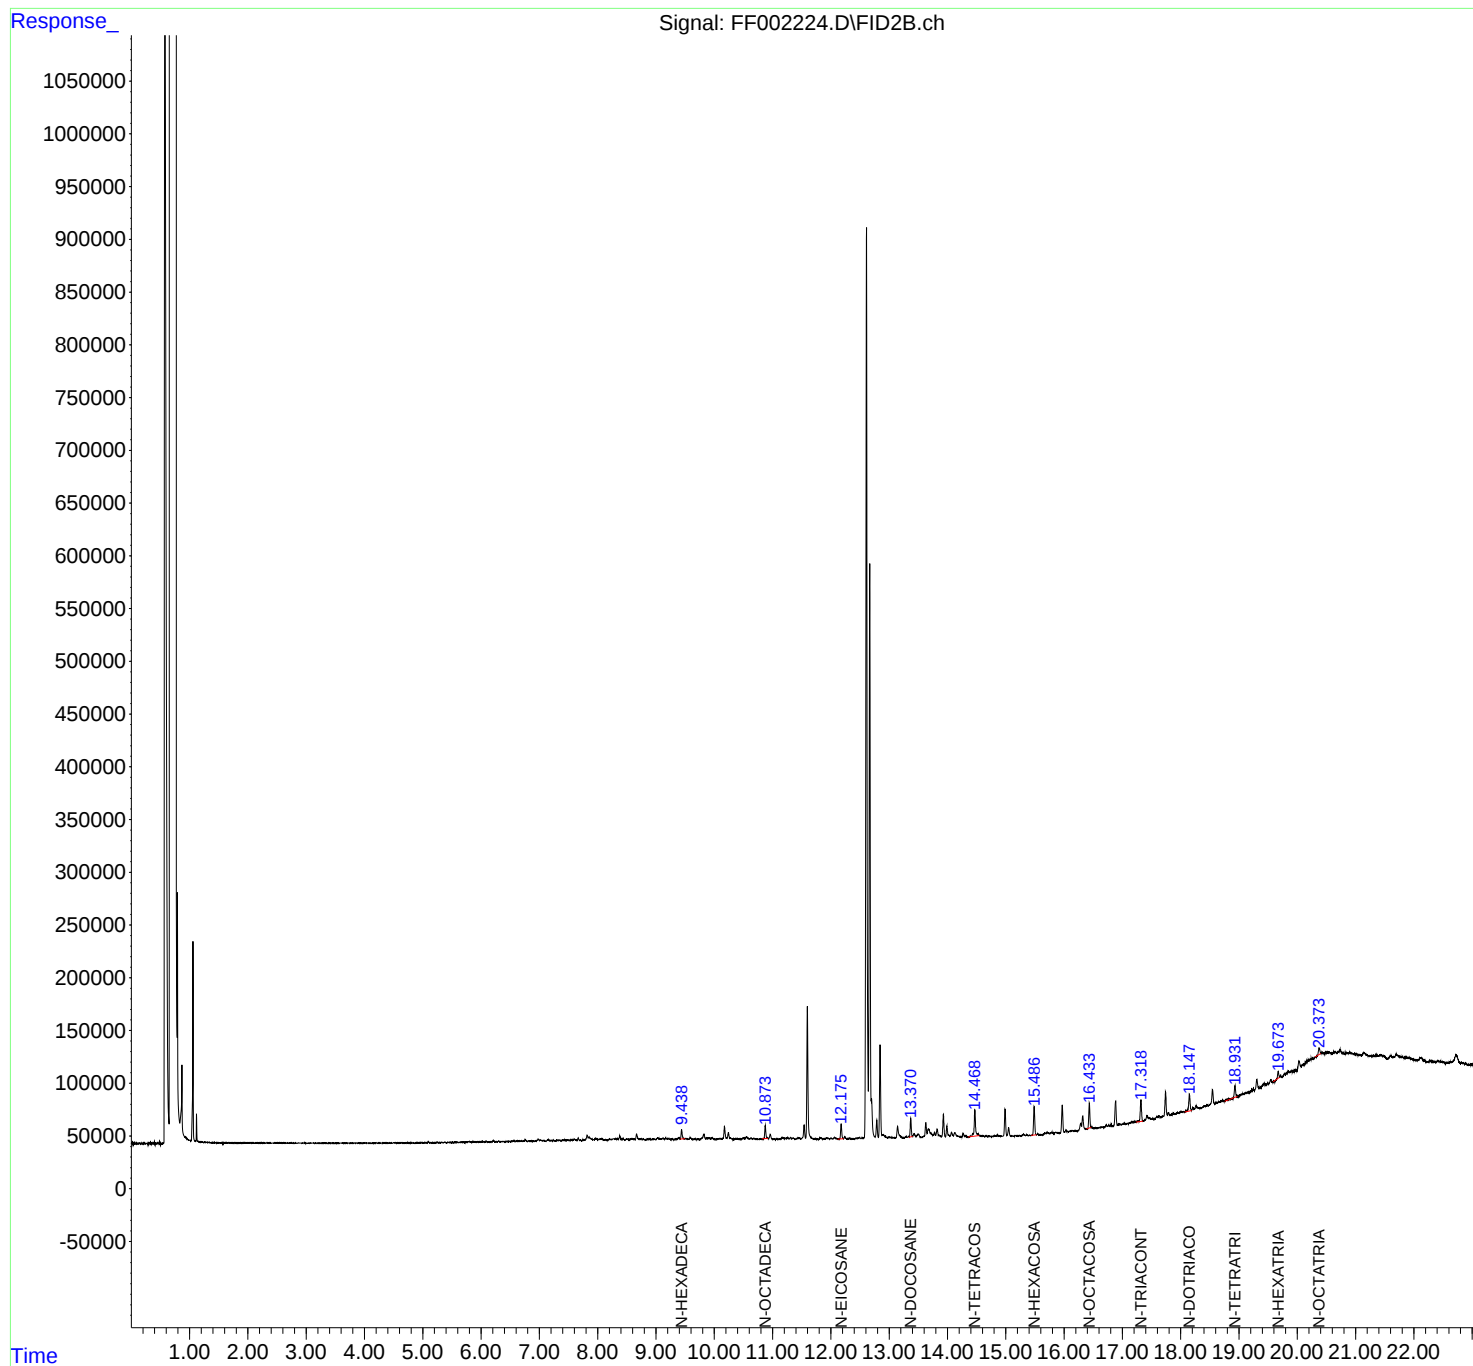

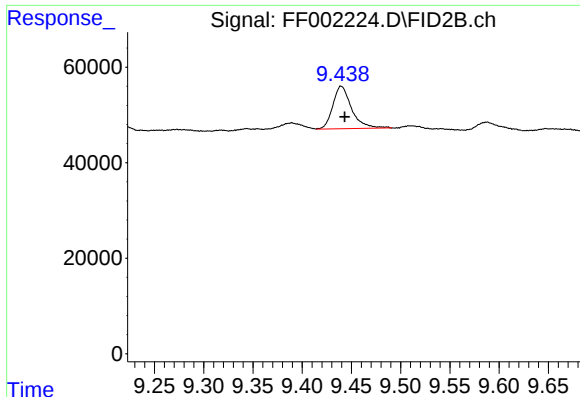


#5 N-HEXADECANE

R.T.: 9.440 min
Delta R.T.: -0.004 min
Response: 117469
Conc: 0.86 ug/ml

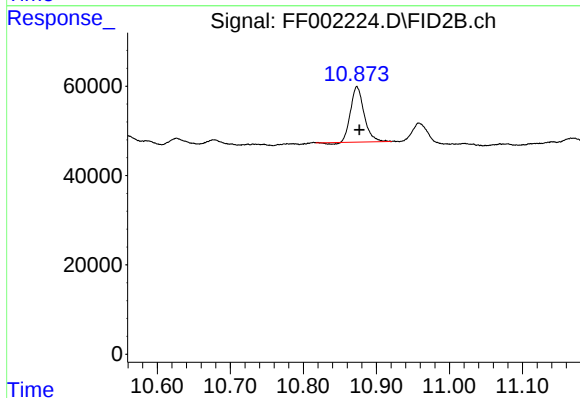


#6 N-OCTADECANE

R.T.: 10.873 min
Delta R.T.: -0.003 min
Response: 157724
Conc: 1.12 ug/ml

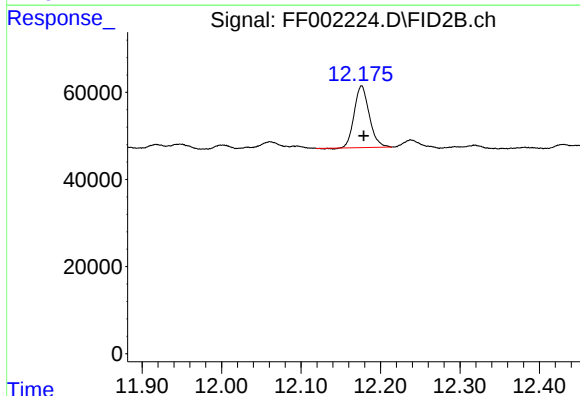


#7 N-EICOSANE

R.T.: 12.176 min
Delta R.T.: -0.002 min
Response: 185770
Conc: 1.30 ug/ml

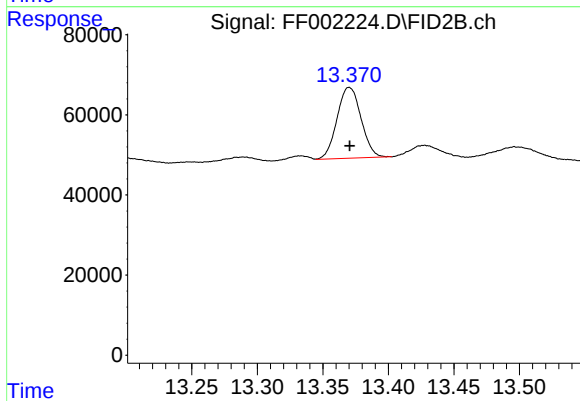


#8 N-DOCOSANE

R.T.: 13.370 min
Delta R.T.: 0.000 min
Response: 225136
Conc: 1.58 ug/ml

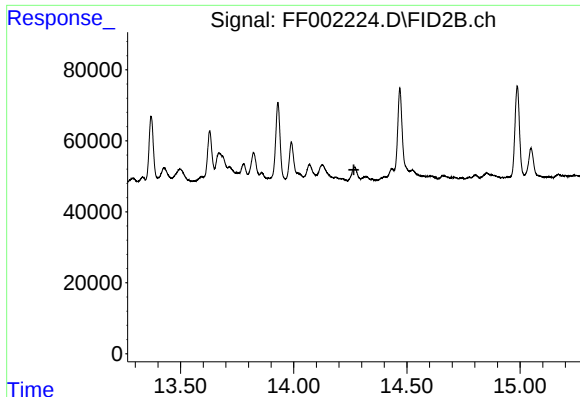


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.266 min
Response: 0
Conc: N.D.

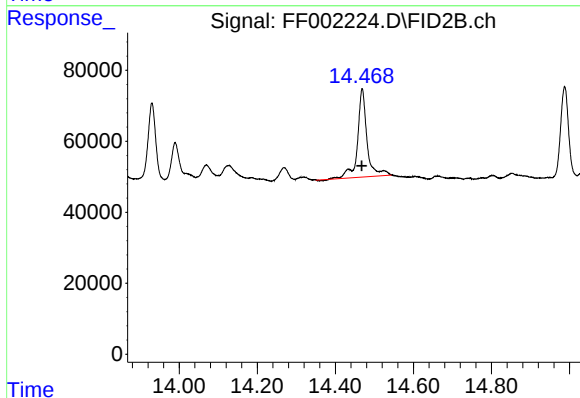


#10 N-TETRACOSANE

R.T.: 14.469 min
Delta R.T.: 0.000 min
Response: 418779
Conc: 2.95 ug/ml

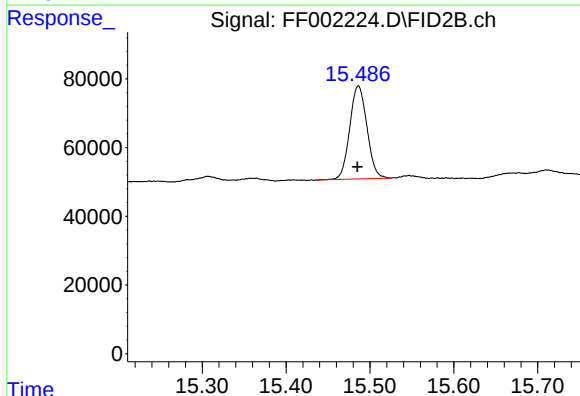


#11 N-HEXACOSANE

R.T.: 15.486 min
Delta R.T.: 0.001 min
Response: 385403
Conc: 2.71 ug/ml

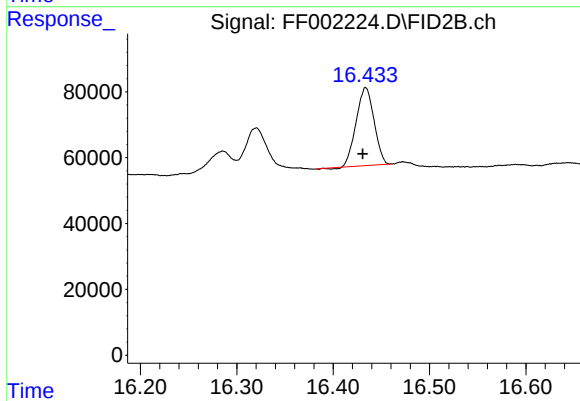


#12 N-OCTACOSANE

R.T.: 16.434 min
Delta R.T.: 0.003 min
Response: 304177
Conc: 2.12 ug/ml

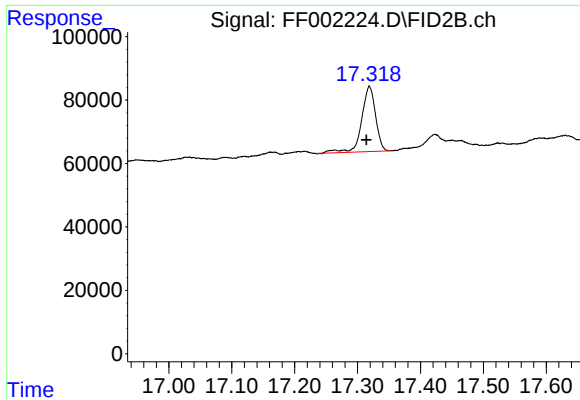


#13 N-TRIACONTANE

R.T.: 17.319 min
Delta R.T.: 0.005 min
Response: 315235
Conc: 2.17 ug/ml

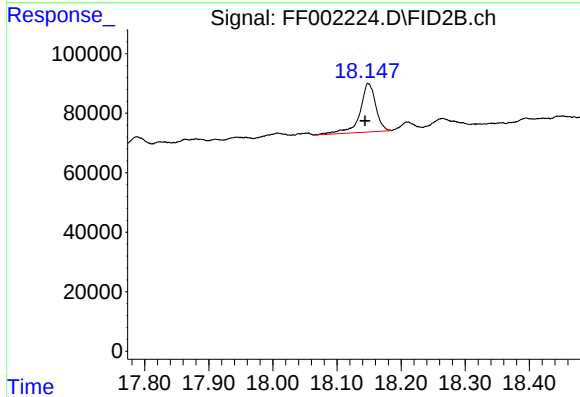


#14 N-DOTRIACONTANE

R.T.: 18.149 min
Delta R.T.: 0.005 min
Response: 279510
Conc: 1.98 ug/ml

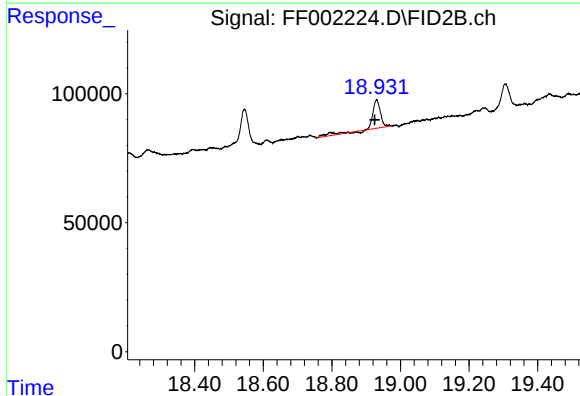


#15 N-TETRATRIACONTANE

R.T.: 18.931 min
Delta R.T.: 0.006 min
Response: 186323
Conc: 1.39 ug/ml

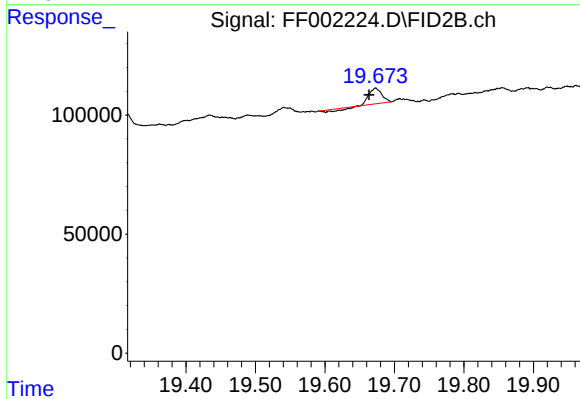

#16 N-HEXATRIACONTANE

R.T.: 19.673 min
Delta R.T.: 0.010 min
Response: 66049
Conc: 0.53 ug/ml

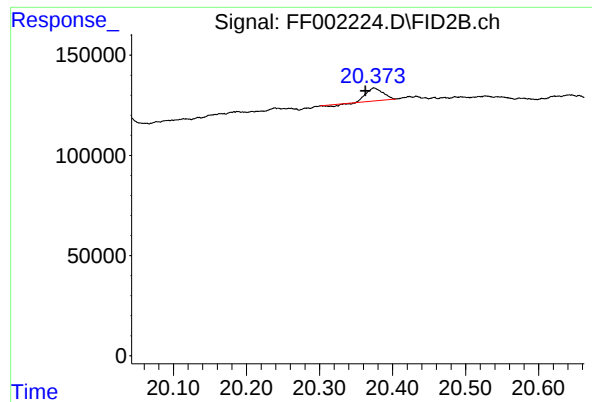

#17 N-OCTATRIACONTANE

R.T.: 20.375 min
Delta R.T.: 0.012 min
Response: 94909
Conc: 0.87 ug/ml