

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092518\
 Data File : FF002232.D
 Signal(s) : FID2B.ch
 Acq On : 25 Sep 2018 17:22
 Operator : AJ\SJ
 Sample : J4779-09 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 26 03:39:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:20:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.266	133431	1.065 ug/ml
Target Compounds			
3) N-DODECANE	6.084	421219	3.366 ug/ml
4) N-TETRADECANE	7.892	1297732	9.794 ug/ml
5) N-HEXADECANE	9.437	1532558	11.190 ug/ml
6) N-OCTADECANE	10.863	673708	4.804 ug/ml
7) N-EICOSANE	12.174	435495	3.055 ug/ml
10) N-TETRACOSANE	14.452	357445	2.519 ug/ml
12) N-OCTACOSANE	16.416	580781	4.048 ug/ml
13) N-TRIACONTANE	17.317	124877	0.861 ug/ml
14) N-DOTRIACONTANE	18.148	171268	1.215 ug/ml
15) N-TETRATRIACONTANE	18.929	270609	2.012 ug/ml
16) N-HEXATRIACONTANE	19.672	228783	1.837 ug/ml
17) N-OCTATRIACONTANE	20.371	135514	1.238 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092518\
Data File : FF002232.D
Signal(s) : FID2B.ch
Acq On : 25 Sep 2018 17:22
Operator : AJ\SJ
Sample : J4779-09 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 26 03:39:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

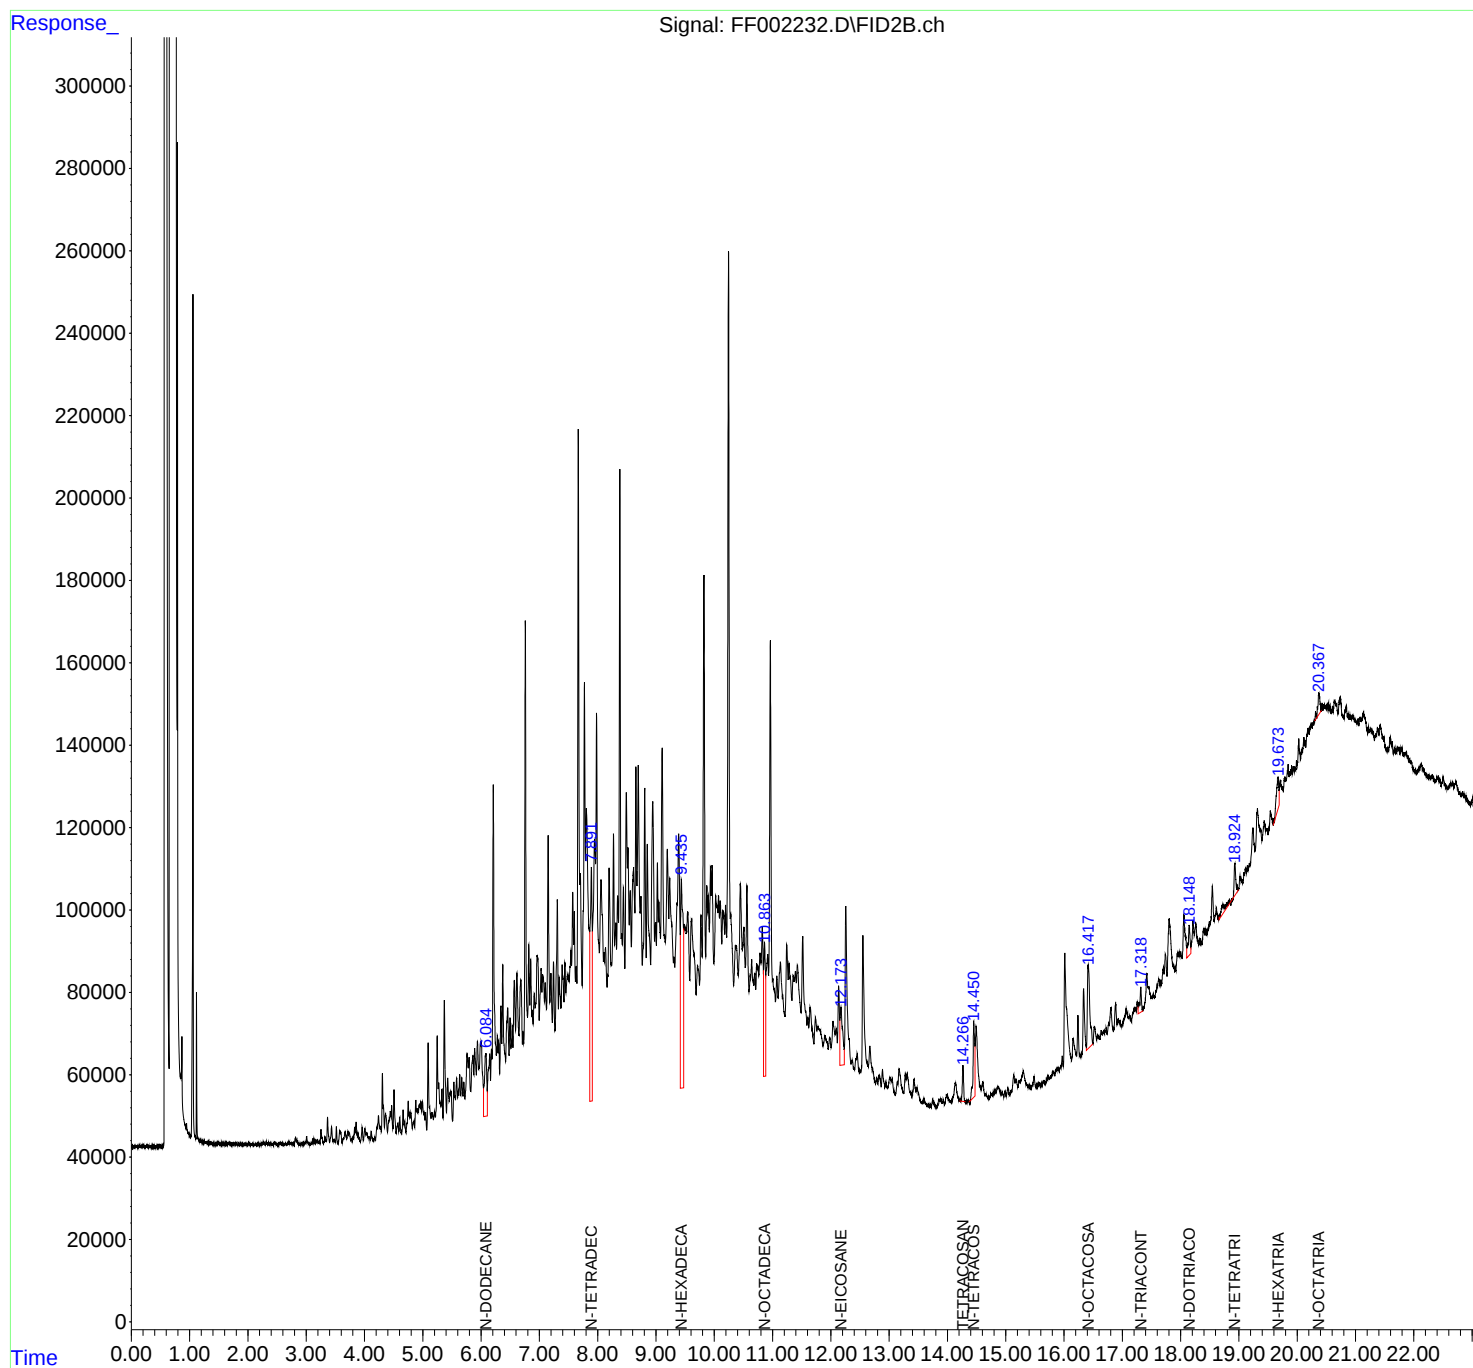

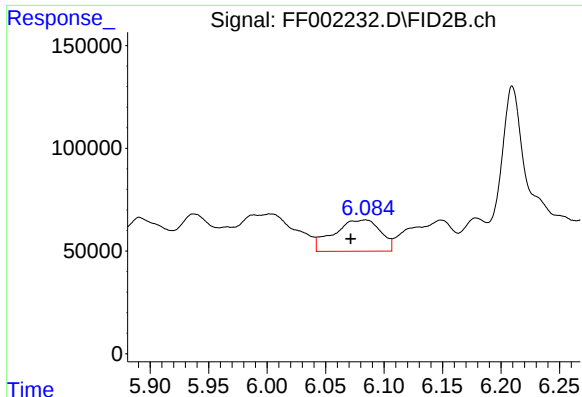


#3 N-DODECANE

R.T.: 6.084 min
Delta R.T.: 0.013 min
Response: 421219
Conc: 3.37 ug/ml

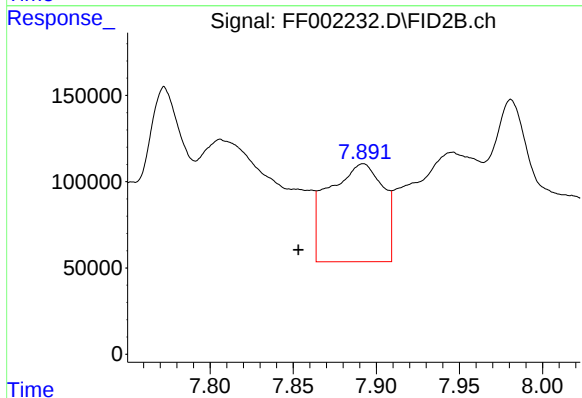


#4 N-TETRADECANE

R.T.: 7.892 min
Delta R.T.: 0.039 min
Response: 1297732
Conc: 9.79 ug/ml

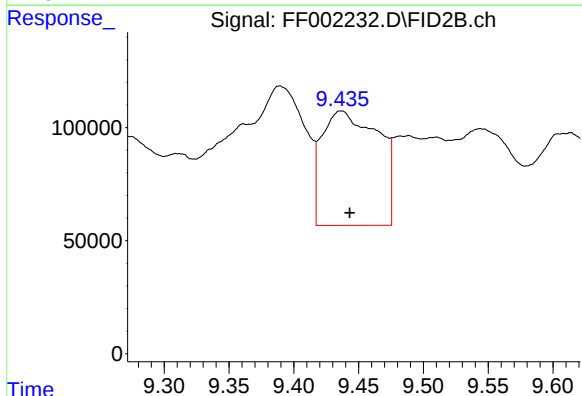


#5 N-HEXADECANE

R.T.: 9.437 min
Delta R.T.: -0.007 min
Response: 1532558
Conc: 11.19 ug/ml

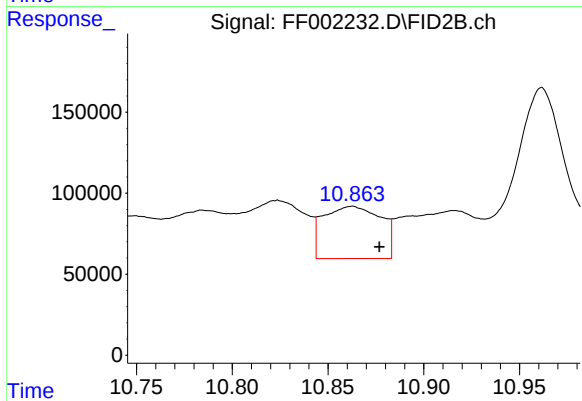


#6 N-OCTADECANE

R.T.: 10.863 min
Delta R.T.: -0.014 min
Response: 673708
Conc: 4.80 ug/ml

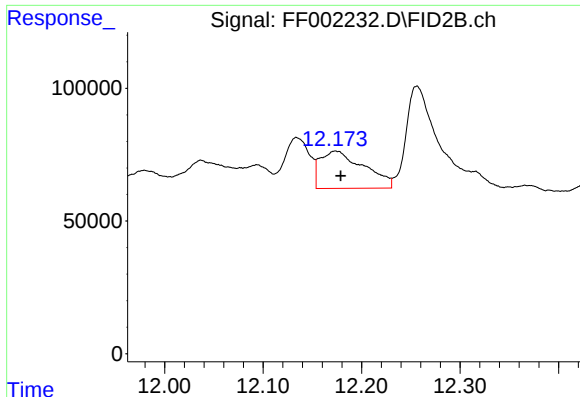


#7 N-EICOSANE

R.T.: 12.174 min
Delta R.T.: -0.005 min
Response: 435495
Conc: 3.06 ug/ml

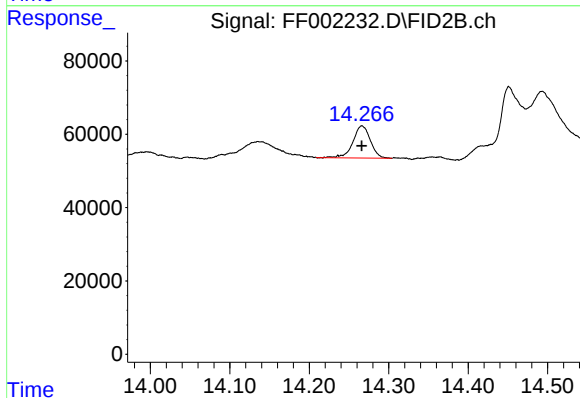


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.266 min
Delta R.T.: 0.000 min
Response: 133431
Conc: 1.06 ug/ml

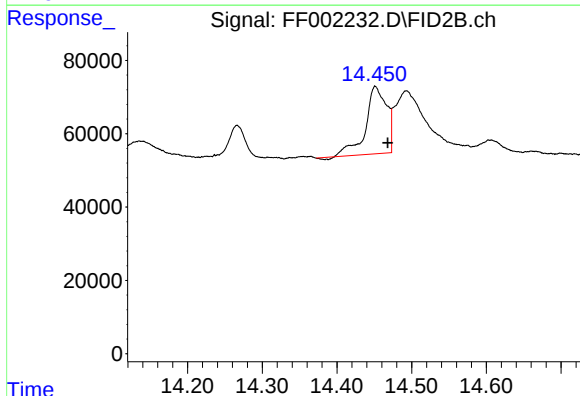


#10 N-TETRACOSANE

R.T.: 14.452 min
Delta R.T.: -0.016 min
Response: 357445
Conc: 2.52 ug/ml

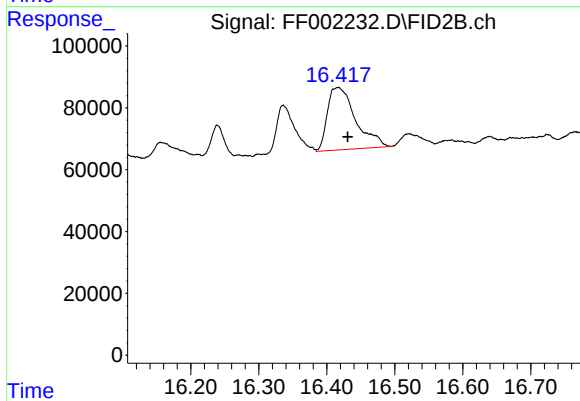


#12 N-OCTACOSANE

R.T.: 16.416 min
Delta R.T.: -0.015 min
Response: 580781
Conc: 4.05 ug/ml

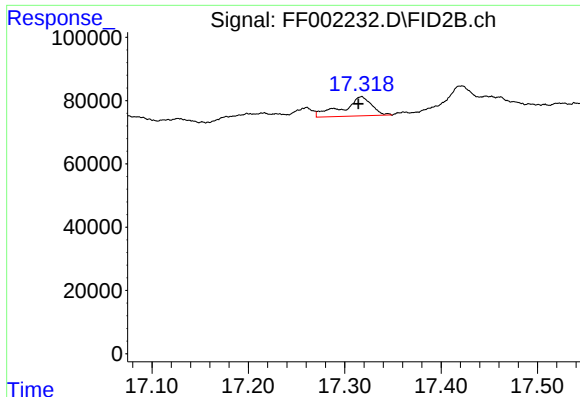


#13 N-TRIACONTANE

R.T.: 17.317 min
Delta R.T.: 0.003 min
Response: 124877
Conc: 0.86 ug/ml

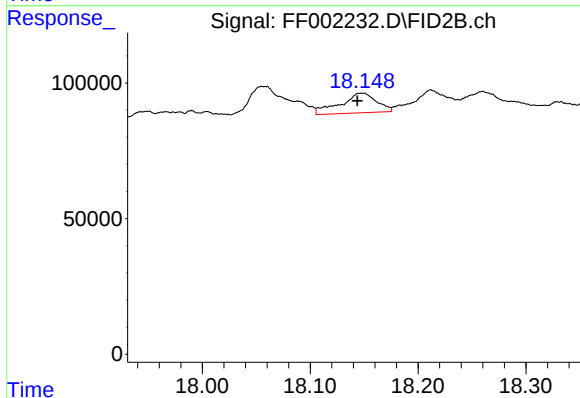


#14 N-DOTRIACONTANE

R.T.: 18.148 min
Delta R.T.: 0.004 min
Response: 171268
Conc: 1.21 ug/ml

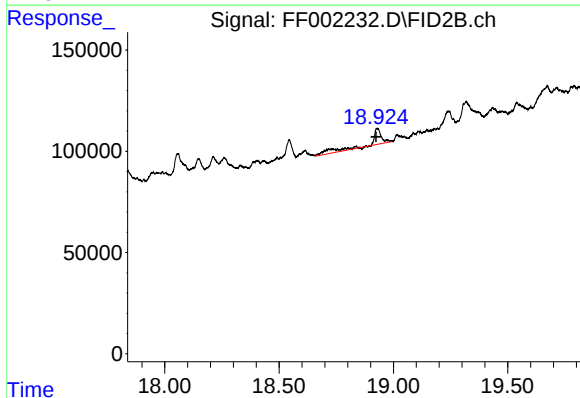


#15 N-TETRATRIACONTANE

R.T.: 18.929 min
Delta R.T.: 0.005 min
Response: 270609
Conc: 2.01 ug/ml

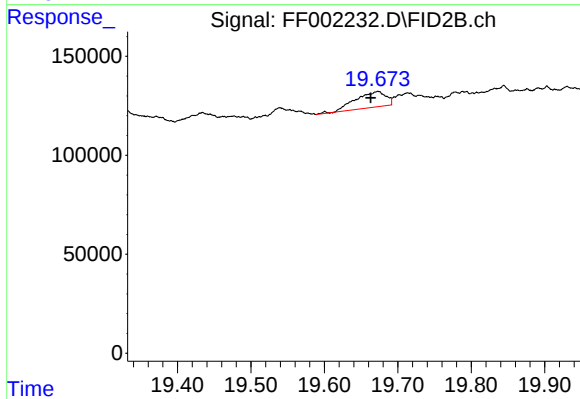

#16 N-HEXATRIACONTANE

R.T.: 19.672 min
Delta R.T.: 0.009 min
Response: 228783
Conc: 1.84 ug/ml

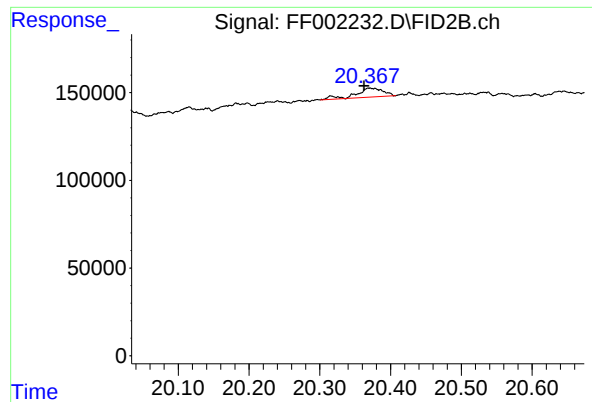

#17 N-OCTATRIACONTANE

R.T.: 20.371 min
Delta R.T.: 0.008 min
Response: 135514
Conc: 1.24 ug/ml