

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092525AR\
 Data File : FF016465.D
 Signal(s) : FID2B.ch
 Acq On : 26 Sep 2025 10:10
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 26 23:13:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aromatic EPH 092425.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 24 16:24:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
19) T	Indeno[1,2,3-cd]pyren...	18.569	67092 0.588 ug/ml
20) T	Dibenz[a,h]anthracene...	18.569	67092 0.514 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092525AR\
Data File : FF016465.D
Signal(s) : FID2B.ch
Acq On : 26 Sep 2025 10:10
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 26 23:13:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aromatic EPH 092425.M
Quant Title : GC Extractables
QLast Update : Wed Sep 24 16:24:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

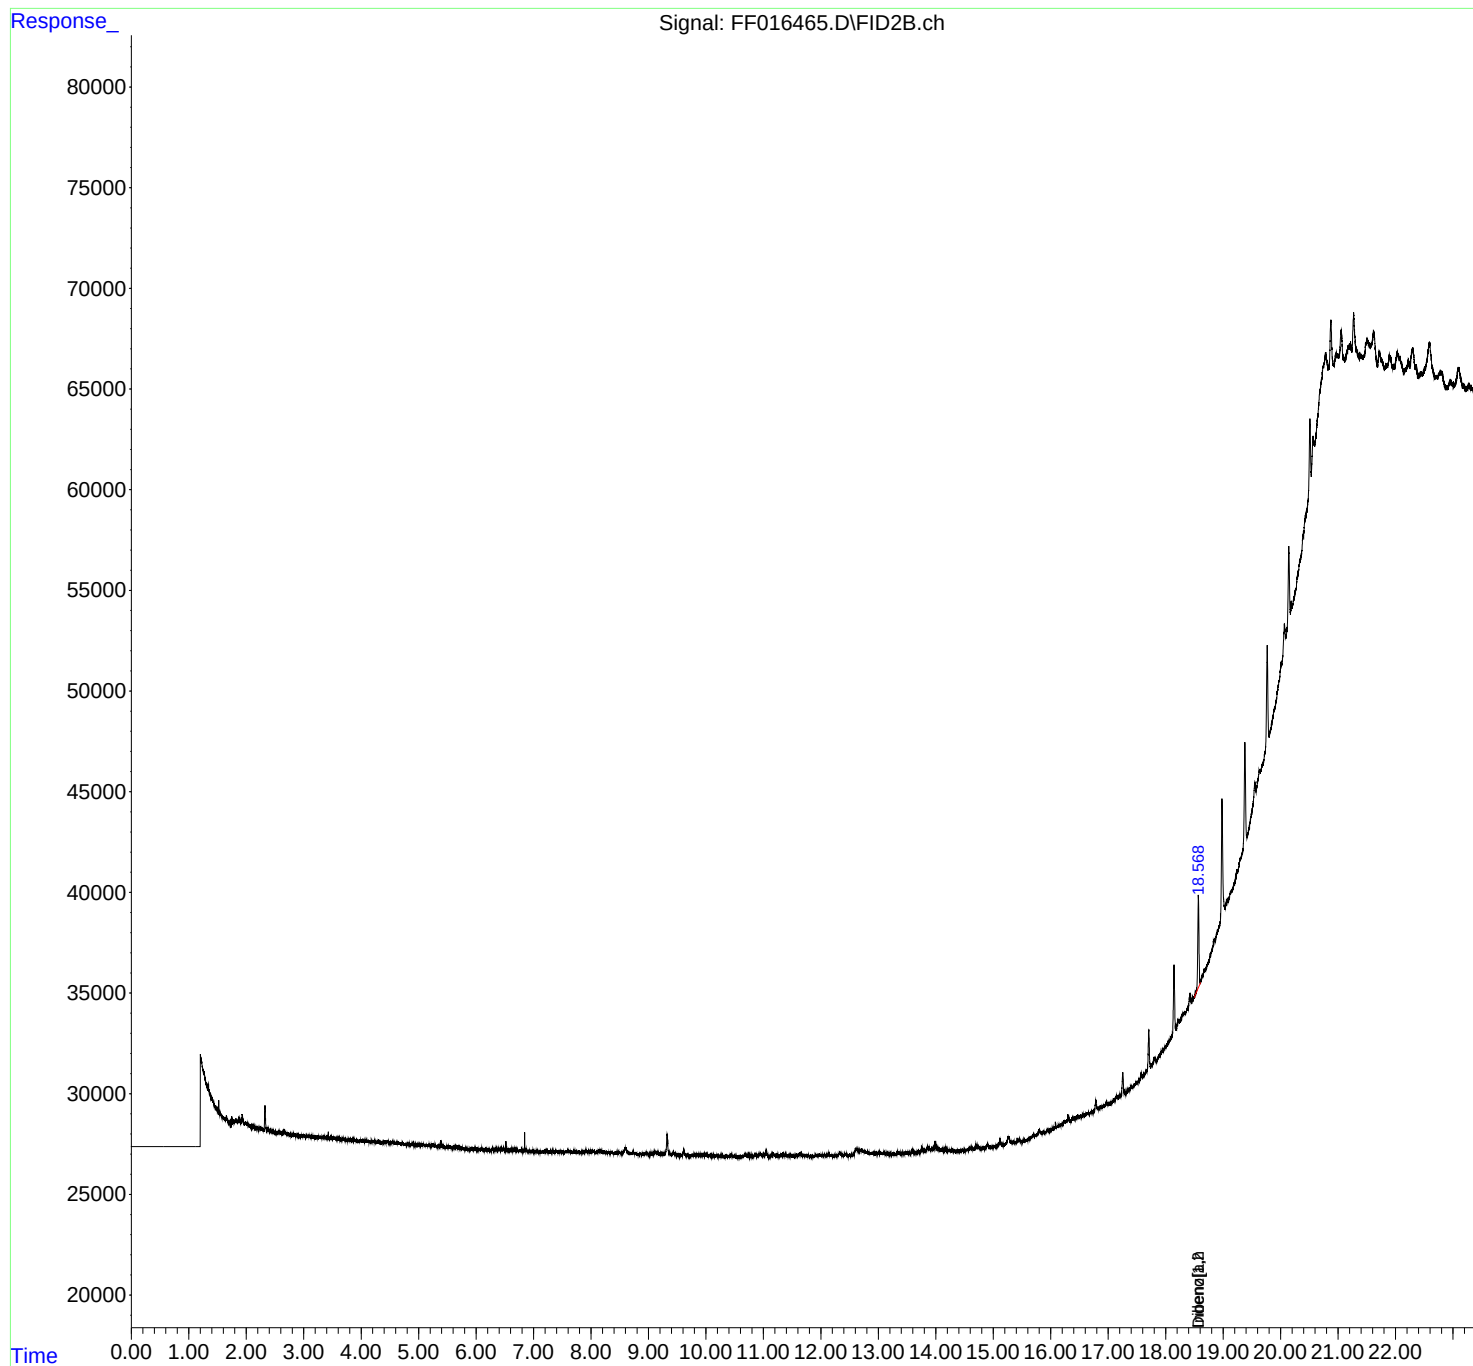


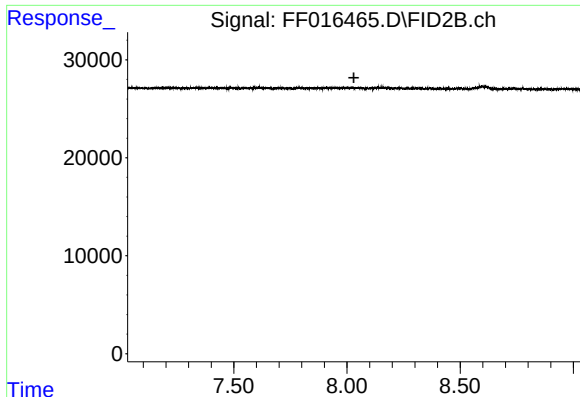

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 8.031 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

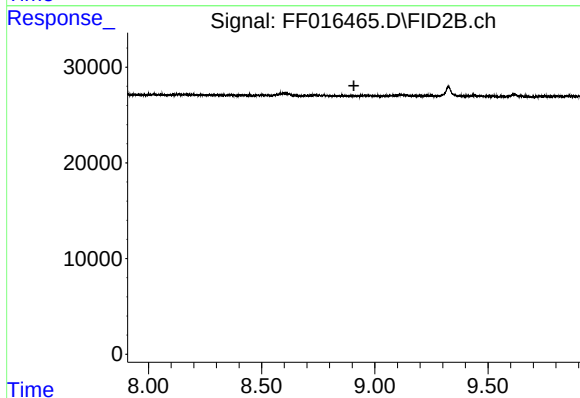


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.908 min
Response: 0
Conc: N.D.

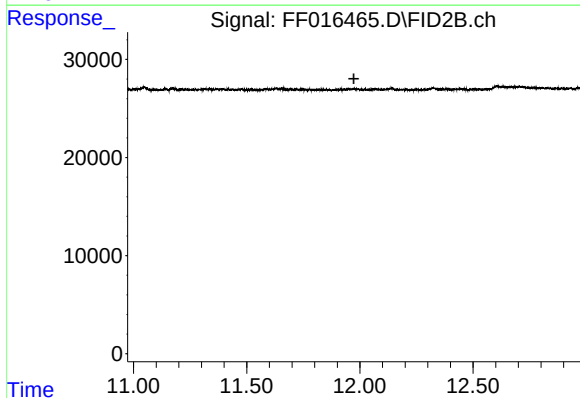


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.974 min
Response: 0
Conc: N.D.

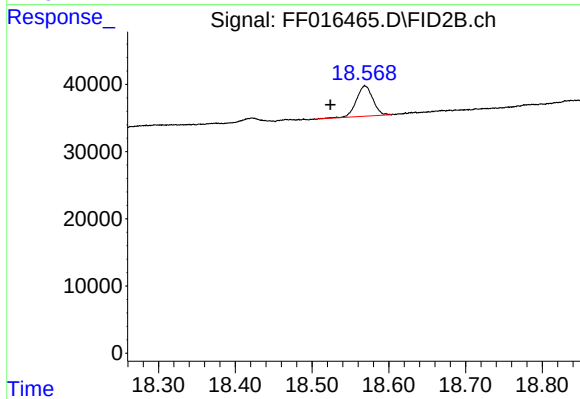

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.569 min
Delta R.T.: 0.045 min
Response: 67092
Conc: 0.59 ug/ml

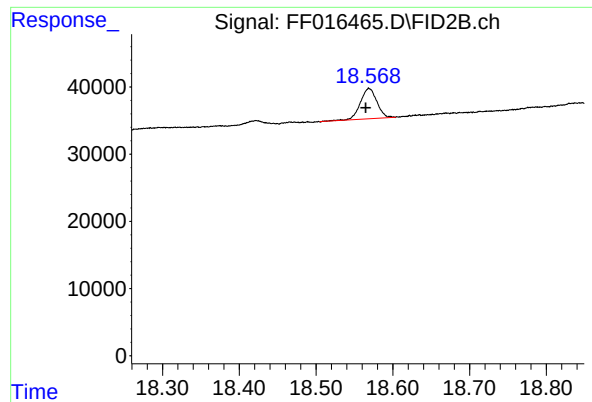

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.569 min
Delta R.T.: 0.004 min
Response: 67092
Conc: 0.51 ug/ml

Instrument :

FID_F

ClientSampleId :