

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092618\
 Data File : FF002241.D
 Signal(s) : FID2B.ch
 Acq On : 26 Sep 2018 11:56
 Operator : AJ\SJ
 Sample : J4779-07RE 10X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 27 04:39:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:20:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.263	790749	6.309 ug/ml
Target Compounds			
6) N-OCTADECANE	10.868	179915	1.283 ug/ml
7) N-EICOSANE	12.127f	1099500	7.714 ug/ml
8) N-DOCOSANE	13.409	804854	5.649 ug/ml
10) N-TETRACOSANE	14.466	3128450	22.045 ug/ml
12) N-OCTACOSANE	16.381	2689105	18.744 ug/ml
13) N-TRIACONTANE	17.322	139849	0.964 ug/ml
14) N-DOTRIACONTANE	18.154	321111	2.278 ug/ml
15) N-TETRATRIACONTANE	18.933	263476	1.959 ug/ml
16) N-HEXATRIACONTANE	19.687	495046	3.975 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092618\
Data File : FF002241.D
Signal(s) : FID2B.ch
Acq On : 26 Sep 2018 11:56
Operator : AJ\SJ
Sample : J4779-07RE 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 27 04:39:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

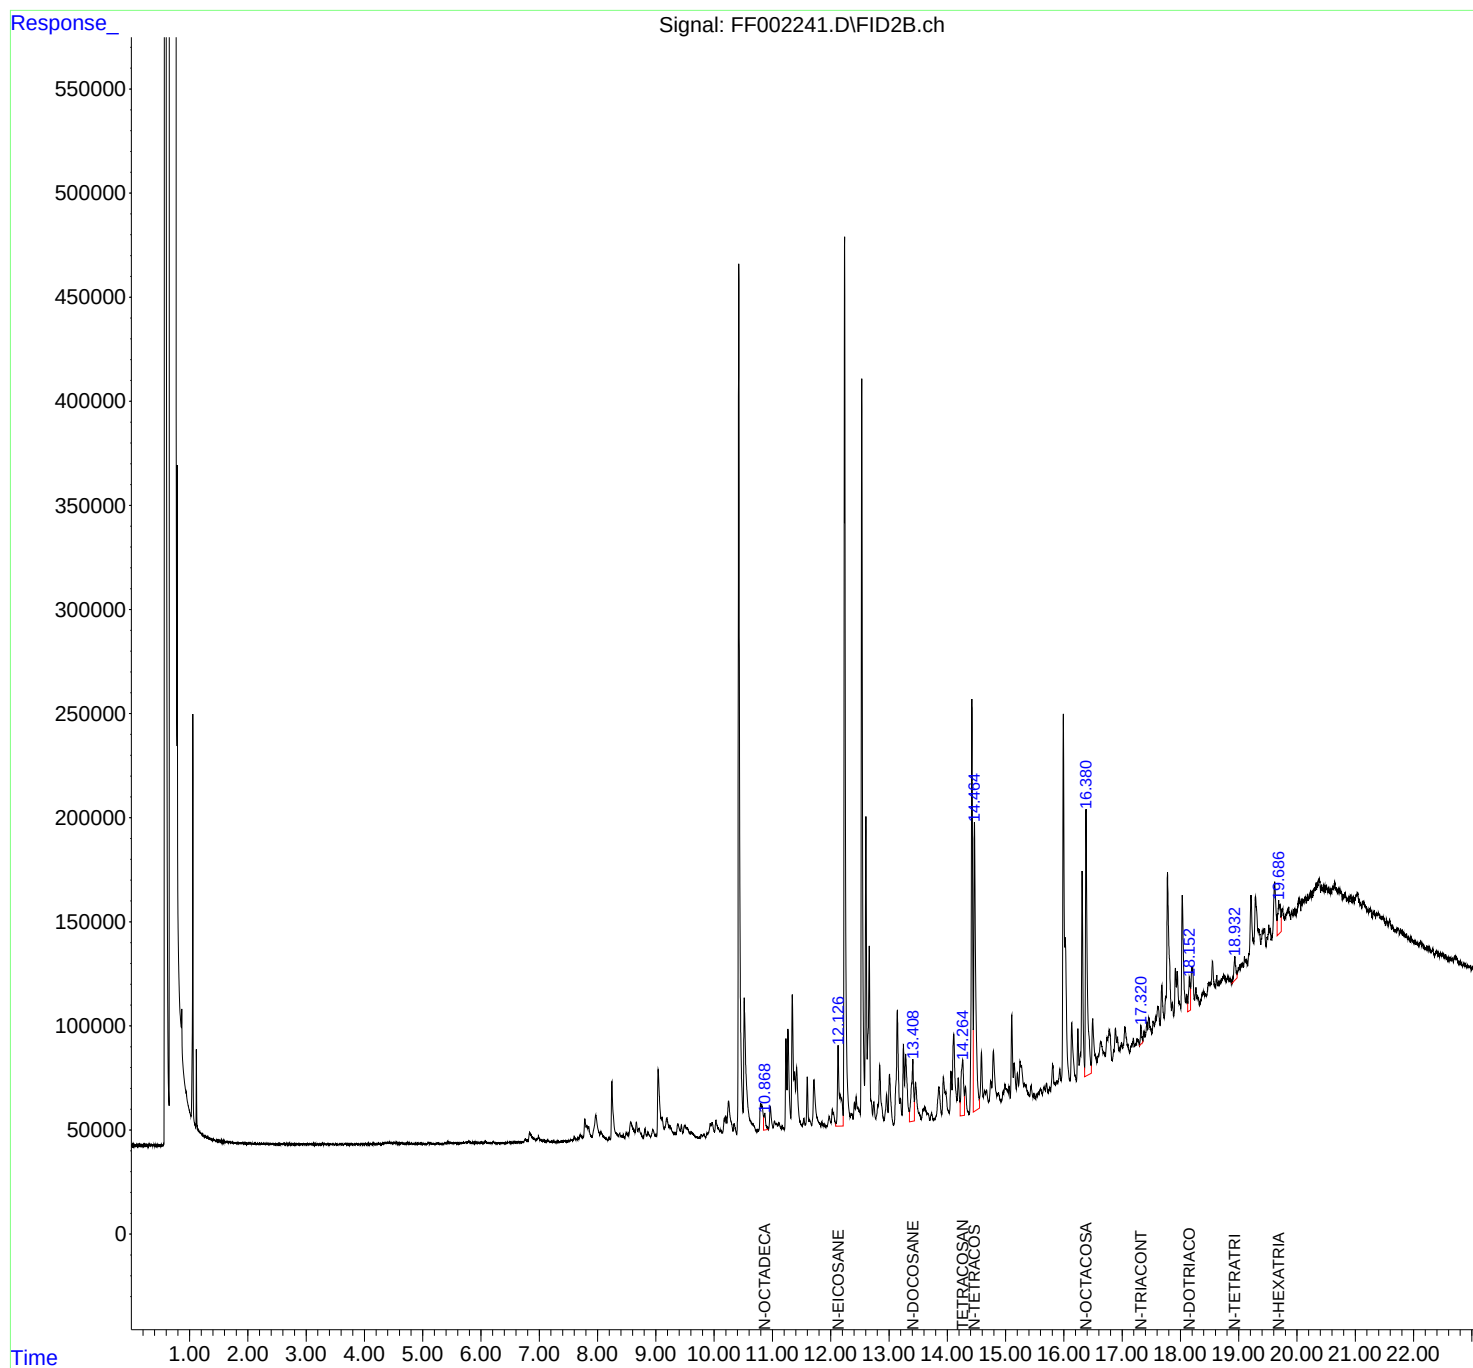

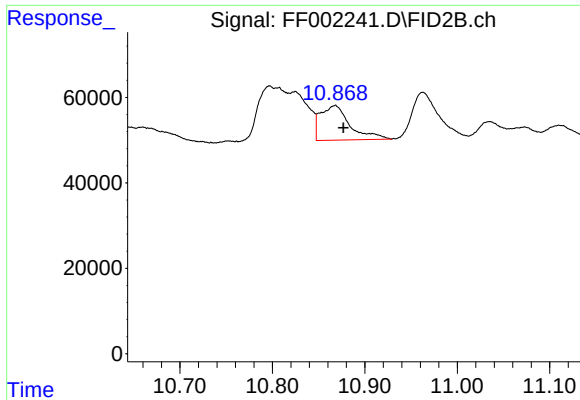


#6 N-OCTADECANE

R.T.: 10.868 min
Delta R.T.: -0.009 min
Response: 179915
Conc: 1.28 ug/ml

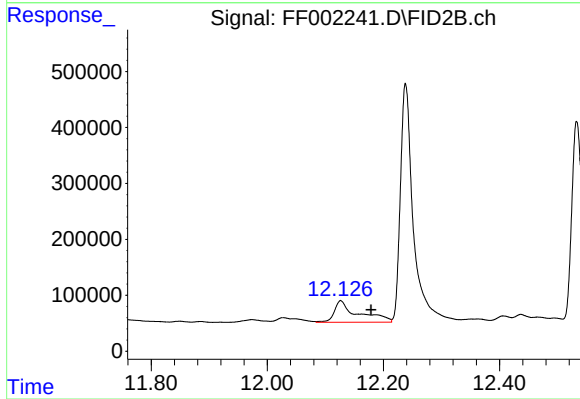


#7 N-EICOSANE

R.T.: 12.127 min
Delta R.T.: -0.052 min
Response: 1099500
Conc: 7.71 ug/ml

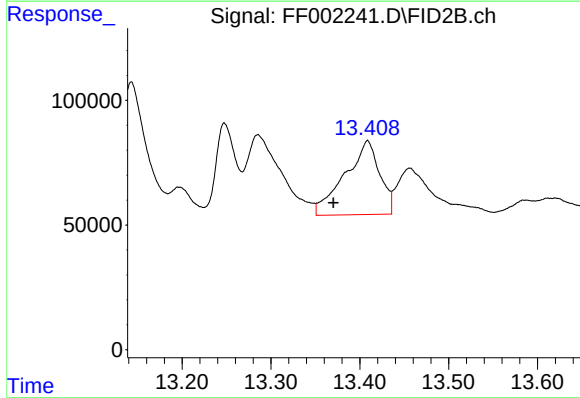


#8 N-DOCOSANE

R.T.: 13.409 min
Delta R.T.: 0.038 min
Response: 804854
Conc: 5.65 ug/ml

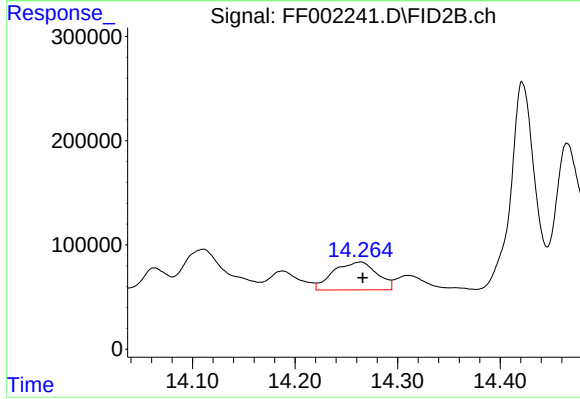


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.263 min
Delta R.T.: -0.003 min
Response: 790749
Conc: 6.31 ug/ml

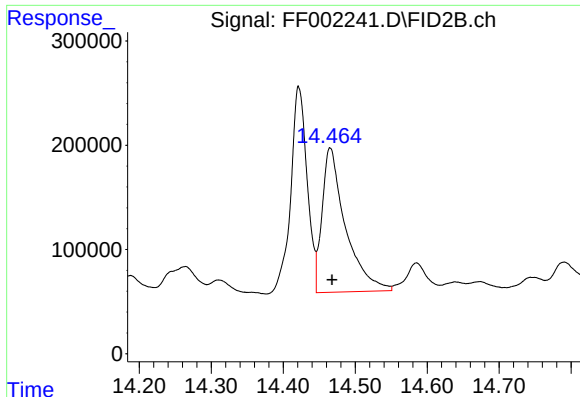


#10 N-TETRACOSANE

R.T.: 14.466 min
Delta R.T.: -0.002 min
Response: 3128450
Conc: 22.05 ug/ml

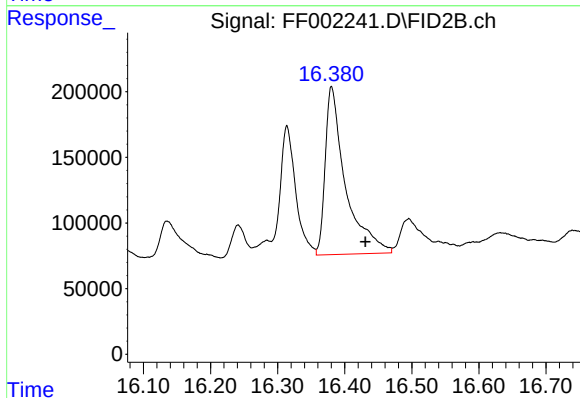


#12 N-OCTACOSANE

R.T.: 16.381 min
Delta R.T.: -0.050 min
Response: 2689105
Conc: 18.74 ug/ml

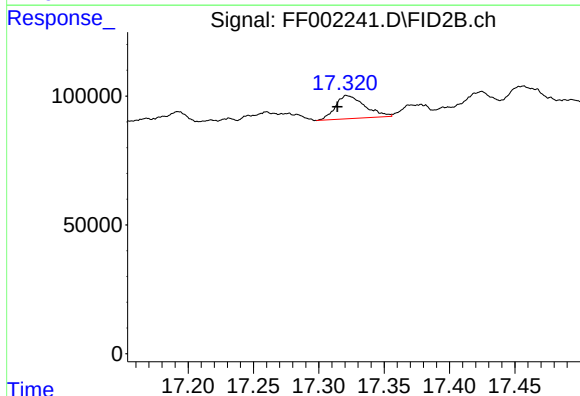


#13 N-TRIACONTANE

R.T.: 17.322 min
Delta R.T.: 0.008 min
Response: 139849
Conc: 0.96 ug/ml

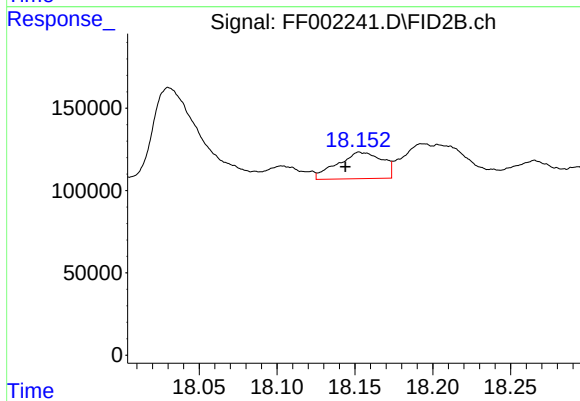


#14 N-DOTRIACONTANE

R.T.: 18.154 min
Delta R.T.: 0.011 min
Response: 321111
Conc: 2.28 ug/ml

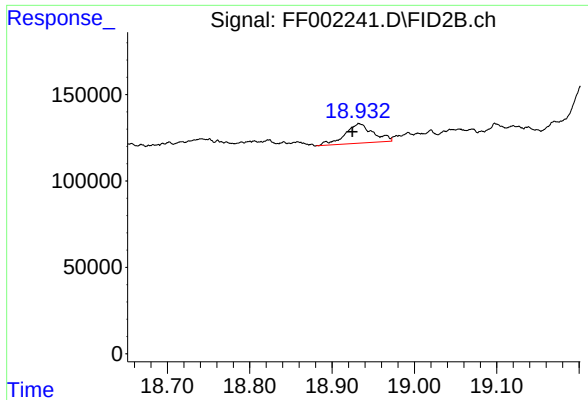

#15 N-TETRATRIACONTANE

R.T.: 18.933 min
Delta R.T.: 0.009 min
Response: 263476
Conc: 1.96 ug/ml

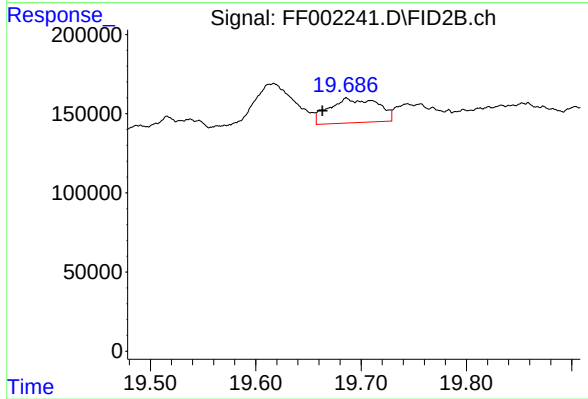

#16 N-HEXATRIACONTANE

R.T.: 19.687 min
Delta R.T.: 0.023 min
Response: 495046
Conc: 3.97 ug/ml