

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092618\
Data File : FF002252.D
Signal(s) : FID2B.ch
Acq On : 26 Sep 2018 18:13
Operator : AJ\SJ
Sample : J4773-13 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 27 04:41:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.266	149989	1.197 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.148	91885	0.652 ug/ml
16) N-HEXATRIACONTANE	19.702	72251	0.580 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092618\
Data File : FF002252.D
Signal(s) : FID2B.ch
Acq On : 26 Sep 2018 18:13
Operator : AJ\SJ
Sample : J4773-13 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 27 04:41:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

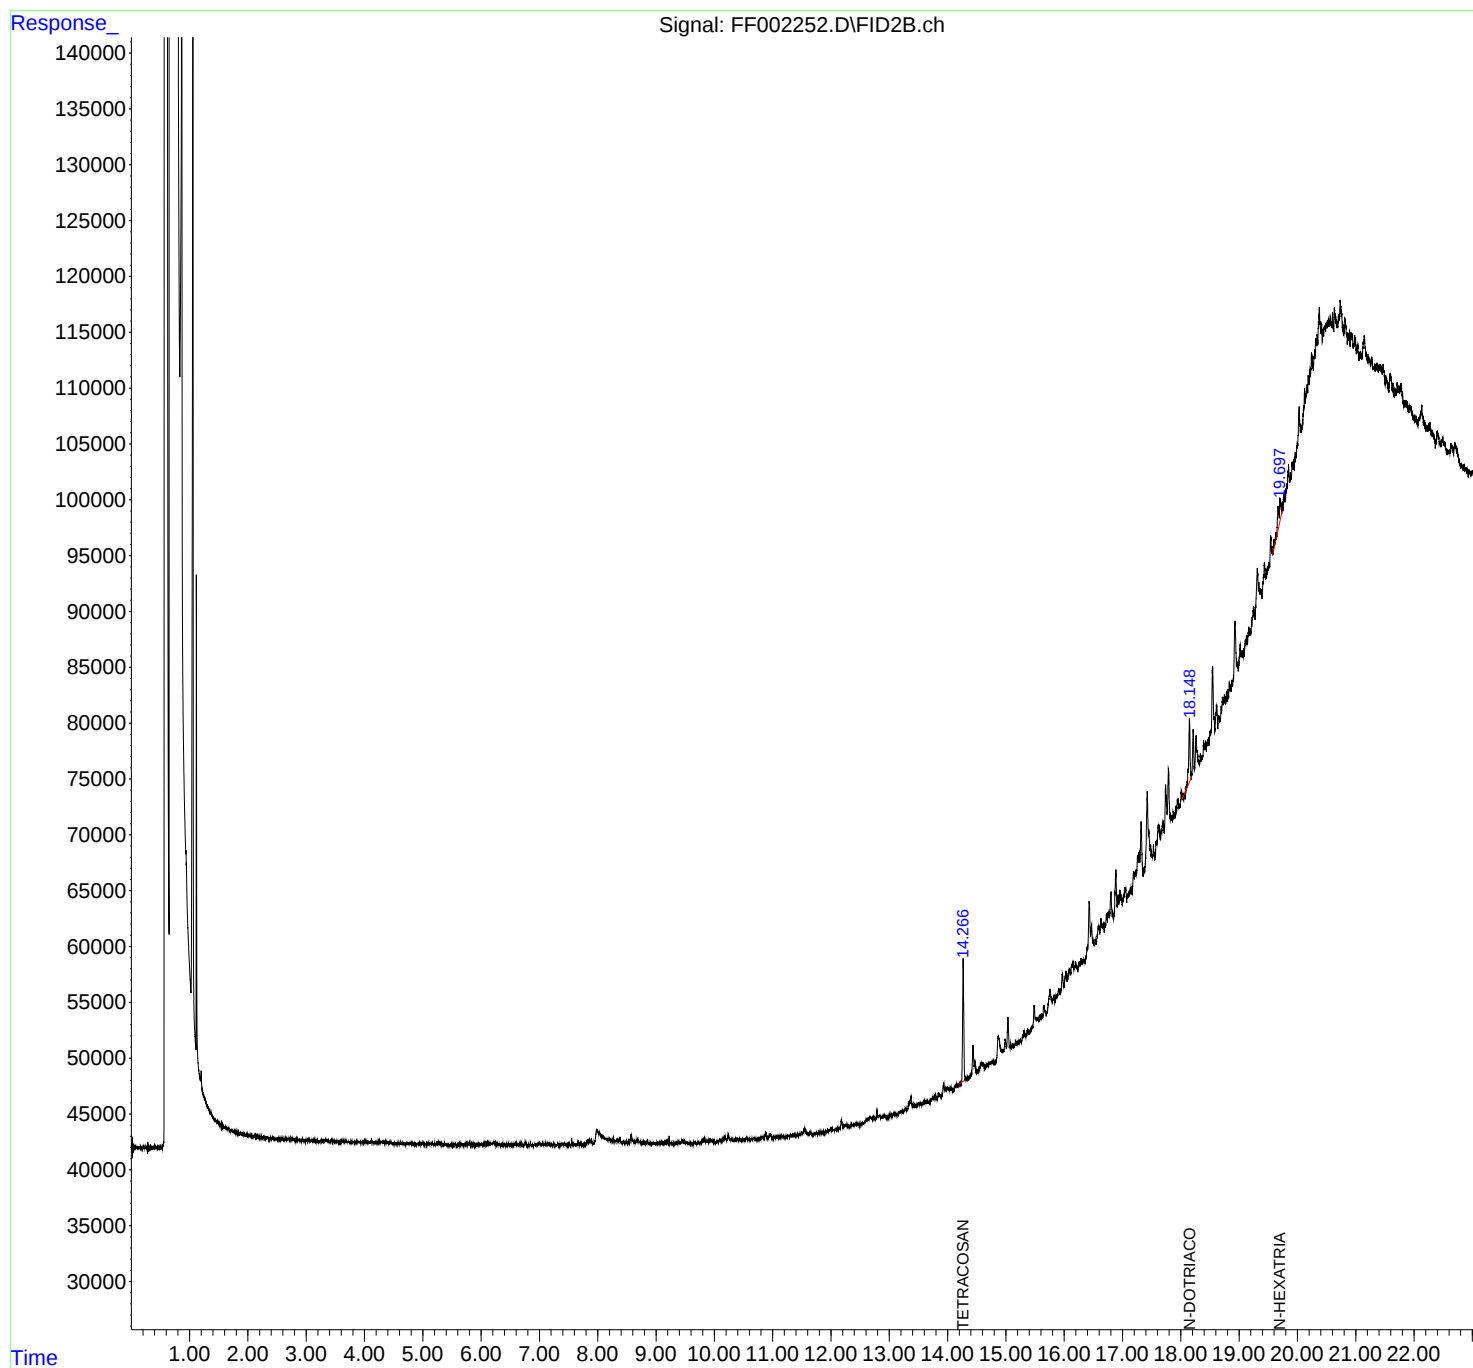

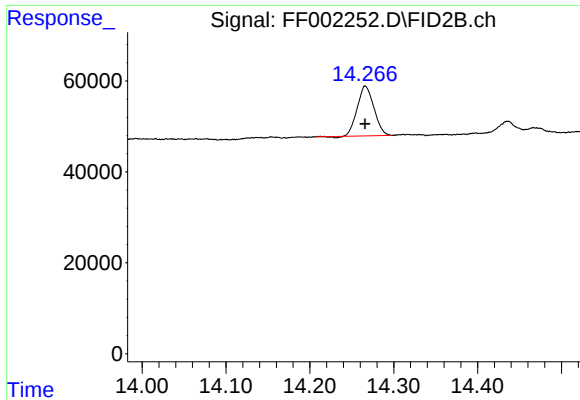


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.266 min
Delta R.T.: 0.000 min
Response: 149989
Conc: 1.20 ug/ml

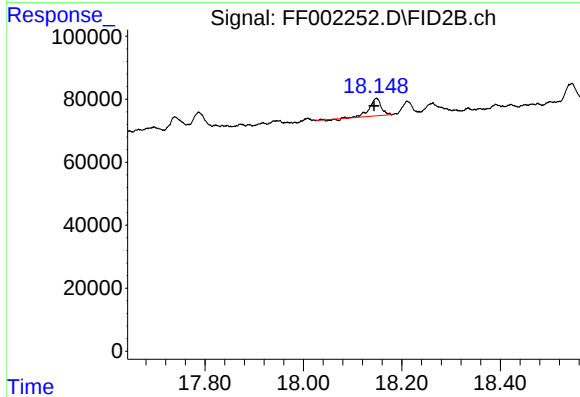

#14 N-DOTRIACONTANE

R.T.: 18.148 min
Delta R.T.: 0.005 min
Response: 91885
Conc: 0.65 ug/ml

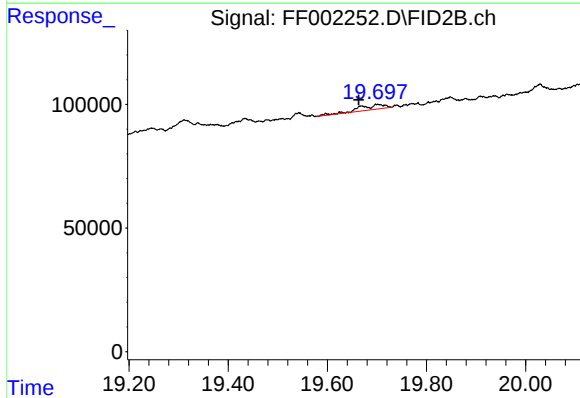

#16 N-HEXATRIACONTANE

R.T.: 19.702 min
Delta R.T.: 0.039 min
Response: 72251
Conc: 0.58 ug/ml