

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092618\
 Data File : FF002246.D
 Signal(s) : FID2B.ch
 Acq On : 26 Sep 2018 14:39
 Operator : AJ\SJ
 Sample : J5081-01MSD
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 27 04:40:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:20:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.268	1968663	15.707 ug/mlm
Target Compounds			
2) N-DECANE	4.057	1744178	15.050 ug/ml
3) N-DODECANE	6.063	2051495	16.395 ug/ml
4) N-TETRADECANE	7.846	2317305	17.489 ug/ml
5) N-HEXADECANE	9.438	2326490	16.987 ug/ml
6) N-OCTADECANE	10.874	2336216	16.660 ug/ml
7) N-EICOSANE	12.178	2318400	16.265 ug/mlm
8) N-DOCOSANE	13.371	2262593	15.881 ug/ml
10) N-TETRACOSANE	14.469	3128484	22.046 ug/mlm
11) N-HEXACOSANE	15.488	2248786	15.811 ug/ml
12) N-OCTACOSANE	16.436	2714827	18.923 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092618\
Data File : FF002246.D
Signal(s) : FID2B.ch
Acq On : 26 Sep 2018 14:39
Operator : AJ\SJ
Sample : J5081-01MSD
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 27 04:40:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

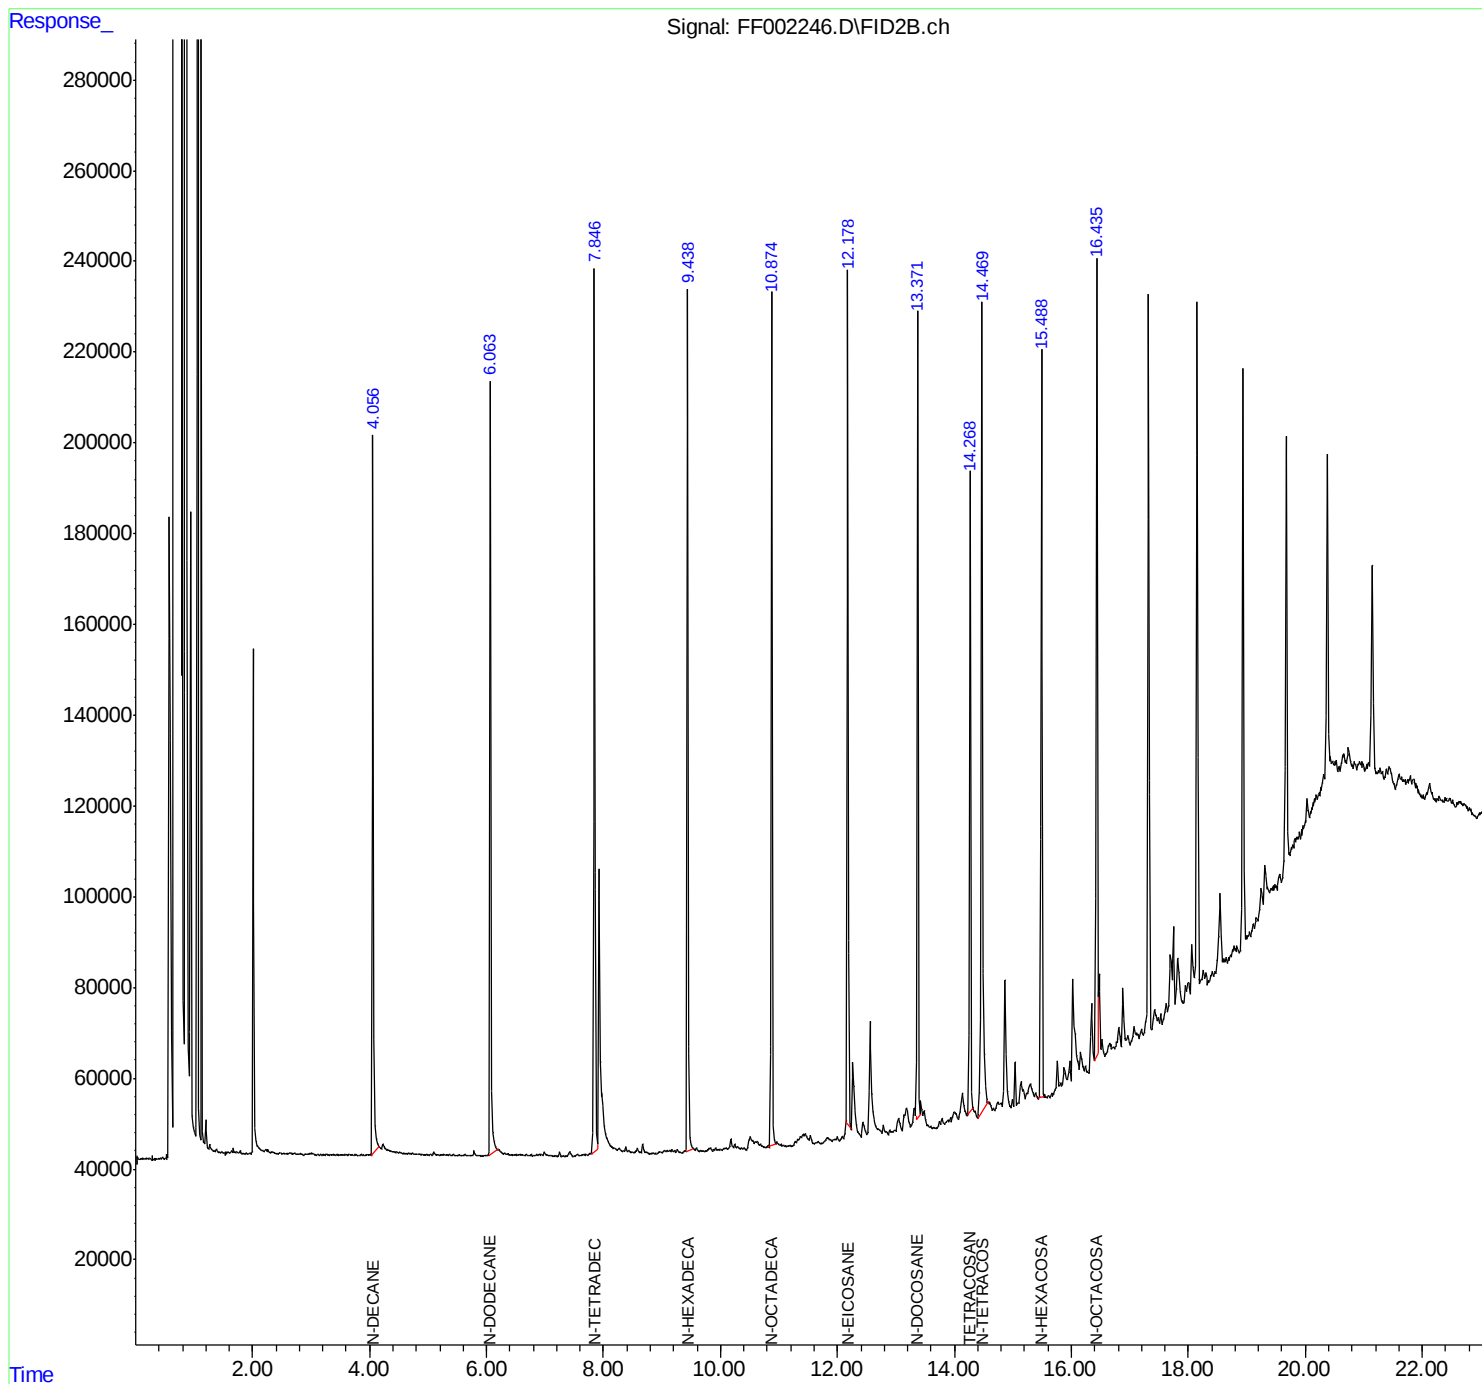

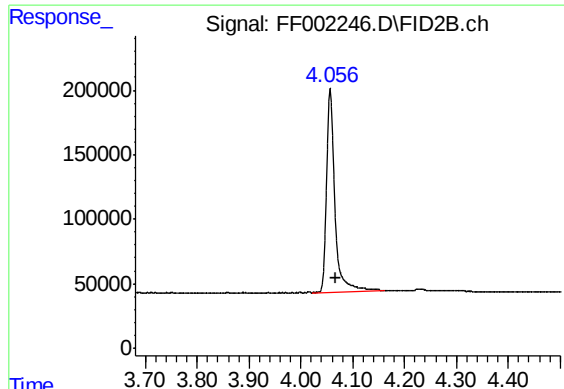


#2 N-DECANE

R.T.: 4.057 min
Delta R.T.: -0.010 min
Response: 1744178
Conc: 15.05 ug/ml

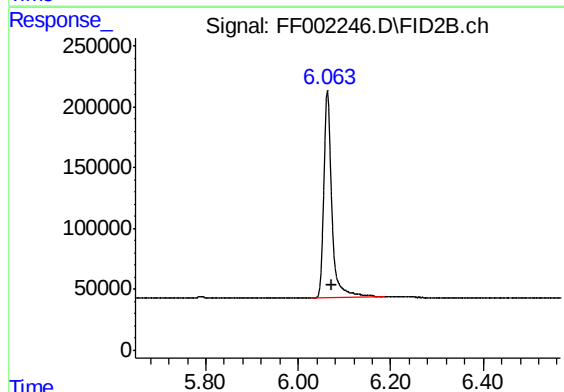


#3 N-DODECANE

R.T.: 6.063 min
Delta R.T.: -0.008 min
Response: 2051495
Conc: 16.40 ug/ml

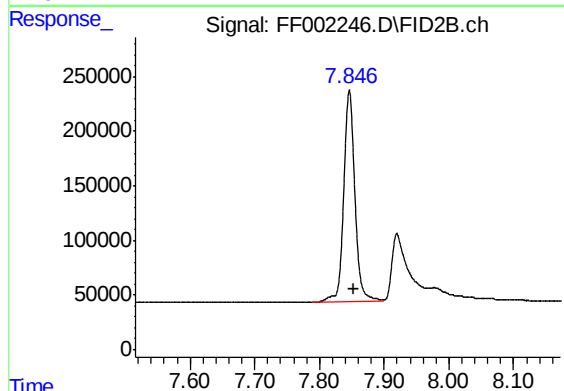


#4 N-TETRADECANE

R.T.: 7.846 min
Delta R.T.: -0.007 min
Response: 2317305
Conc: 17.49 ug/ml

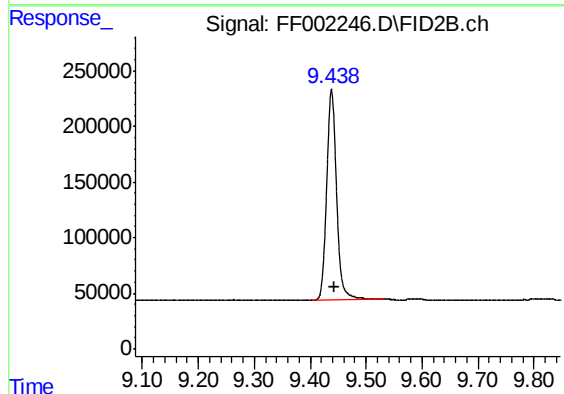


#5 N-HEXADECANE

R.T.: 9.438 min
Delta R.T.: -0.005 min
Response: 2326490
Conc: 16.99 ug/ml

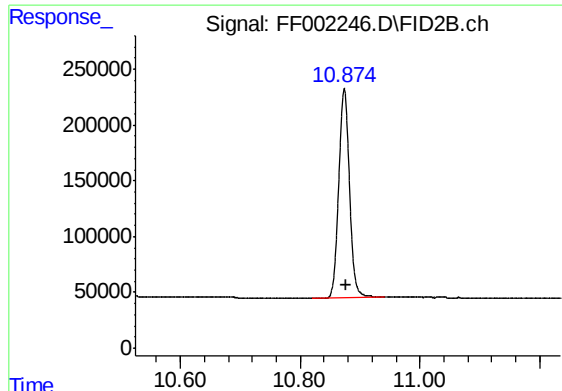


#6 N-OCTADECANE

R.T.: 10.874 min
Delta R.T.: -0.003 min
Response: 2336216
Conc: 16.66 ug/ml

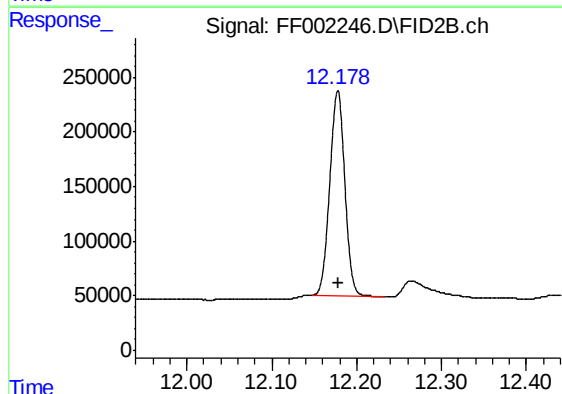


#7 N-EICOSANE

R.T.: 12.178 min
Delta R.T.: 0.000 min
Response: 2318400
Conc: 16.27 ug/ml m

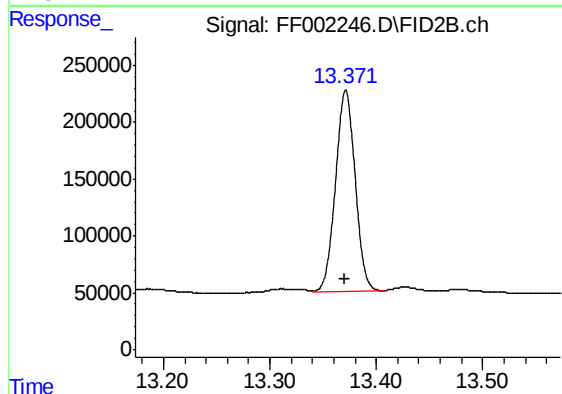


#8 N-DOCOSANE

R.T.: 13.371 min
Delta R.T.: 0.000 min
Response: 2262593
Conc: 15.88 ug/ml

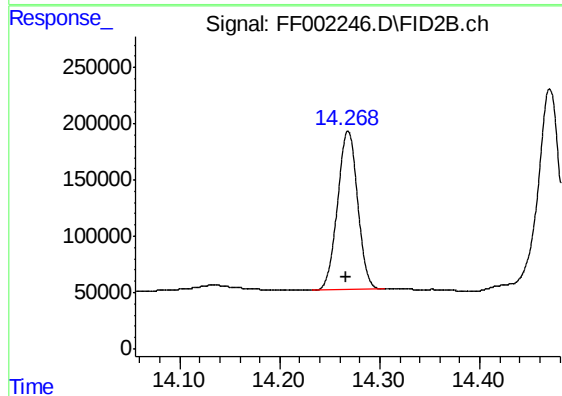


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.268 min
Delta R.T.: 0.002 min
Response: 1968663
Conc: 15.71 ug/ml m

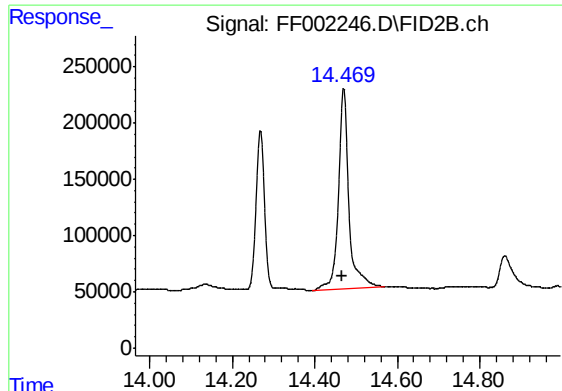


#10 N-TETRACOSANE

R.T.: 14.469 min
Delta R.T.: 0.001 min
Response: 3128484
Conc: 22.05 ug/ml m

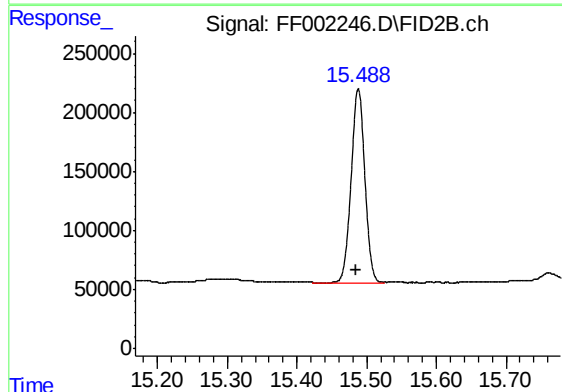

#11 N-HEXACOSANE

R.T.: 15.488 min
Delta R.T.: 0.003 min
Response: 2248786
Conc: 15.81 ug/ml

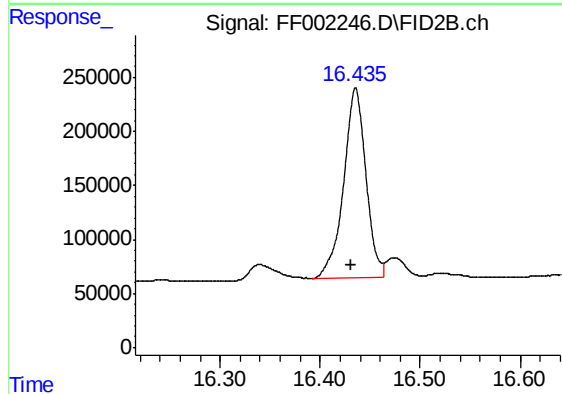

#12 N-OCTACOSANE

R.T.: 16.436 min
Delta R.T.: 0.005 min
Response: 2714827
Conc: 18.92 ug/ml