

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092619\
Data File : FF005684.D
Signal(s) : FID2B.ch
Acq On : 26 Sep 2019 12:06
Operator : DD\AJ
Sample : K5019-03 25X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
QNWP8-MW26S-GW

Integration File: autoint1.e
Quant Time: Sep 27 01:06:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) N-DECANE	4.382	456089	3.190 ug/ml
3) N-DODECANE	6.394	227210	1.585 ug/ml
4) N-TETRADECANE	8.108f	123456	0.876 ug/ml
5) N-HEXADECANE	9.757	595132	4.255 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092619\
Data File : FF005684.D
Signal(s) : FID2B.ch
Acq On : 26 Sep 2019 12:06
Operator : DD\AJ
Sample : K5019-03 25X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
QNWP8-MW26S-GW

Integration File: autoint1.e
Quant Time: Sep 27 01:06:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

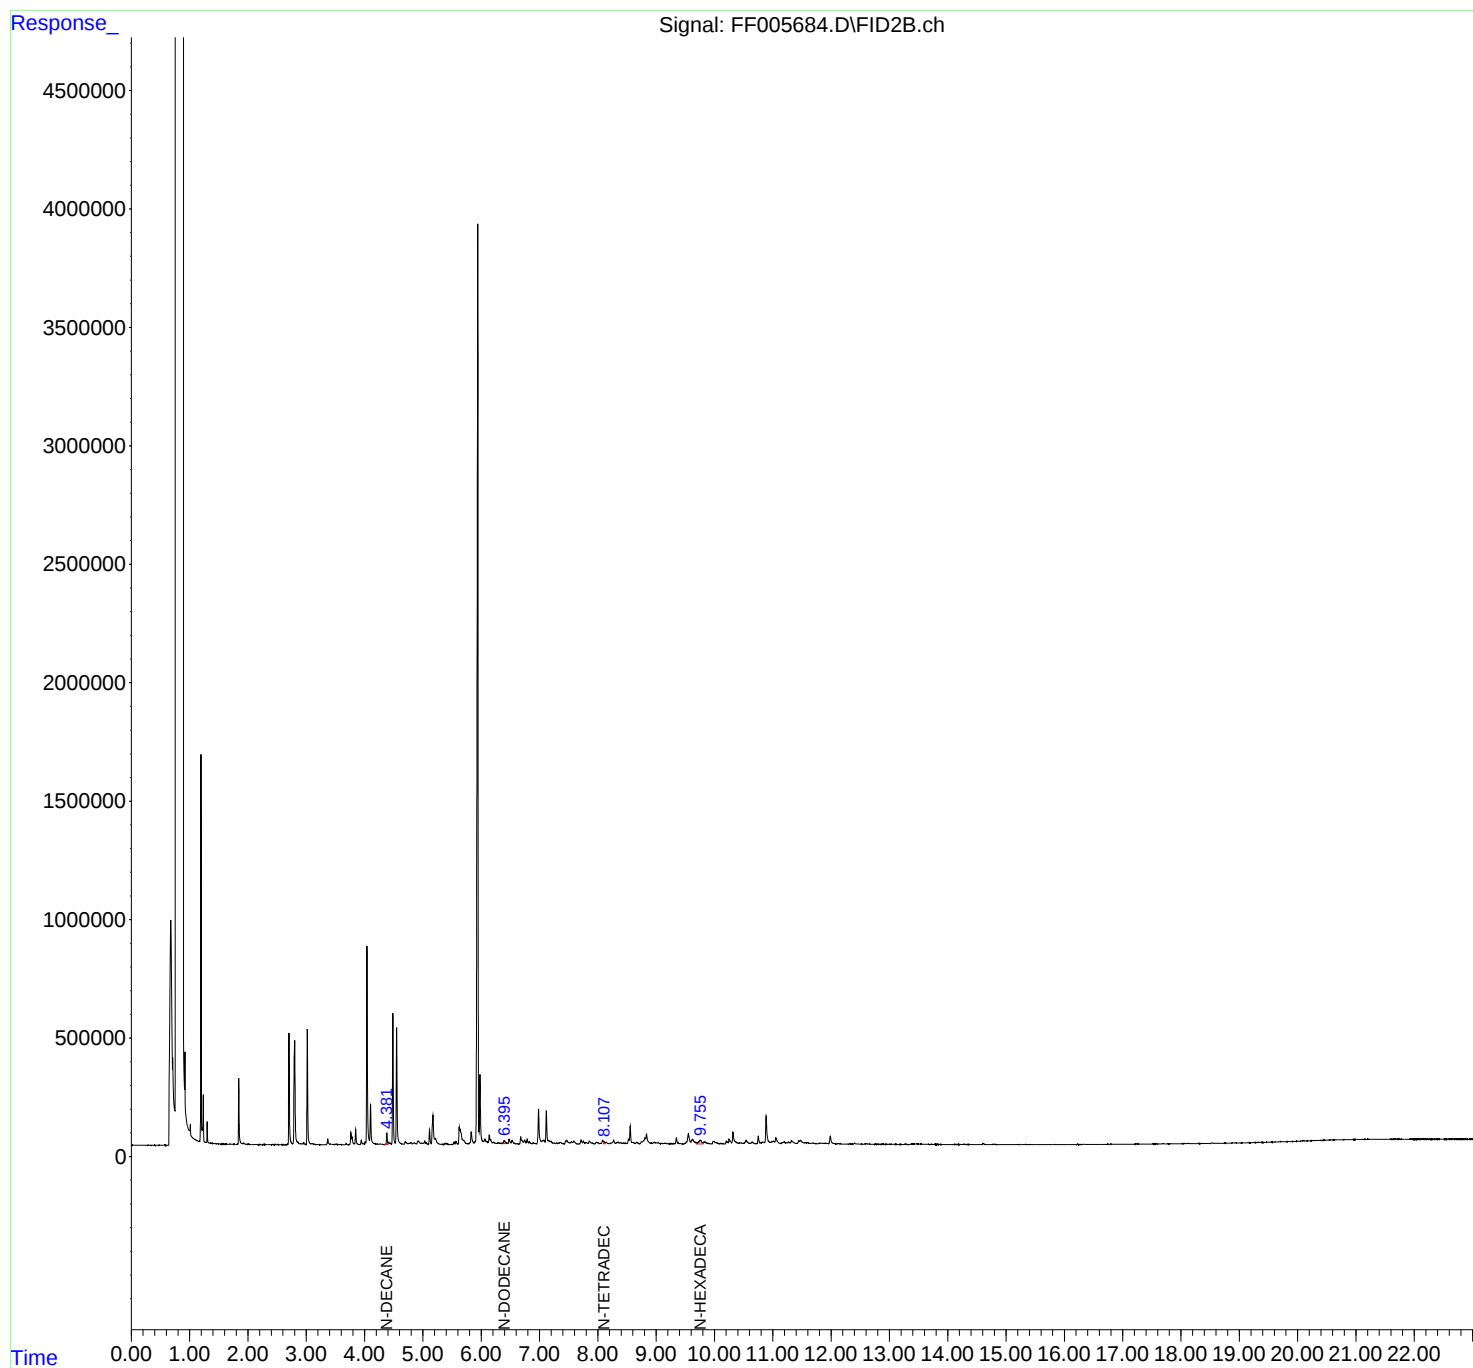


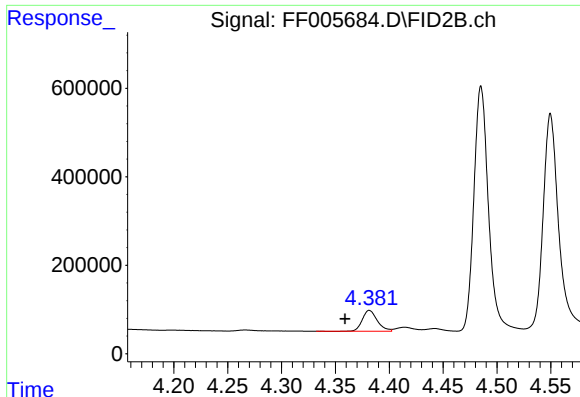

#2 N-DECANE


R.T.: 4.382 min
Delta R.T.: 0.023 min
Response: 456089
Conc: 3.19 ug/ml

Instrument :
FID_F
ClientSampleId :
QNWP8-MW26S-GW

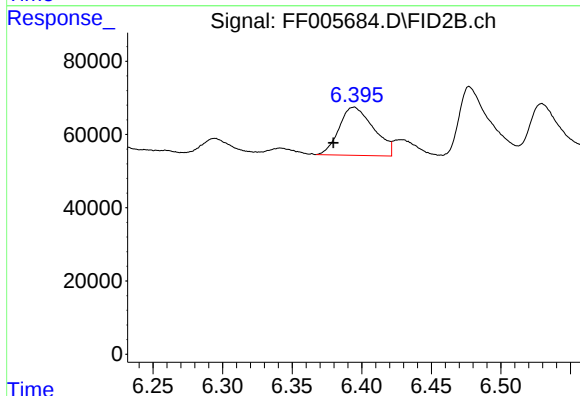


#3 N-DODECANE

R.T.: 6.394 min
Delta R.T.: 0.015 min
Response: 227210
Conc: 1.59 ug/ml

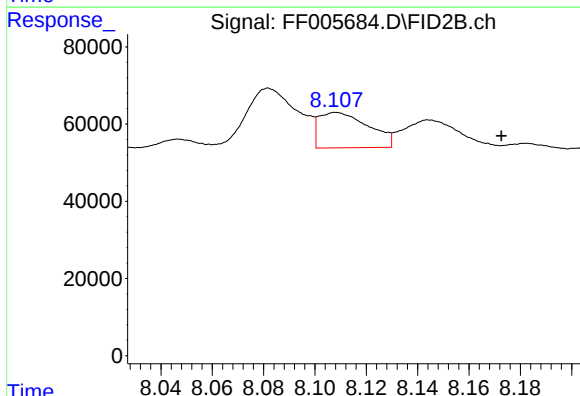


#4 N-TETRADECANE

R.T.: 8.108 min
Delta R.T.: -0.064 min
Response: 123456
Conc: 0.88 ug/ml

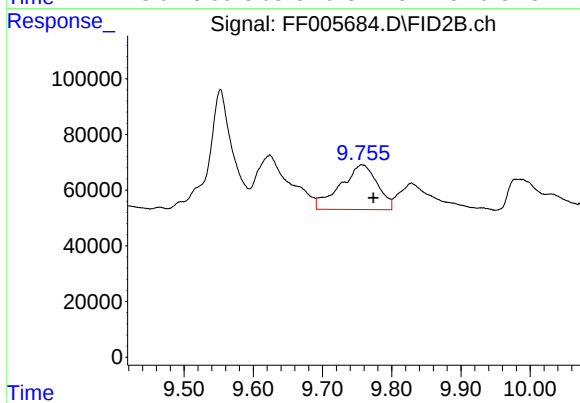

#5 N-HEXADECANE

R.T.: 9.757 min
Delta R.T.: -0.017 min
Response: 595132
Conc: 4.26 ug/ml

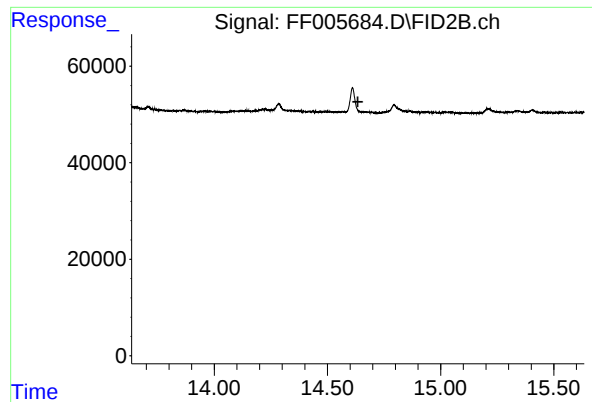

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.635 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
QNWP8-MW26S-GW