

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092619\
 Data File : FF005690.D
 Signal(s) : FID2B.ch
 Acq On : 26 Sep 2019 16:42
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 27 01:07:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.571f	346626	3.239 ug/ml
Target Compounds			
3) N-DODECANE	6.359	3916979	27.325 ug/ml
11) N-HEXACOSANE	15.841	98500	0.823 ug/ml
12) N-OCTACOSANE	16.796	4763690	39.922 ug/ml
13) N-TRIACONTANE	17.686	700729	5.793 ug/ml
14) N-DOTRIACONTANE	18.524	822963	6.639 ug/ml
15) N-TETRATRIACONTANE	19.316	576521	4.784 ug/ml
16) N-HEXATRIACONTANE	20.064	369814	3.081 ug/ml
17) N-OCTATRIACONTANE	20.807	232504	2.131 ug/ml
18) N-TETRACONTANE	21.707	188490	1.483 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092619\
Data File : FF005690.D
Signal(s) : FID2B.ch
Acq On : 26 Sep 2019 16:42
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Sep 27 01:07:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

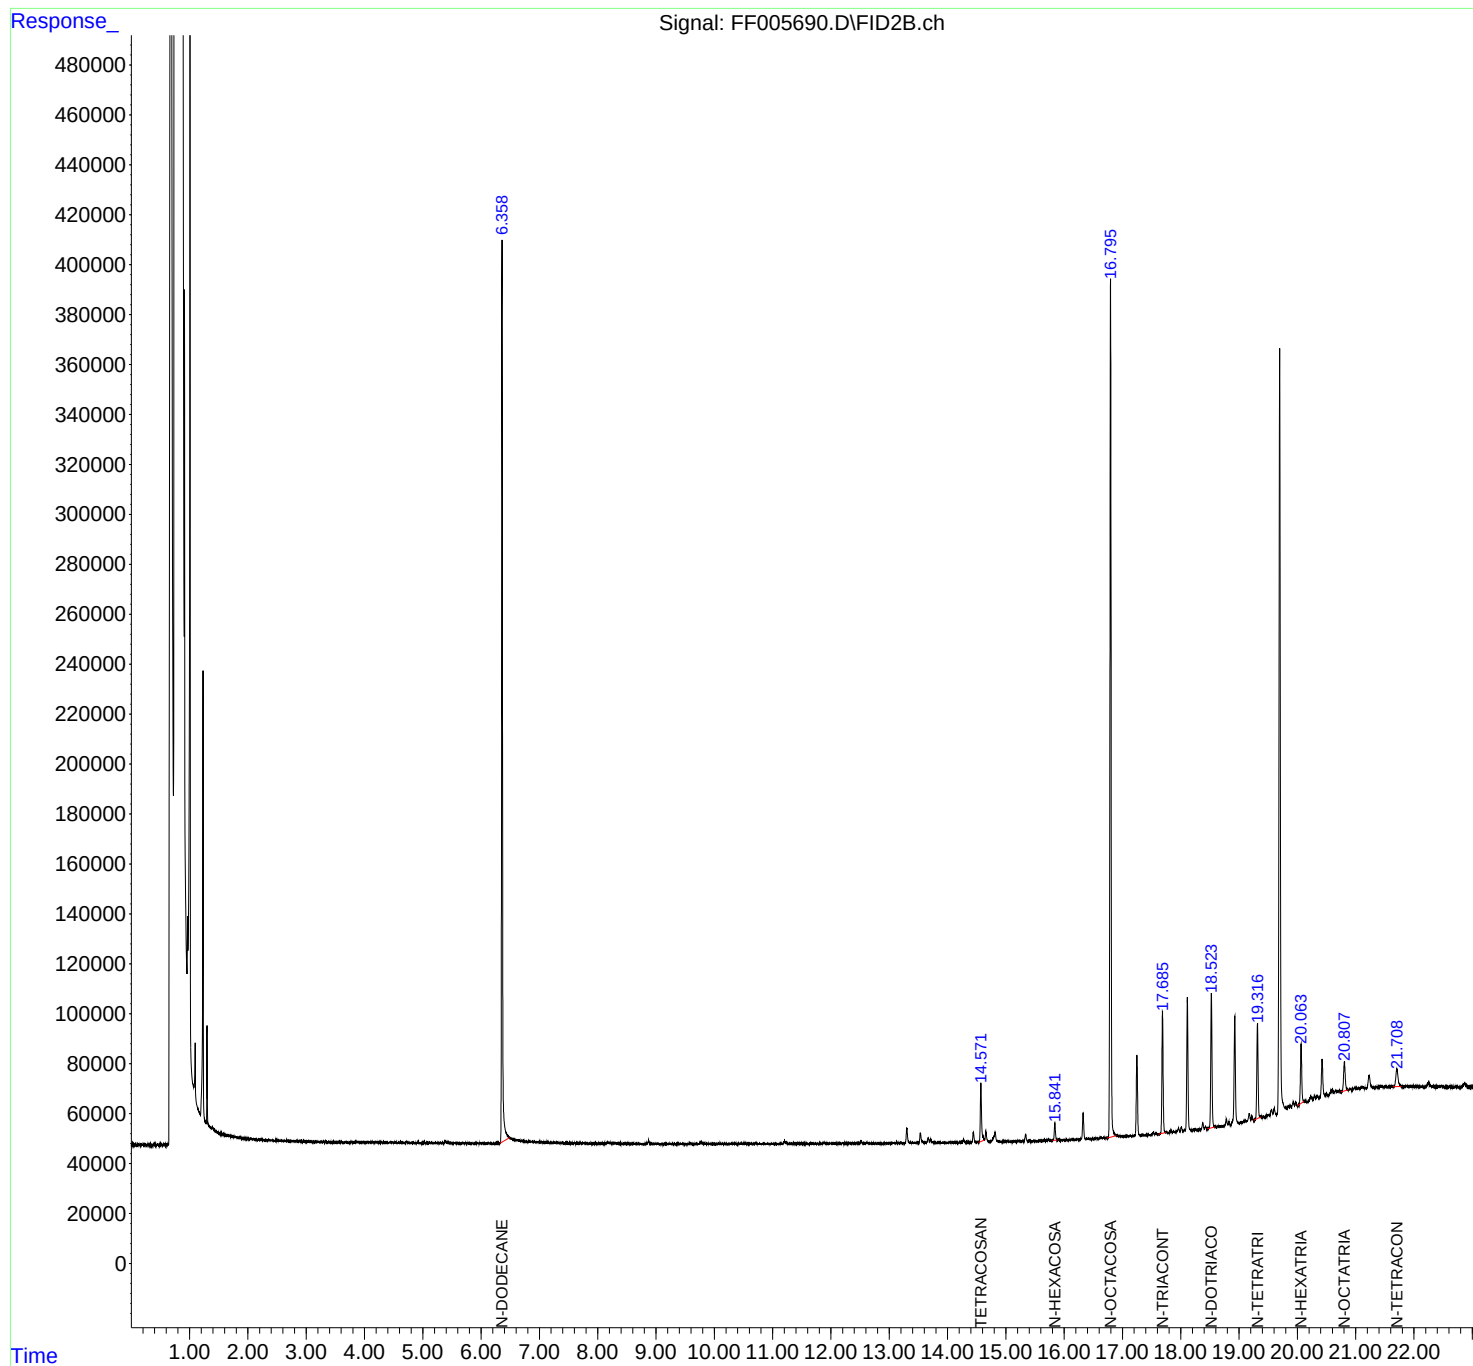


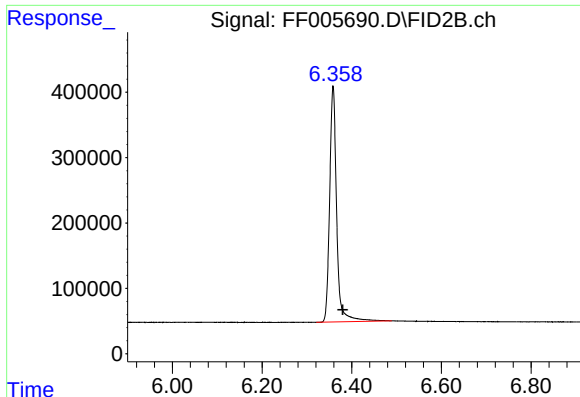

#3 N-DODECANE


R.T.: 6.359 min
Delta R.T.: -0.021 min
Response: 3916979
Conc: 27.32 ug/ml

Instrument :
FID_F
ClientSampleId :

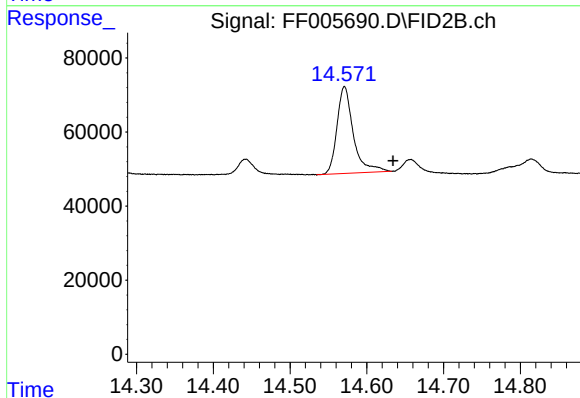


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.571 min
Delta R.T.: -0.064 min
Response: 346626
Conc: 3.24 ug/ml

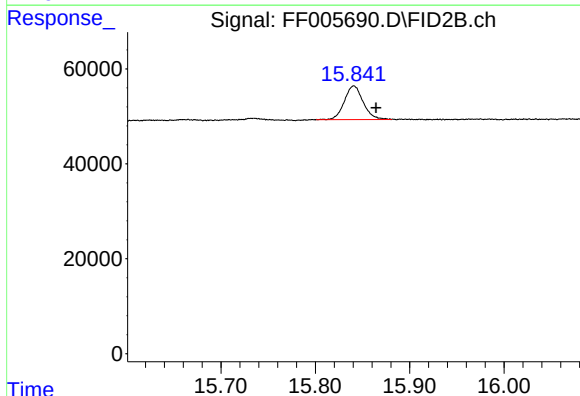


#11 N-HEXACOSANE

R.T.: 15.841 min
Delta R.T.: -0.023 min
Response: 98500
Conc: 0.82 ug/ml

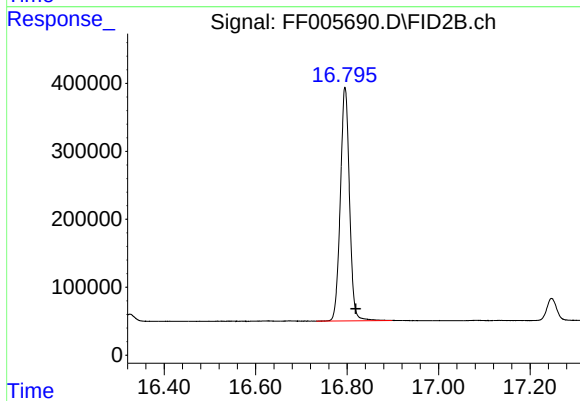

#12 N-OCTACOSANE


R.T.: 16.796 min
Delta R.T.: -0.023 min
Response: 4763690
Conc: 39.92 ug/ml

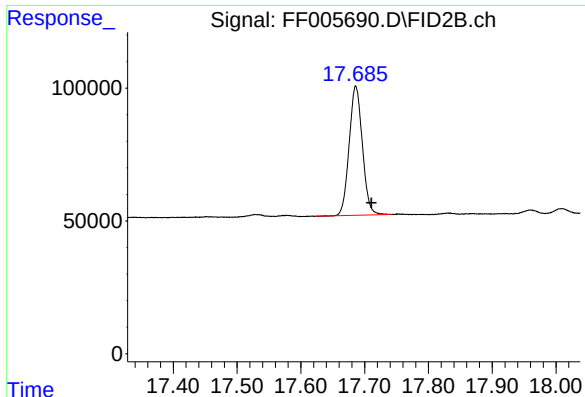

#13 N-TRIACONTANE


R.T.: 17.686 min
Delta R.T.: -0.025 min
Response: 700729
Conc: 5.79 ug/ml

Instrument :
FID_F
ClientSampleId :

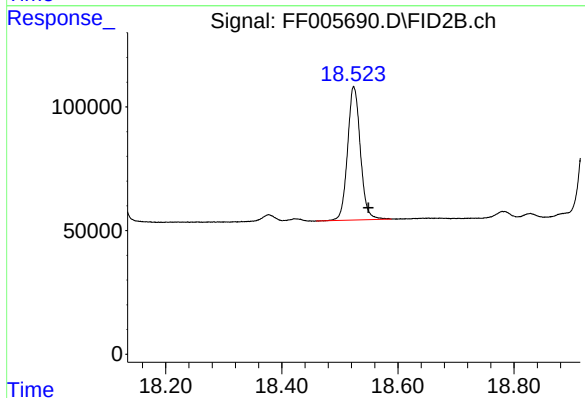


#14 N-DOTRIACONTANE

R.T.: 18.524 min
Delta R.T.: -0.025 min
Response: 822963
Conc: 6.64 ug/ml

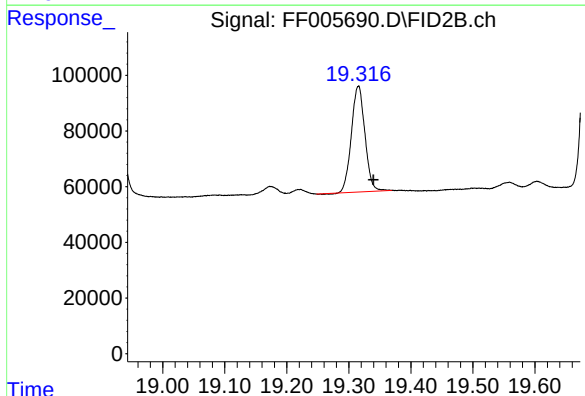


#15 N-TETRATRIACONTANE

R.T.: 19.316 min
Delta R.T.: -0.024 min
Response: 576521
Conc: 4.78 ug/ml

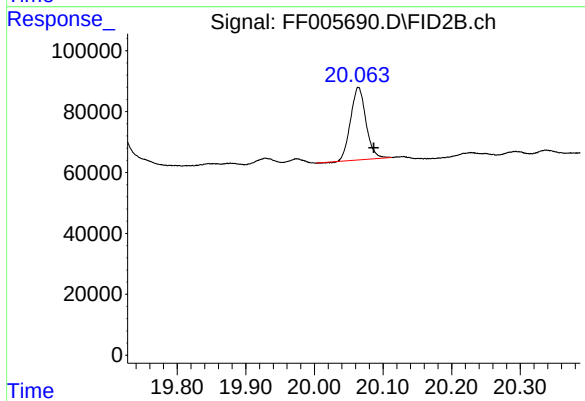

#16 N-HEXATRIACONTANE


R.T.: 20.064 min
Delta R.T.: -0.023 min
Response: 369814
Conc: 3.08 ug/ml

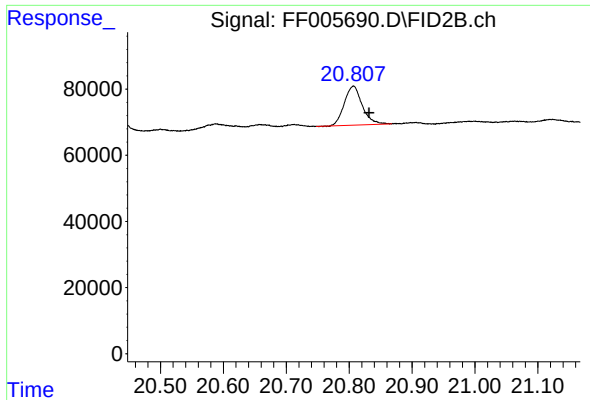

#17 N-OCTATRIACONTANE

R.T.: 20.807 min
Delta R.T.: -0.024 min
Response: 232504
Conc: 2.13 ug/ml

Instrument :
FID_F
ClientSampleId :

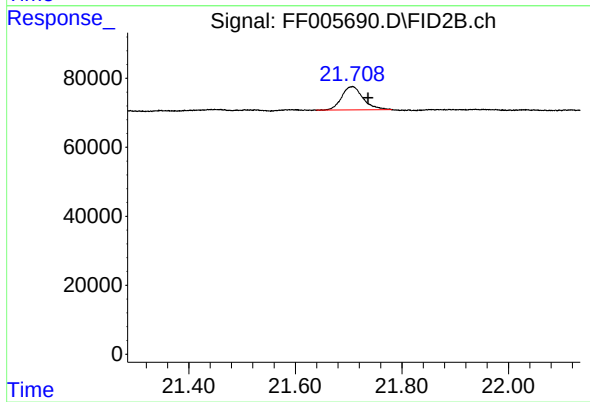

#18 N-TETRACONTANE

R.T.: 21.707 min
Delta R.T.: -0.030 min
Response: 188490
Conc: 1.48 ug/ml