

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092619\
 Data File : FF005691.D
 Signal(s) : FID2B.ch
 Acq On : 26 Sep 2019 17:12
 Operator : DD\AJ
 Sample : PB123394BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 27 01:08:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.611	2256847	21.090 ug/ml
Target Compounds			
4) N-TETRADECANE	8.222	162072	1.150 ug/ml
11) N-HEXACOSANE	15.840	155832	1.302 ug/ml
12) N-OCTACOSANE	16.794	411481	3.448 ug/ml
13) N-TRIACONTANE	17.688	579459	4.790 ug/ml
14) N-DOTRIACONTANE	18.527	340696	2.748 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF092619\
Data File : FF005691.D
Signal(s) : FID2B.ch
Acq On : 26 Sep 2019 17:12
Operator : DD\AJ
Sample : PB123394BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 27 01:08:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

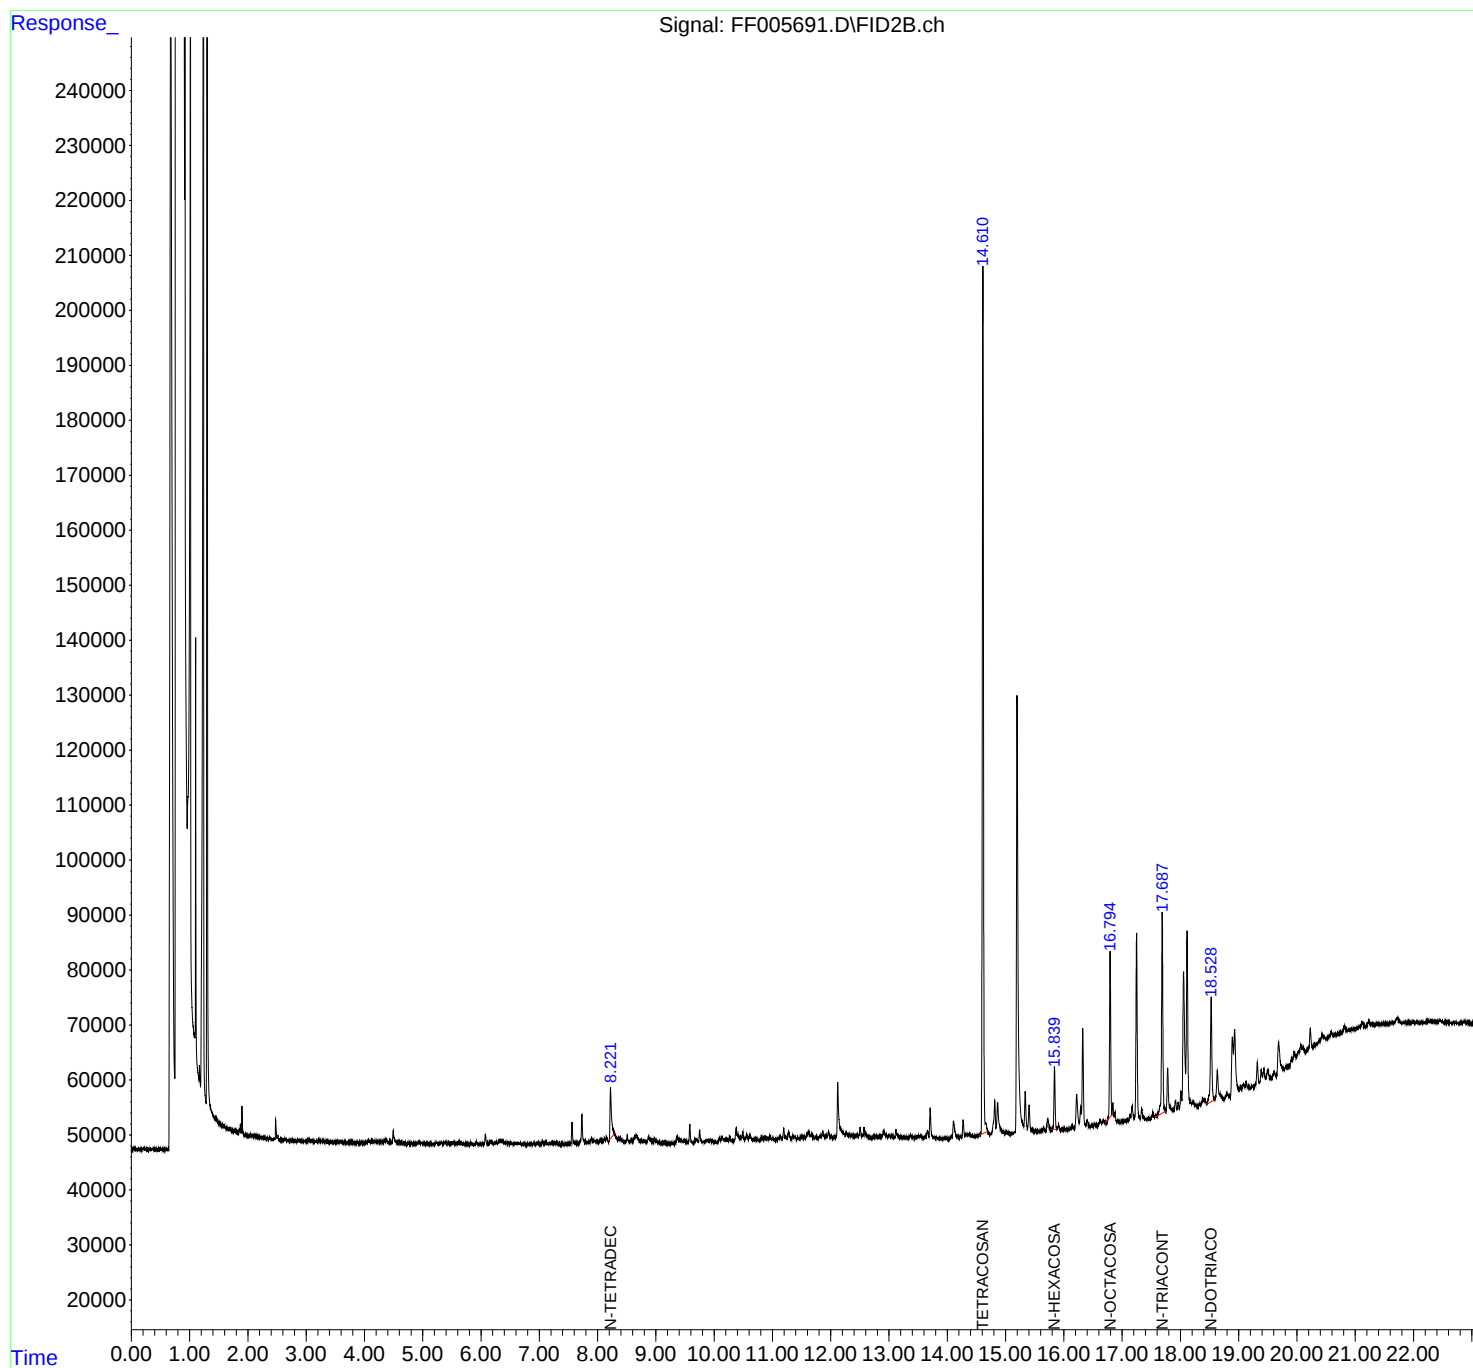


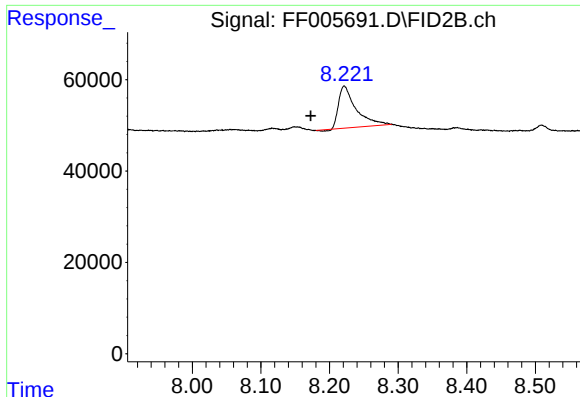

#4 N-TETRADECANE


R.T.: 8.222 min
Delta R.T.: 0.049 min
Response: 162072
Conc: 1.15 ug/ml

Instrument :
FID_F
ClientSampleId :

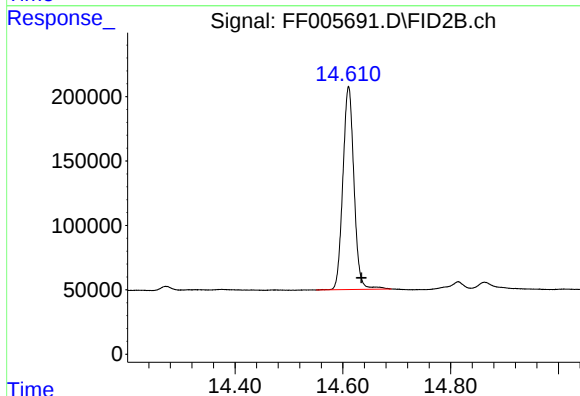


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.611 min
Delta R.T.: -0.024 min
Response: 2256847
Conc: 21.09 ug/ml

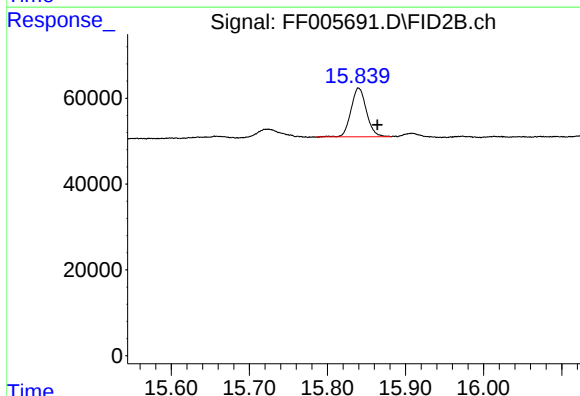


#11 N-HEXACOSANE

R.T.: 15.840 min
Delta R.T.: -0.024 min
Response: 155832
Conc: 1.30 ug/ml

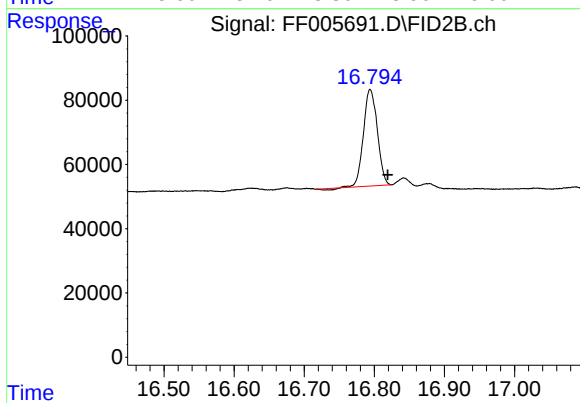

#12 N-OCTACOSANE


R.T.: 16.794 min
Delta R.T.: -0.025 min
Response: 411481
Conc: 3.45 ug/ml

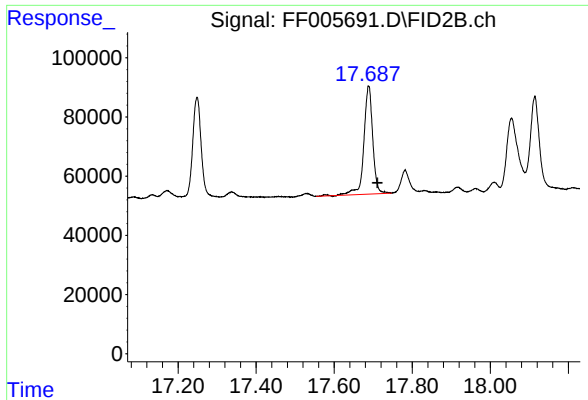

#13 N-TRIACONTANE

R.T.: 17.688 min
Delta R.T.: -0.022 min
Response: 579459
Conc: 4.79 ug/ml

Instrument :
FID_F
ClientSampleId :

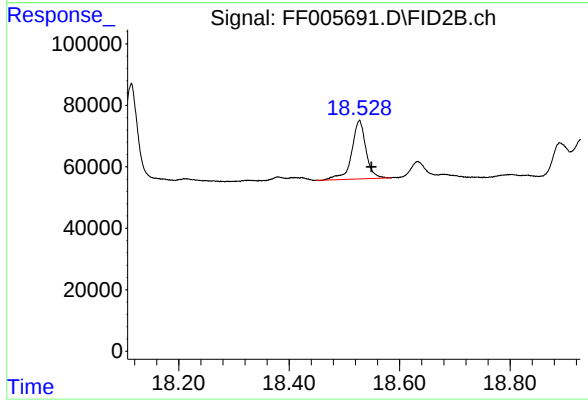

#14 N-DOTRIACONTANE

R.T.: 18.527 min
Delta R.T.: -0.022 min
Response: 340696
Conc: 2.75 ug/ml