

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
 Data File : FF002284.D
 Signal(s) : FID2B.ch
 Acq On : 01 Oct 2018 14:45
 Operator : AJ\SJ
 Sample : PB113351BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 02 03:46:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.638	2747898	19.267 ug/ml
Target Compounds			
1) N-OCTANE	2.289	3008786	19.034 ug/ml
2) N-DECANE	4.390	3091464	19.085 ug/ml
3) N-DODECANE	6.408	3145875	19.124 ug/ml
4) N-TETRADECANE	8.197	3192152	19.163 ug/ml
5) N-HEXADECANE	9.795	3217959	19.215 ug/ml
6) N-OCTADECANE	11.235	3230607	19.240 ug/ml
7) N-EICOSANE	12.543	3191964	19.273 ug/ml
8) N-DOCOSANE	13.739	3138975	19.237 ug/ml
10) N-TETRACOSANE	14.840	3071739	19.210 ug/ml
11) N-HEXACOSANE	15.860	3014667	19.248 ug/ml
12) N-OCTACOSANE	16.807	2963583	19.374 ug/ml
13) N-TRIACONTANE	17.694	2932041	19.602 ug/ml
14) N-DOTRIACONTANE	18.525	2857919	19.830 ug/ml
15) N-TETRATRIACONTANE	19.308	2724080	19.614 ug/ml
16) N-HEXATRIACONTANE	20.048	2475217	19.211 ug/ml
17) N-OCTATRIACONTANE	20.779	2215968	19.400 ug/ml
18) N-TETRACONTANE	21.675	2322977	20.553 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
Data File : FF002284.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2018 14:45
Operator : AJ\SJ
Sample : PB113351BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 02 03:46:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

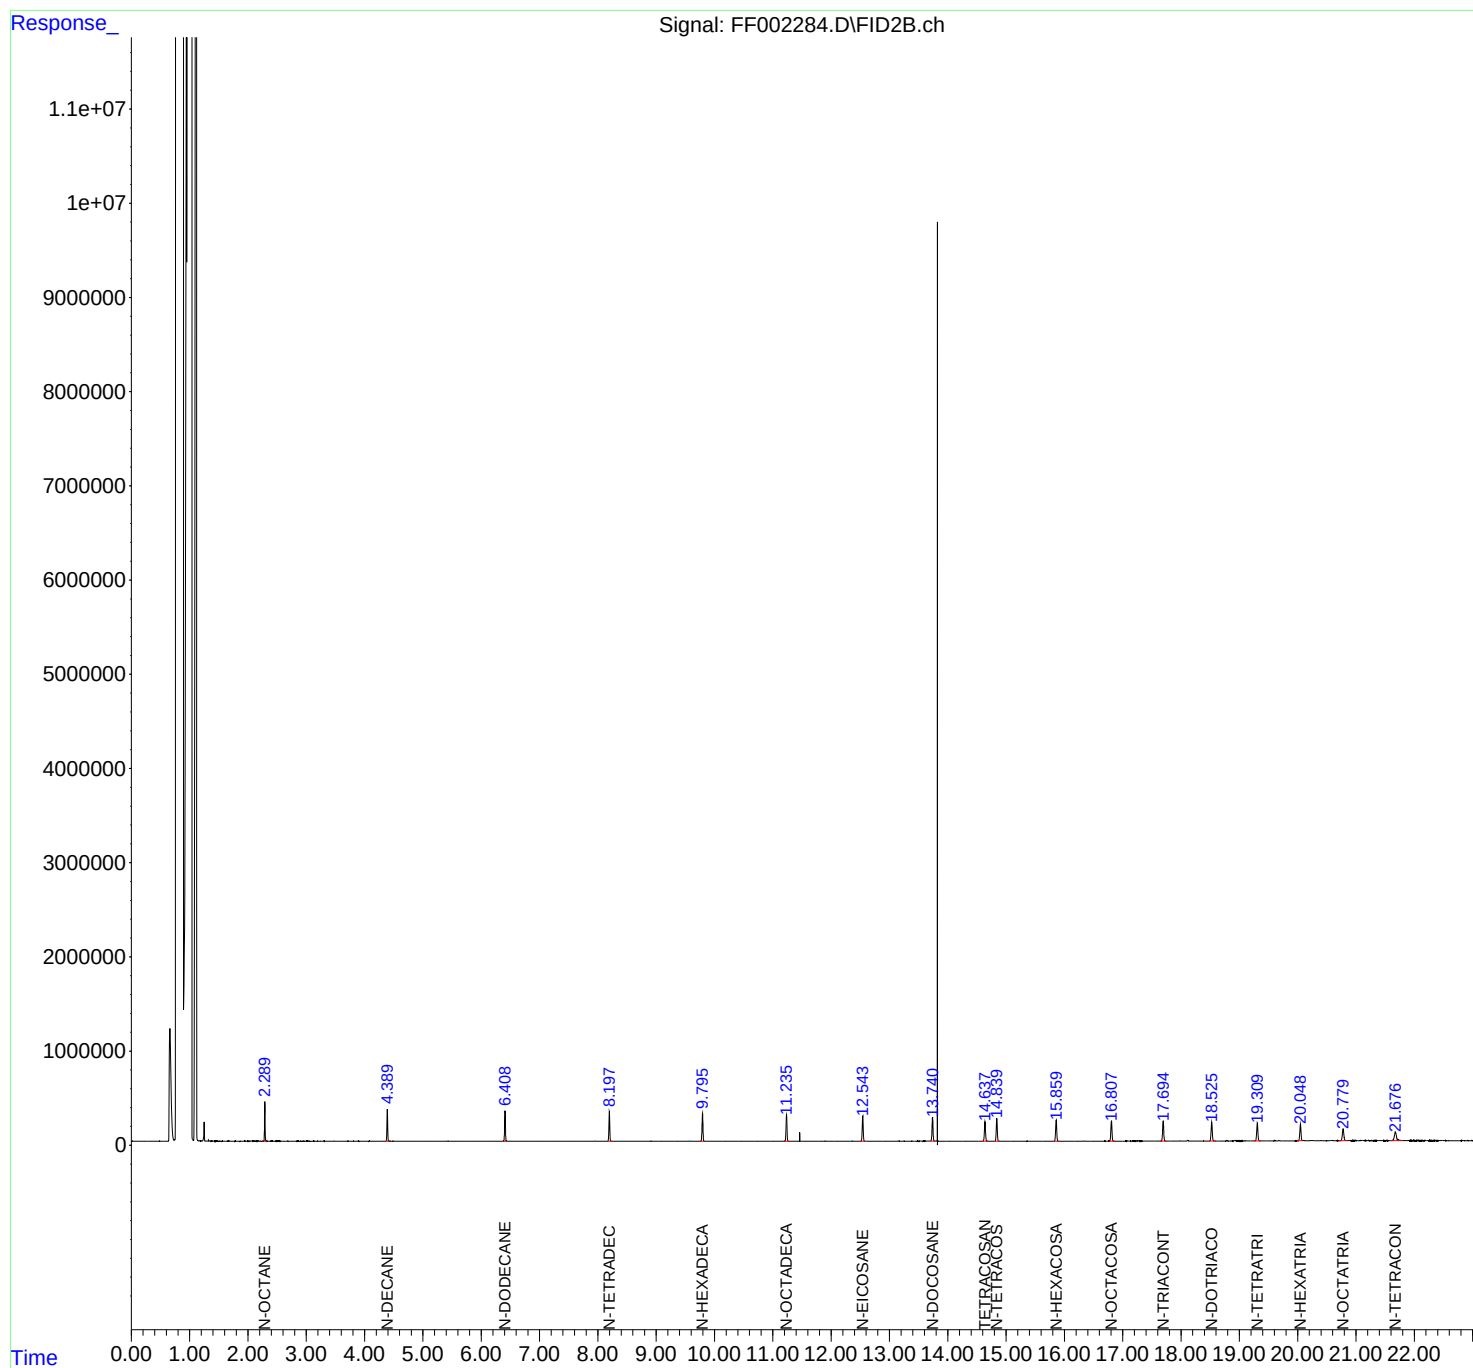


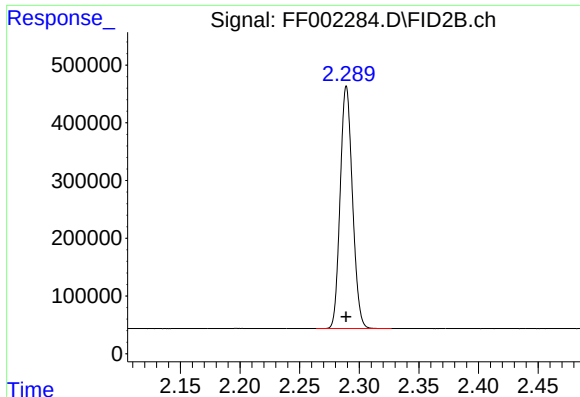

#1 N-OCTANE


R.T.: 2.289 min
Delta R.T.: 0.000 min
Response: 3008786
Conc: 19.03 ug/ml

Instrument :
FID_F
ClientSampleId :

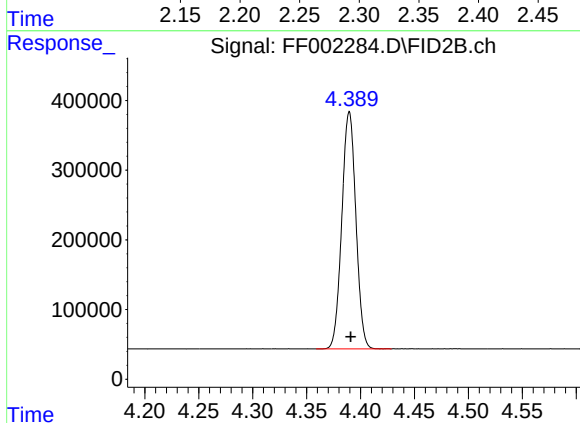


#2 N-DECANE

R.T.: 4.390 min
Delta R.T.: -0.001 min
Response: 3091464
Conc: 19.08 ug/ml

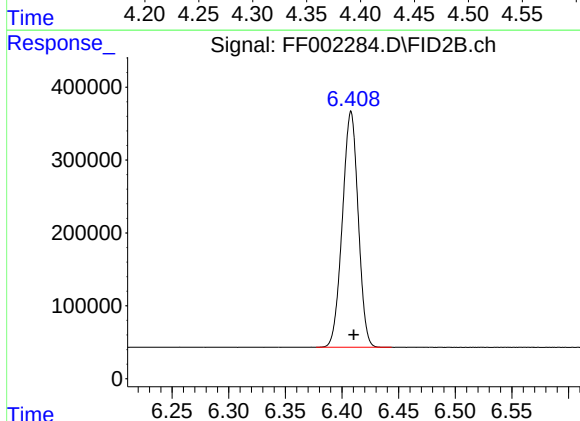


#3 N-DODECANE

R.T.: 6.408 min
Delta R.T.: -0.003 min
Response: 3145875
Conc: 19.12 ug/ml

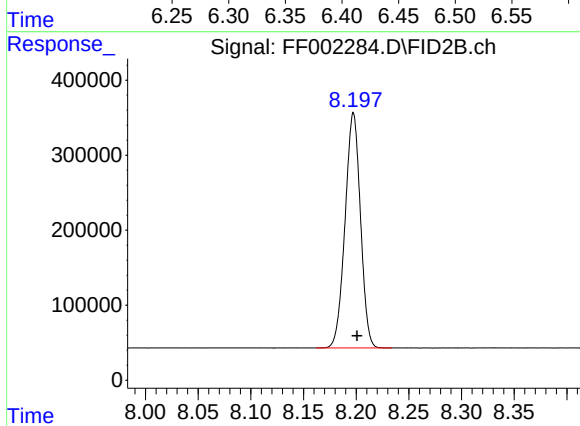

#4 N-TETRADECANE


R.T.: 8.197 min
Delta R.T.: -0.003 min
Response: 3192152
Conc: 19.16 ug/ml

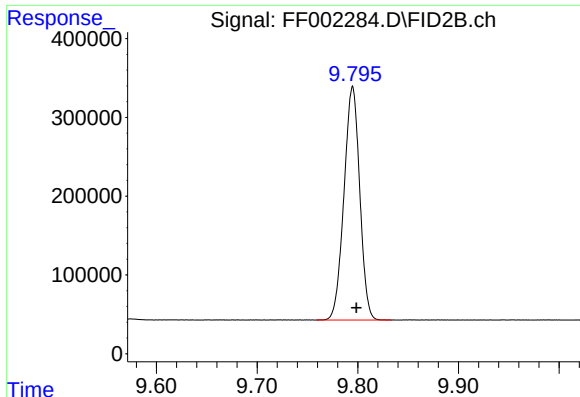

#5 N-HEXADECANE


R.T.: 9.795 min
Delta R.T.: -0.004 min
Response: 3217959
Conc: 19.21 ug/ml

Instrument :
FID_F
ClientSampleId :

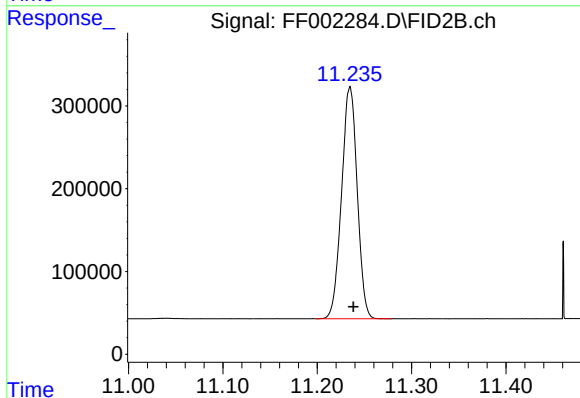


#6 N-OCTADECANE

R.T.: 11.235 min
Delta R.T.: -0.004 min
Response: 3230607
Conc: 19.24 ug/ml

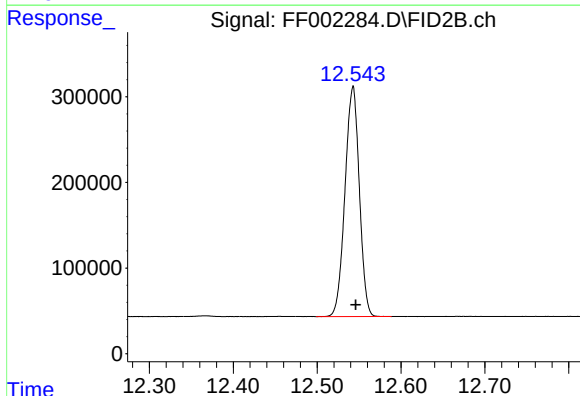


#7 N-EICOSANE

R.T.: 12.543 min
Delta R.T.: -0.003 min
Response: 3191964
Conc: 19.27 ug/ml

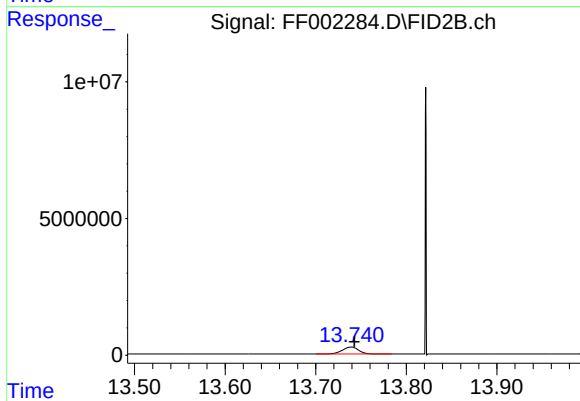

#8 N-DOCOSANE


R.T.: 13.739 min
Delta R.T.: -0.003 min
Response: 3138975
Conc: 19.24 ug/ml

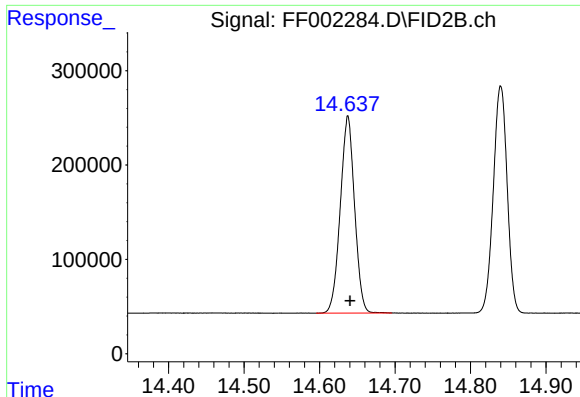

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.638 min
Delta R.T.: -0.003 min
Response: 2747898
Conc: 19.27 ug/ml

Instrument :
FID_F
ClientSampleId :

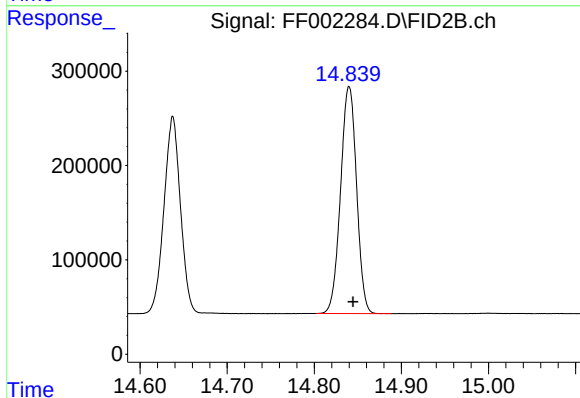


#10 N-TETRACOSANE

R.T.: 14.840 min
Delta R.T.: -0.005 min
Response: 3071739
Conc: 19.21 ug/ml

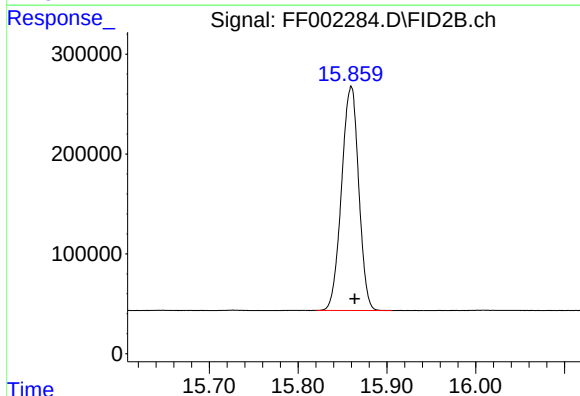


#11 N-HEXACOSANE

R.T.: 15.860 min
Delta R.T.: -0.004 min
Response: 3014667
Conc: 19.25 ug/ml

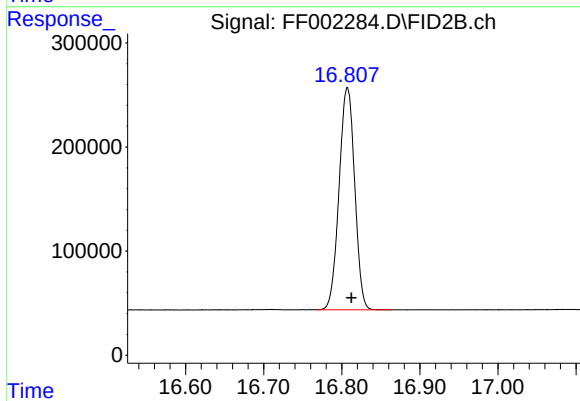

#12 N-OCTACOSANE


R.T.: 16.807 min
Delta R.T.: -0.005 min
Response: 2963583
Conc: 19.37 ug/ml

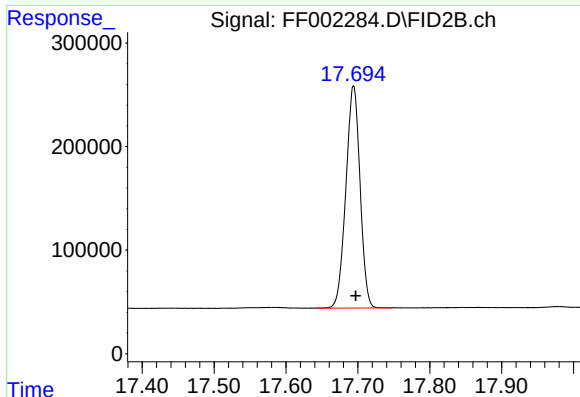

#13 N-TRIACONTANE


R.T.: 17.694 min
Delta R.T.: -0.003 min
Response: 2932041
Conc: 19.60 ug/ml

Instrument :
FID_F
ClientSampleId :

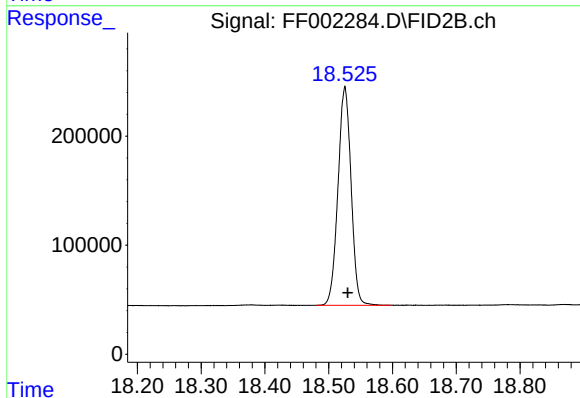


#14 N-DOTRIACONTANE

R.T.: 18.525 min
Delta R.T.: -0.004 min
Response: 2857919
Conc: 19.83 ug/ml

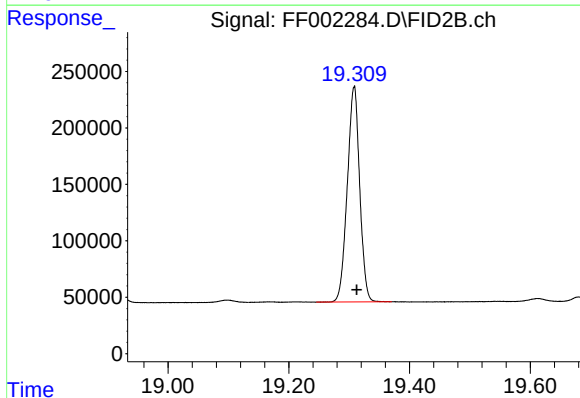


#15 N-TETRATRIACONTANE

R.T.: 19.308 min
Delta R.T.: -0.004 min
Response: 2724080
Conc: 19.61 ug/ml

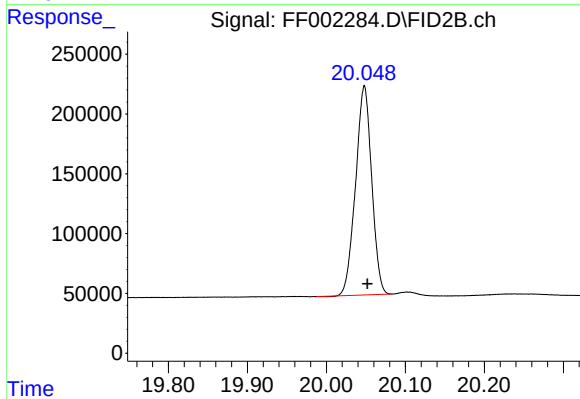

#16 N-HEXATRIACONTANE


R.T.: 20.048 min
Delta R.T.: -0.004 min
Response: 2475217
Conc: 19.21 ug/ml

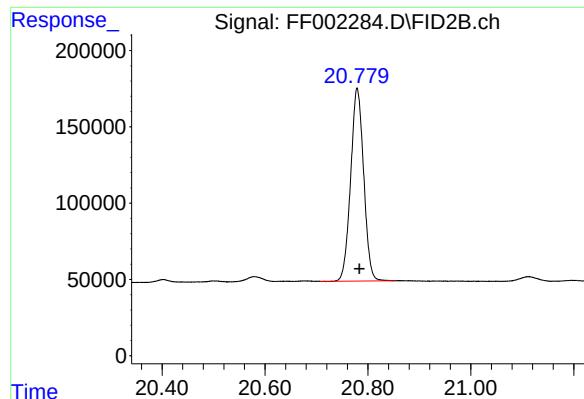

#17 N-OCTATRIACONTANE

R.T.: 20.779 min
Delta R.T.: -0.005 min
Response: 2215968
Conc: 19.40 ug/ml

Instrument :
FID_F
ClientSampleId :

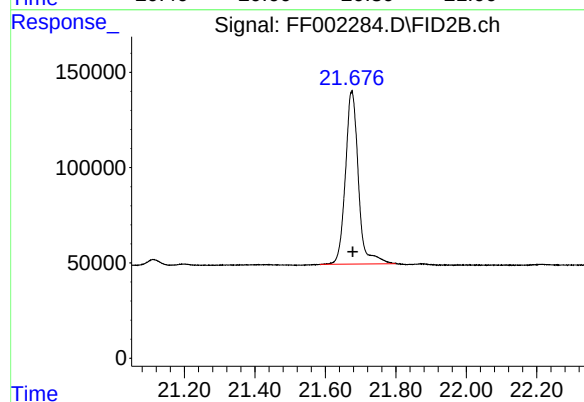

#18 N-TETRACONTANE

R.T.: 21.675 min
Delta R.T.: -0.002 min
Response: 2322977
Conc: 20.55 ug/ml