

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
 Data File : FF002287.D
 Signal(s) : FID2B.ch
 Acq On : 01 Oct 2018 16:18
 Operator : AJ\SJ
 Sample : J5155-02
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 02 03:46:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.636	3285239	23.034 ug/ml
Target Compounds			
1) N-OCTANE	2.219f	673101	4.258 ug/ml
2) N-DECANE	4.433	6317301	38.999 ug/ml
3) N-DODECANE	6.433	914954	5.562 ug/ml
4) N-TETRADECANE	8.184	788004	4.731 ug/ml
5) N-HEXADECANE	9.801	1718748	10.263 ug/ml
6) N-OCTADECANE	11.223	904464	5.387 ug/ml
7) N-EICOSANE	12.538	1357109	8.194 ug/ml
8) N-DOCOSANE	13.765	558162	3.421 ug/ml
11) N-HEXACOSANE	15.855	112142	0.716 ug/ml
12) N-OCTACOSANE	16.804	214590	1.403 ug/ml
13) N-TRIACONTANE	17.690	317407	2.122 ug/ml
14) N-DOTRIACONTANE	18.521	263807	1.830 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
Data File : FF002287.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2018 16:18
Operator : AJ\SJ
Sample : J5155-02
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 02 03:46:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

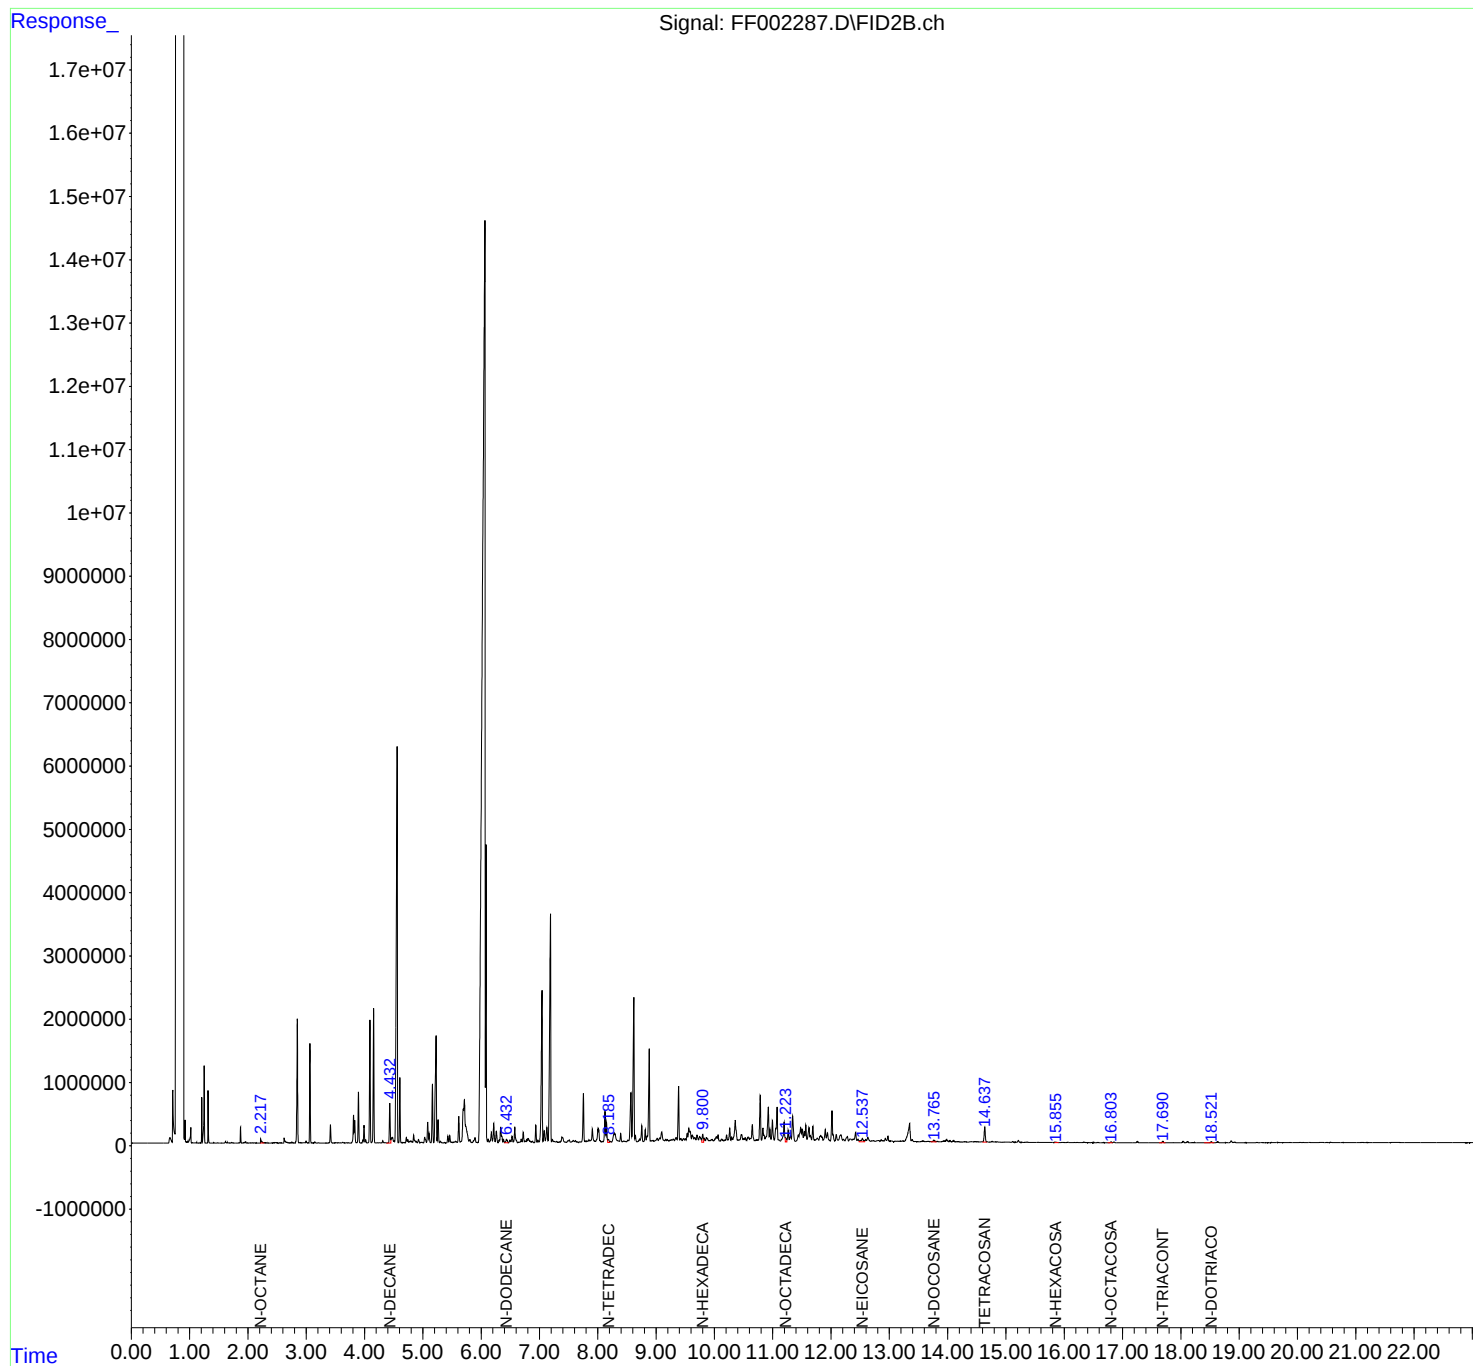


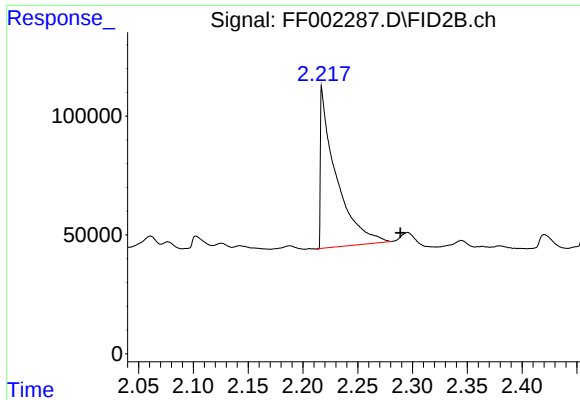

#1 N-OCTANE


R.T.: 2.219 min
Delta R.T.: -0.070 min
Response: 673101
Conc: 4.26 ug/ml

Instrument :
FID_F
ClientSampleId :

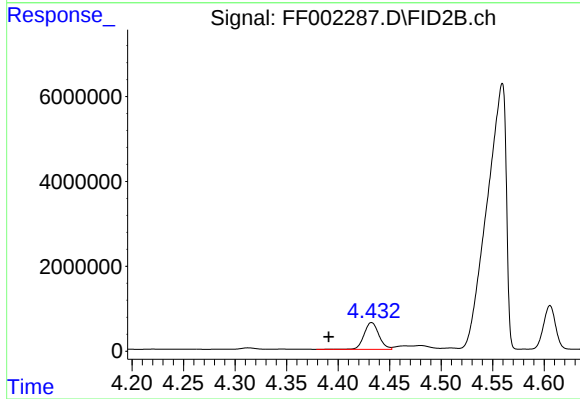


#2 N-DECANE

R.T.: 4.433 min
Delta R.T.: 0.042 min
Response: 6317301
Conc: 39.00 ug/ml

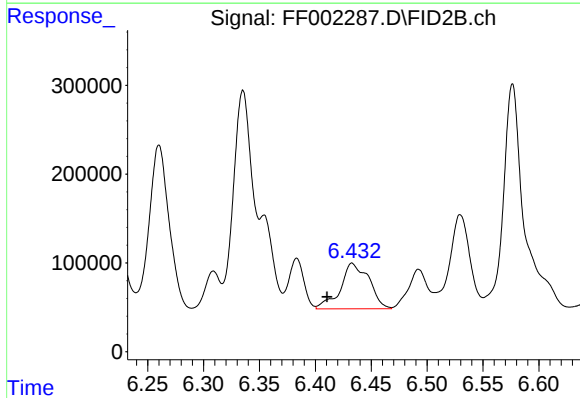


#3 N-DODECANE

R.T.: 6.433 min
Delta R.T.: 0.022 min
Response: 914954
Conc: 5.56 ug/ml

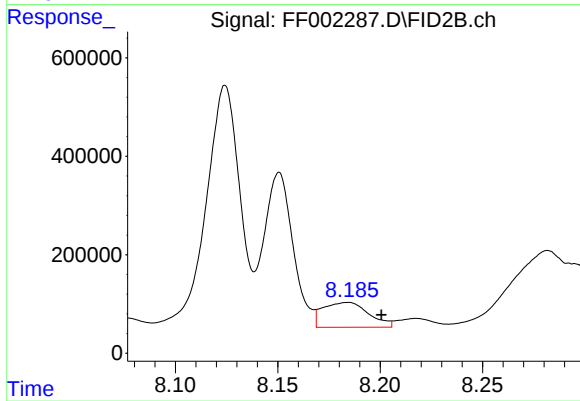

#4 N-TETRADECANE


R.T.: 8.184 min
Delta R.T.: -0.016 min
Response: 788004
Conc: 4.73 ug/ml

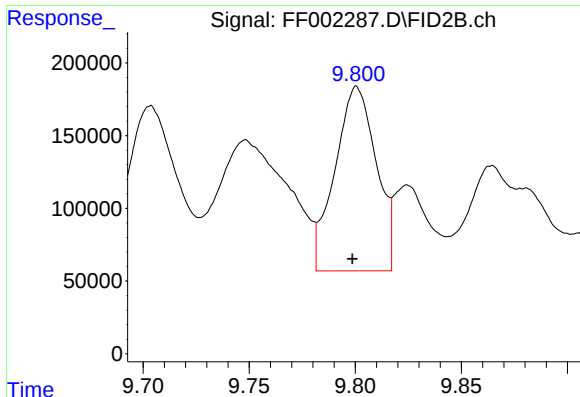

#5 N-HEXADECANE


R.T.: 9.801 min
Delta R.T.: 0.002 min
Response: 1718748
Conc: 10.26 ug/ml

Instrument :
FID_F
ClientSampleId :

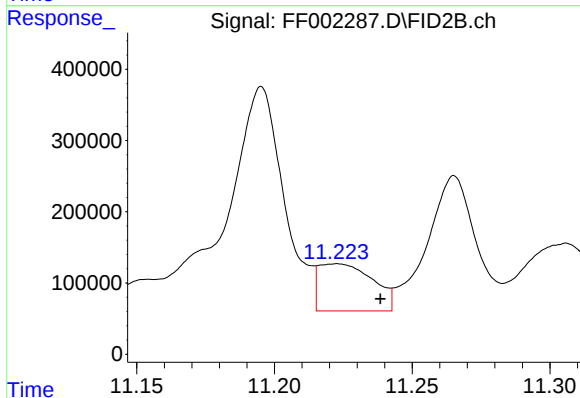


#6 N-OCTADECANE

R.T.: 11.223 min
Delta R.T.: -0.016 min
Response: 904464
Conc: 5.39 ug/ml

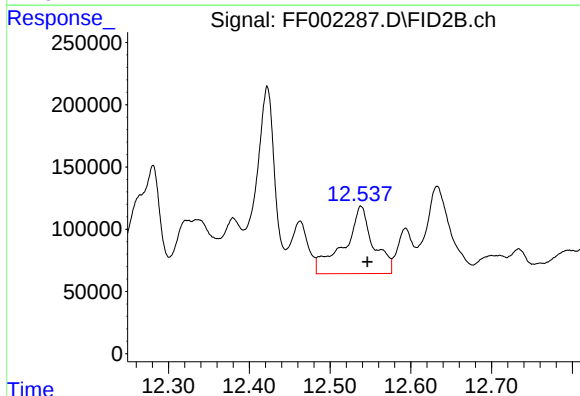


#7 N-EICOSANE

R.T.: 12.538 min
Delta R.T.: -0.008 min
Response: 1357109
Conc: 8.19 ug/ml

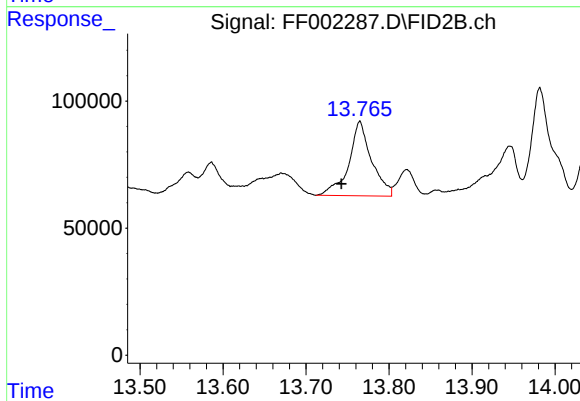

#8 N-DOCOSANE


R.T.: 13.765 min
Delta R.T.: 0.022 min
Response: 558162
Conc: 3.42 ug/ml

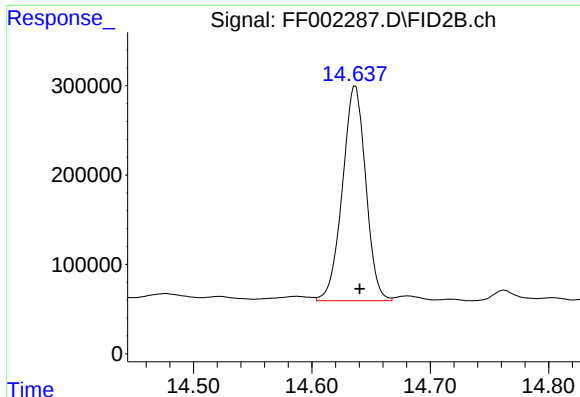

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.636 min
Delta R.T.: -0.004 min
Response: 3285239
Conc: 23.03 ug/ml

Instrument :
FID_F
ClientSampleId :

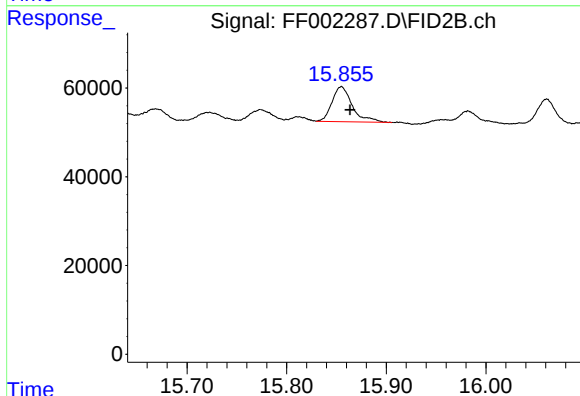


#11 N-HEXACOSANE

R.T.: 15.855 min
Delta R.T.: -0.009 min
Response: 112142
Conc: 0.72 ug/ml

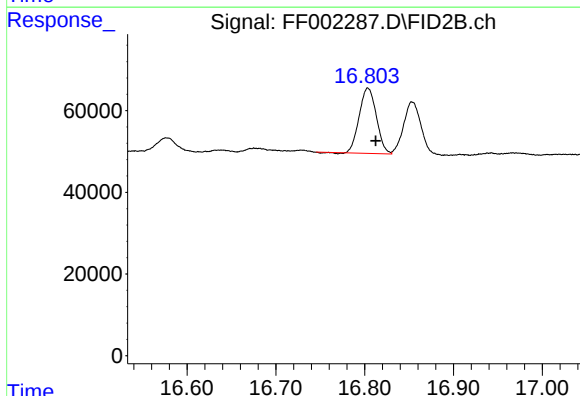


#12 N-OCTACOSANE

R.T.: 16.804 min
Delta R.T.: -0.009 min
Response: 214590
Conc: 1.40 ug/ml

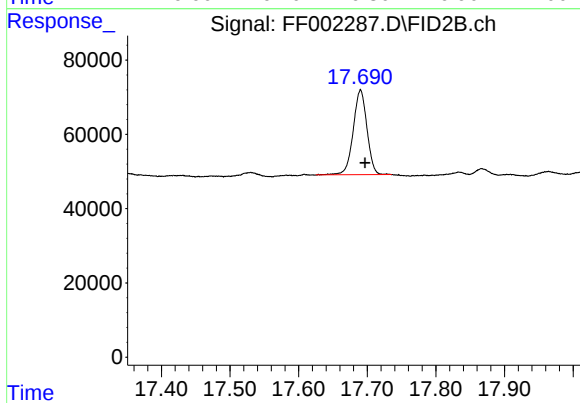

#13 N-TRIACONTANE

R.T.: 17.690 min
Delta R.T.: -0.007 min
Response: 317407
Conc: 2.12 ug/ml

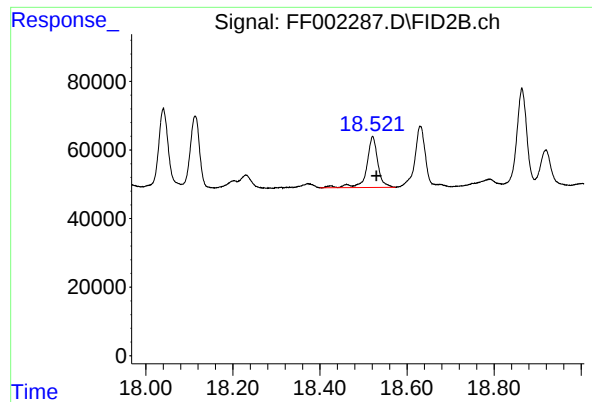

#14 N-DOTRIACONTANE

R.T.: 18.521 min
Delta R.T.: -0.009 min
Response: 263807
Conc: 1.83 ug/ml

Instrument :
FID_F
ClientSampleId :