

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
 Data File : FF002288.D
 Signal(s) : FID2B.ch
 Acq On : 01 Oct 2018 16:50
 Operator : AJ\SJ
 Sample : J5155-03
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 02 03:46:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.638	3427230	24.030 ug/ml
Target Compounds			
1) N-OCTANE	2.290	216443	1.369 ug/ml
2) N-DECANE	4.374	2802416	17.300 ug/ml
3) N-DODECANE	6.403	1236913	7.519 ug/ml
4) N-TETRADECANE	8.188	8068978	48.440 ug/ml
5) N-HEXADECANE	9.801	22314918	133.245 ug/ml
6) N-OCTADECANE	11.236	25128148	149.654 ug/ml
7) N-EICOSANE	12.561	1324602	7.998 ug/ml
8) N-DOCOSANE	13.747	940820	5.766 ug/ml
10) N-TETRACOSANE	14.856	1038135	6.492 ug/ml
11) N-HEXACOSANE	15.858	551885	3.524 ug/ml
12) N-OCTACOSANE	16.805	274654	1.795 ug/ml
13) N-TRIACONTANE	17.690	381555	2.551 ug/ml
14) N-DOTRIACONTANE	18.522	266645	1.850 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
Data File : FF002288.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2018 16:50
Operator : AJ\SJ
Sample : J5155-03
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 02 03:46:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

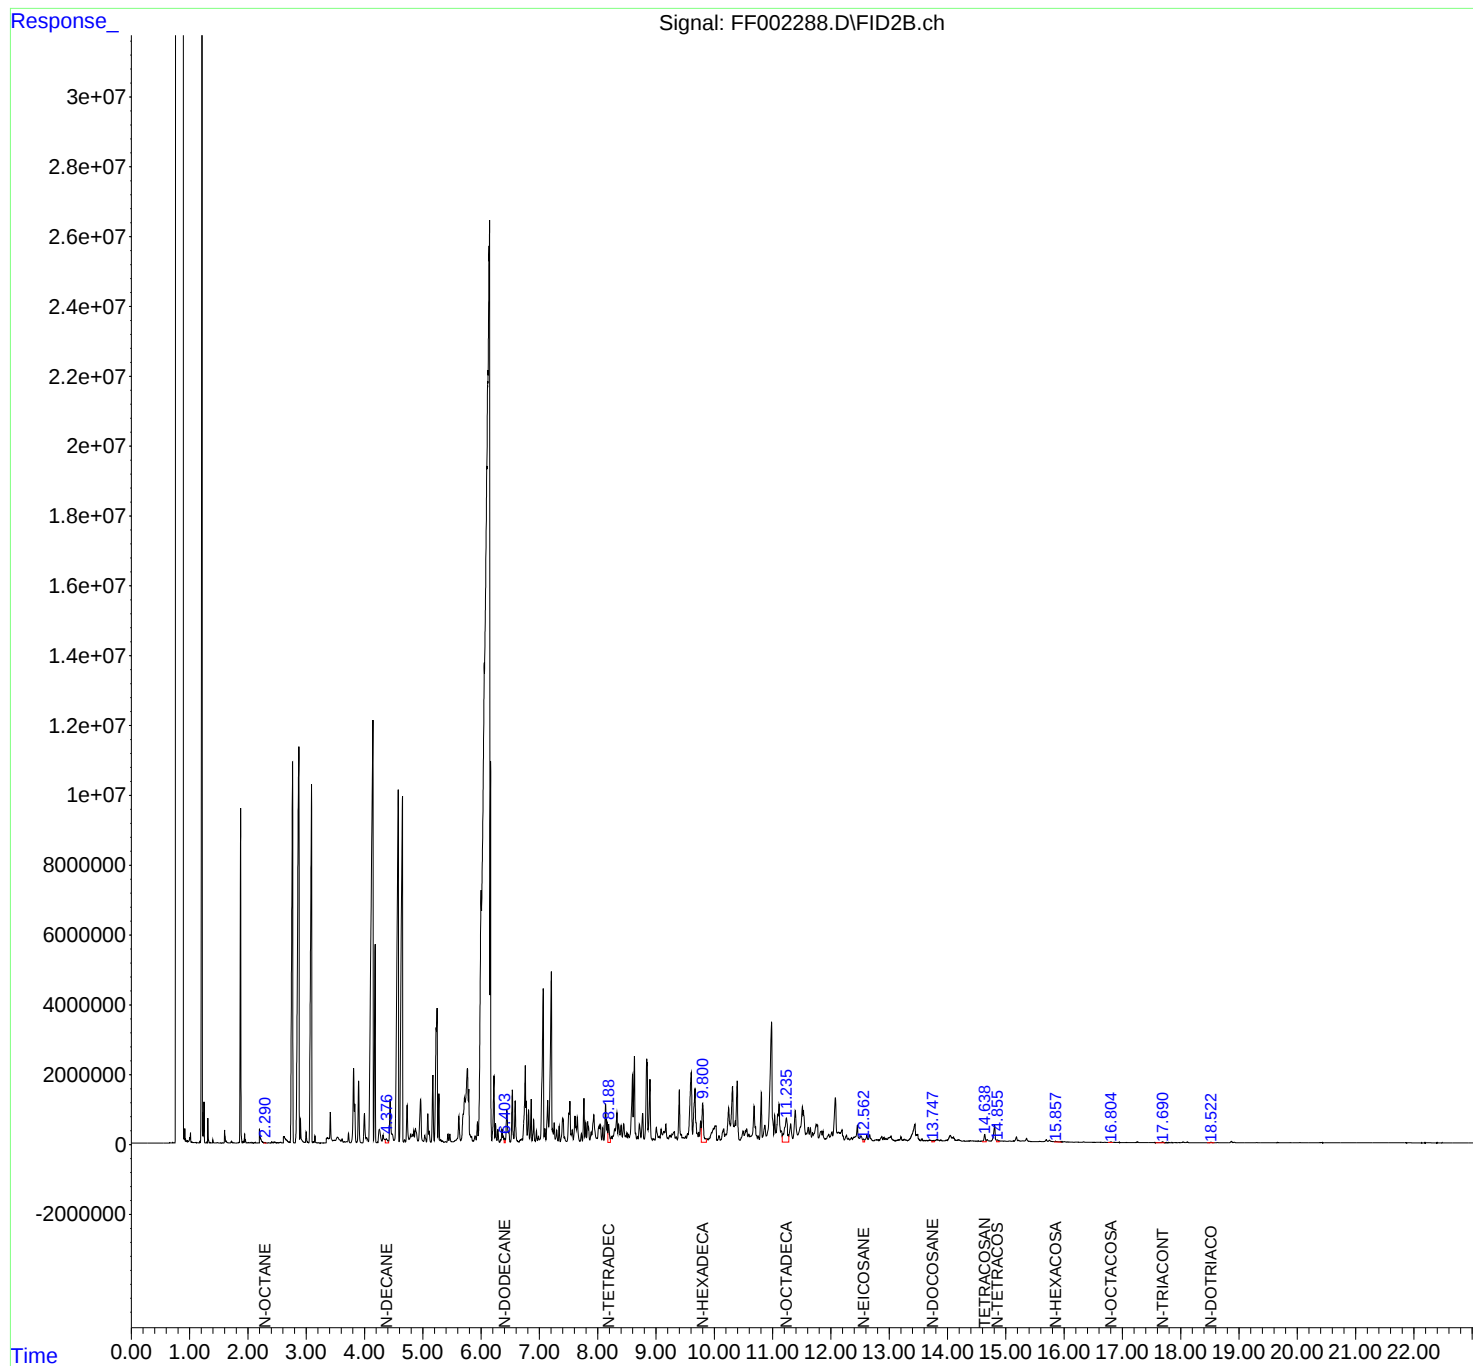


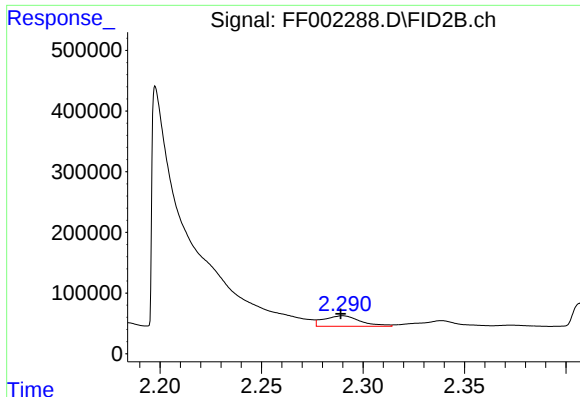

#1 N-OCTANE


R.T.: 2.290 min
Delta R.T.: 0.001 min
Response: 216443
Conc: 1.37 ug/ml

Instrument :
FID_F
ClientSampleId :

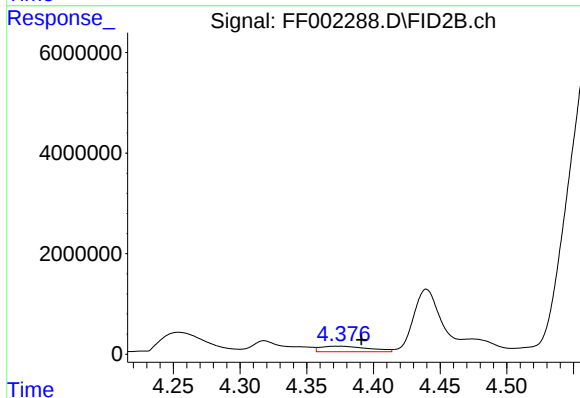


#2 N-DECANE

R.T.: 4.374 min
Delta R.T.: -0.017 min
Response: 2802416
Conc: 17.30 ug/ml

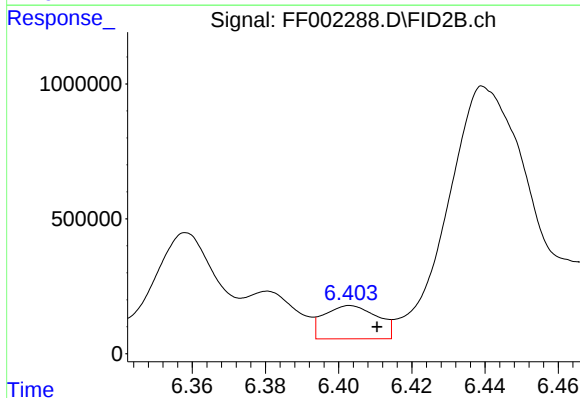


#3 N-DODECANE

R.T.: 6.403 min
Delta R.T.: -0.007 min
Response: 1236913
Conc: 7.52 ug/ml

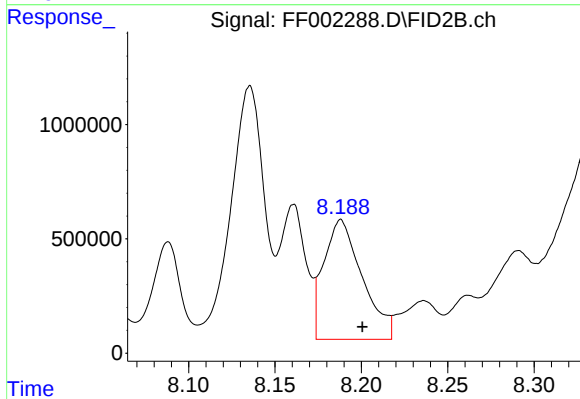

#4 N-TETRADECANE


R.T.: 8.188 min
Delta R.T.: -0.013 min
Response: 8068978
Conc: 48.44 ug/ml

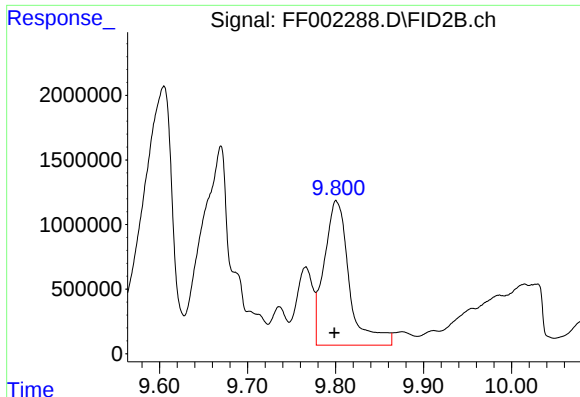

#5 N-HEXADECANE


R.T.: 9.801 min
Delta R.T.: 0.003 min
Response: 22314918
Conc: 133.24 ug/ml

Instrument :
FID_F
ClientSampleId :

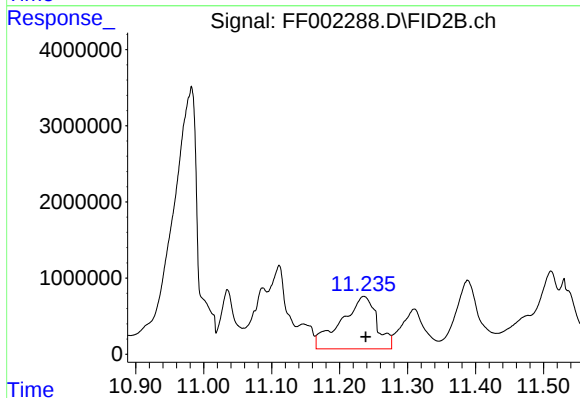


#6 N-OCTADECANE

R.T.: 11.236 min
Delta R.T.: -0.003 min
Response: 25128148
Conc: 149.65 ug/ml

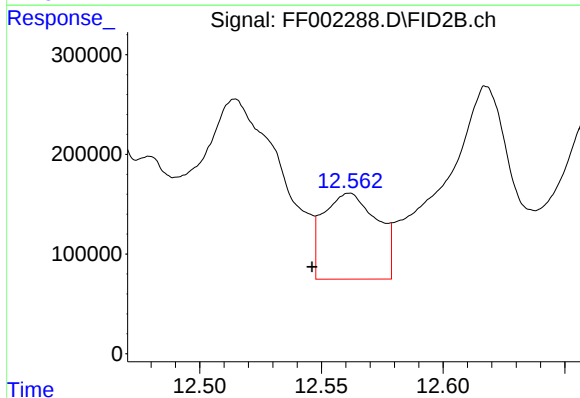


#7 N-EICOSANE

R.T.: 12.561 min
Delta R.T.: 0.015 min
Response: 1324602
Conc: 8.00 ug/ml

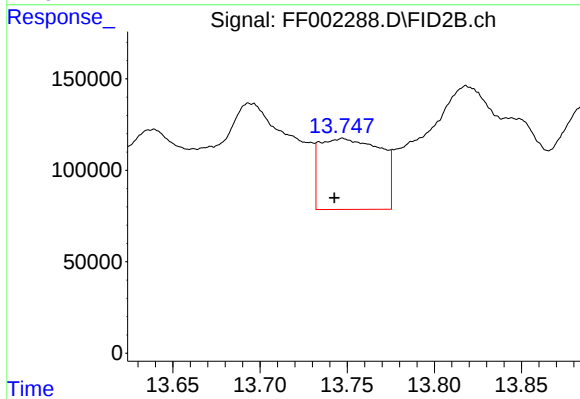

#8 N-DOCOSANE


R.T.: 13.747 min
Delta R.T.: 0.005 min
Response: 940820
Conc: 5.77 ug/ml

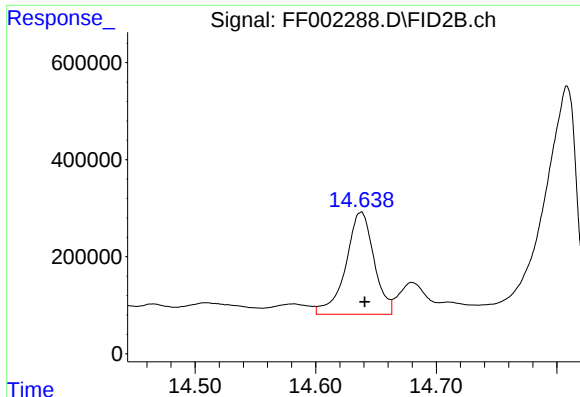

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.638 min
Delta R.T.: -0.003 min
Response: 3427230
Conc: 24.03 ug/ml

Instrument :
FID_F
ClientSampleId :

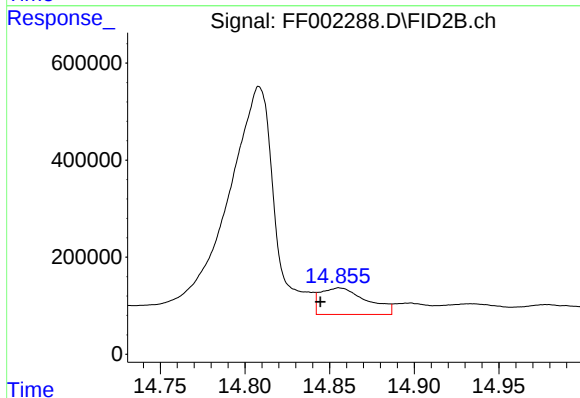


#10 N-TETRACOSANE

R.T.: 14.856 min
Delta R.T.: 0.011 min
Response: 1038135
Conc: 6.49 ug/ml

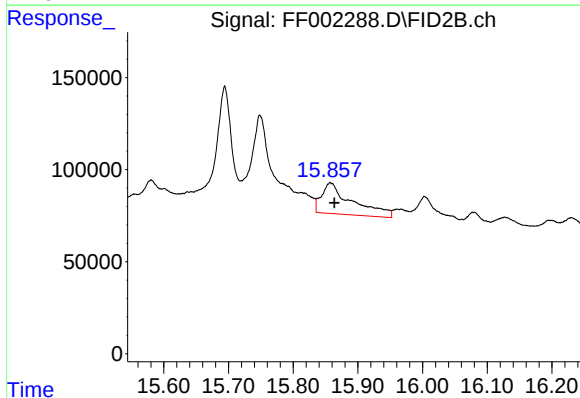


#11 N-HEXACOSANE

R.T.: 15.858 min
Delta R.T.: -0.006 min
Response: 551885
Conc: 3.52 ug/ml

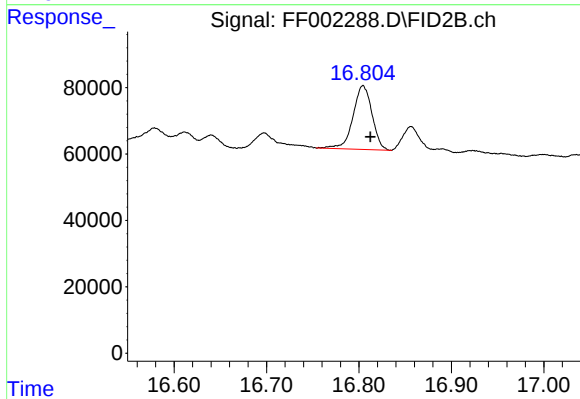

#12 N-OCTACOSANE


R.T.: 16.805 min
Delta R.T.: -0.008 min
Response: 274654
Conc: 1.80 ug/ml

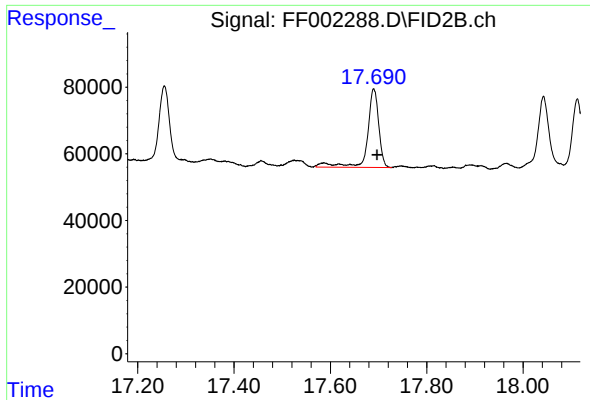

#13 N-TRIACONTANE

R.T.: 17.690 min
Delta R.T.: -0.007 min
Response: 381555
Conc: 2.55 ug/ml

Instrument :
FID_F
ClientSampleId :

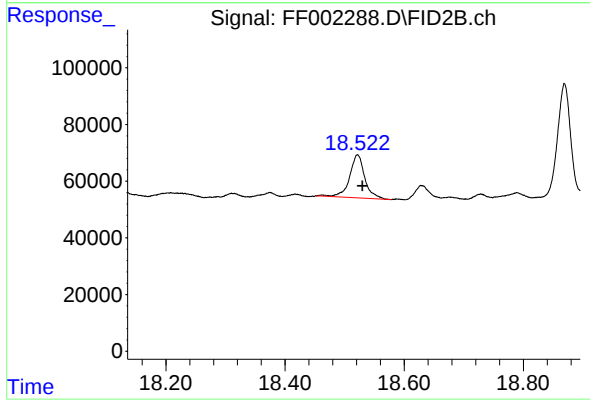

#14 N-DOTRIACONTANE

R.T.: 18.522 min
Delta R.T.: -0.008 min
Response: 266645
Conc: 1.85 ug/ml