

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
 Data File : FF002275.D
 Signal(s) : FID2B.ch
 Acq On : 01 Oct 2018 10:11
 Operator : AJ\SJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 TRPH STD

Integration File: Sample.e
 Quant Time: Oct 01 11:40:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 11:39:55 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.640	6616282	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.289	7449793	50.000 ug/ml
2) N-DECANE	4.391	7674750	50.000 ug/ml
3) N-DODECANE	6.411	7795901	50.000 ug/ml
4) N-TETRADECANE	8.201	7873780	50.000 ug/ml
5) N-HEXADECANE	9.799	7902952	50.000 ug/ml
6) N-OCTADECANE	11.238	7894033	50.000 ug/ml
7) N-EICOSANE	12.546	7751327	50.000 ug/ml
8) N-DOCOSANE	13.743	7592808	50.000 ug/ml
10) N-TETRACOSANE	14.845	7407511	50.000 ug/ml
11) N-HEXACOSANE	15.864	7235462	50.000 ug/ml
12) N-OCTACOSANE	16.812	7035966	50.000 ug/ml
13) N-TRIACONTANE	17.697	6846242	50.000 ug/ml
14) N-DOTRIACONTANE	18.530	6552347	50.000 ug/ml
15) N-TETRATRIACONTANE	19.312	6357421	50.000 ug/ml
16) N-HEXATRIACONTANE	20.052	5948774	50.000 ug/ml
17) N-OCTATRIACONTANE	20.784	5311576	50.000 ug/ml
18) N-TETRACONTANE	21.678	5465698	50.000 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
Data File : FF002275.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2018 10:11
Operator : AJ\SJ
Sample : 50 TRPH STD
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

Integration File: Sample.e
Quant Time: Oct 01 11:40:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 11:39:55 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

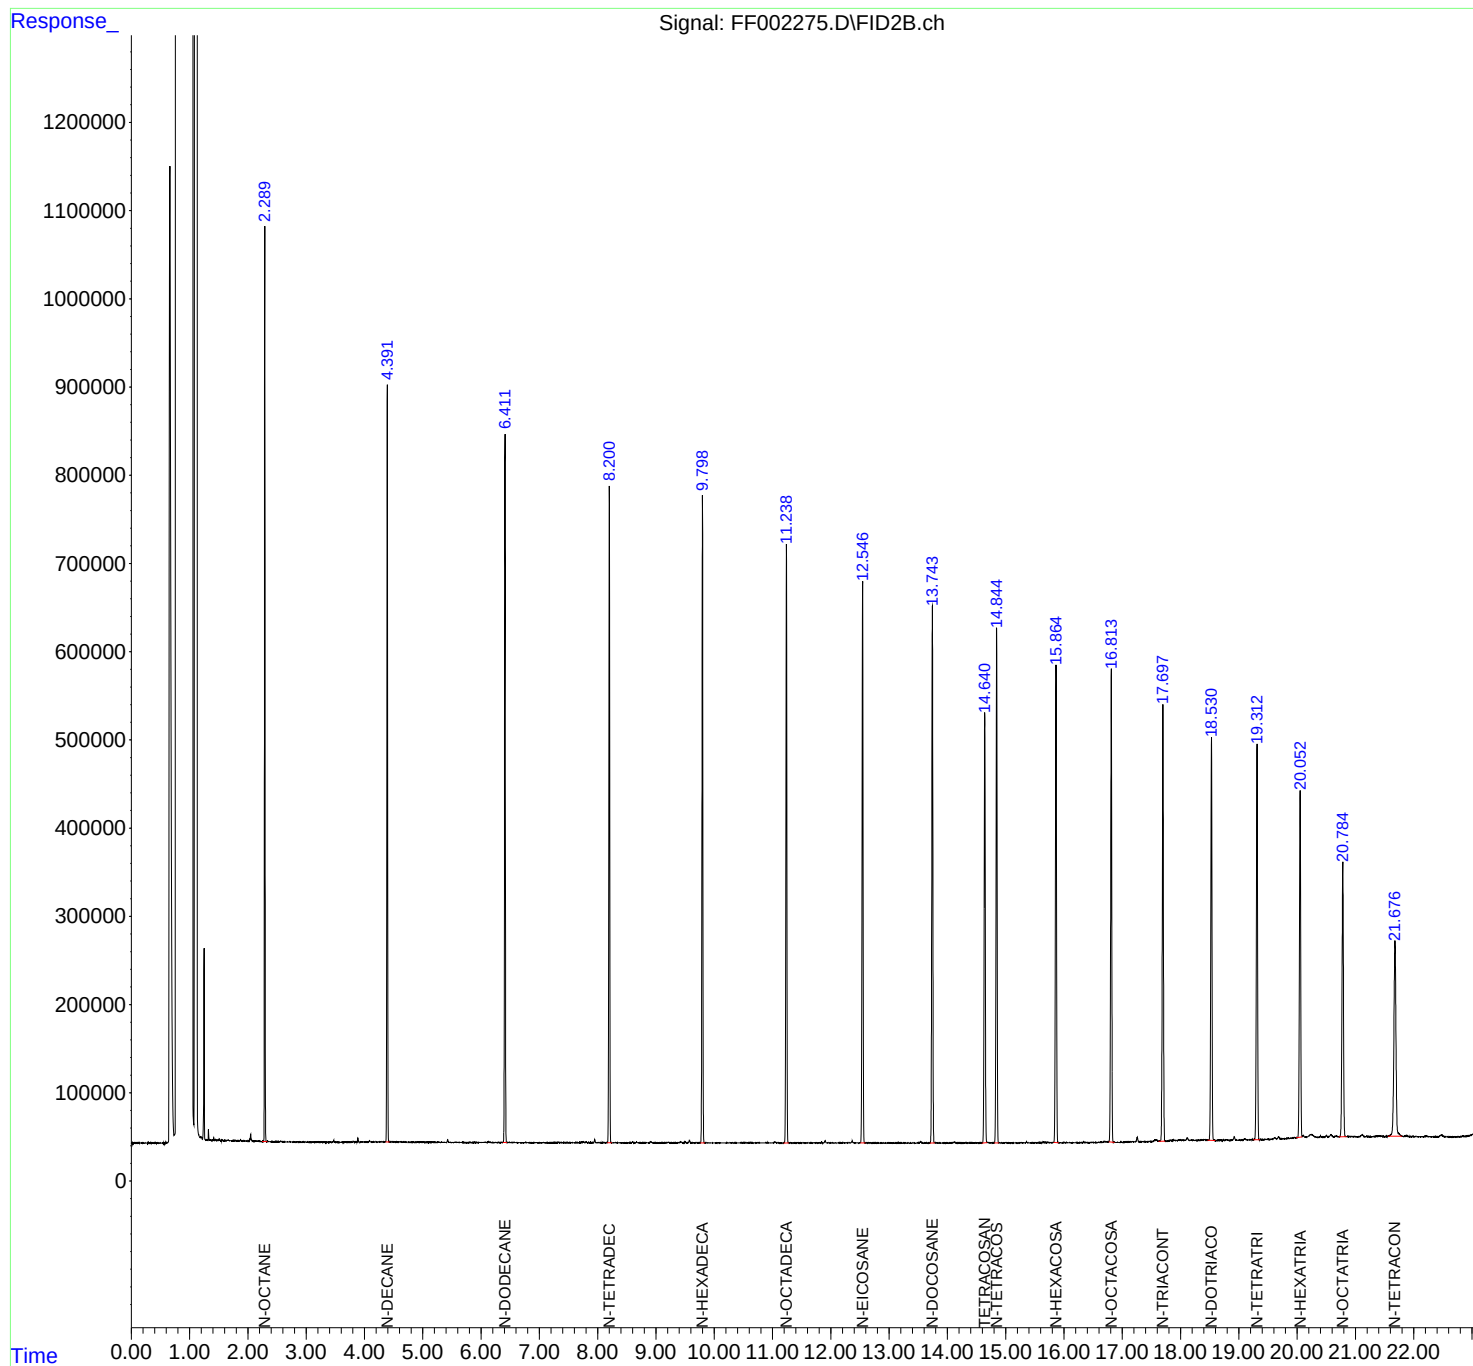


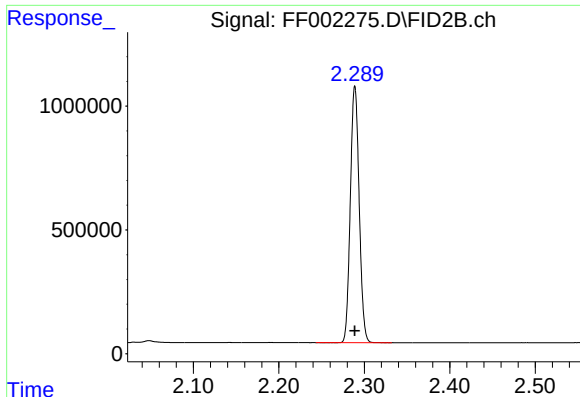

#1 N-OCTANE


R.T.: 2.289 min
Delta R.T.: 0.000 min
Response: 7449793
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

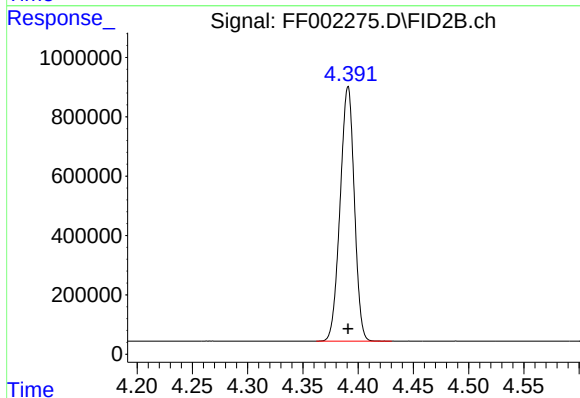


#2 N-DECANE

R.T.: 4.391 min
Delta R.T.: 0.000 min
Response: 7674750
Conc: 50.00 ug/ml

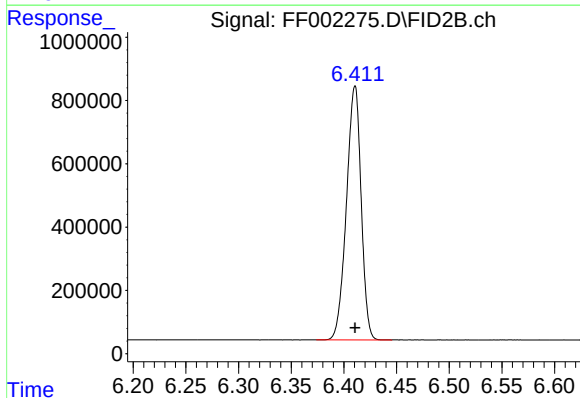


#3 N-DODECANE

R.T.: 6.411 min
Delta R.T.: 0.000 min
Response: 7795901
Conc: 50.00 ug/ml

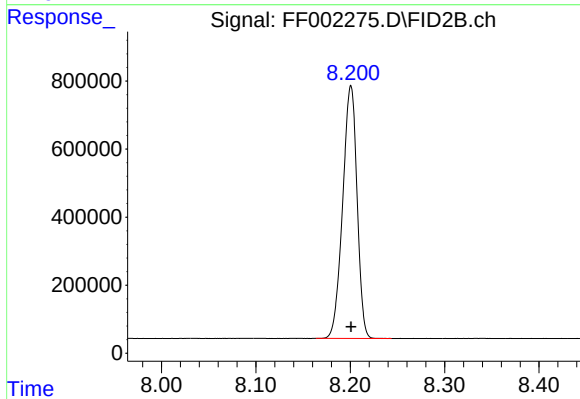

#4 N-TETRADECANE


R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 7873780
Conc: 50.00 ug/ml

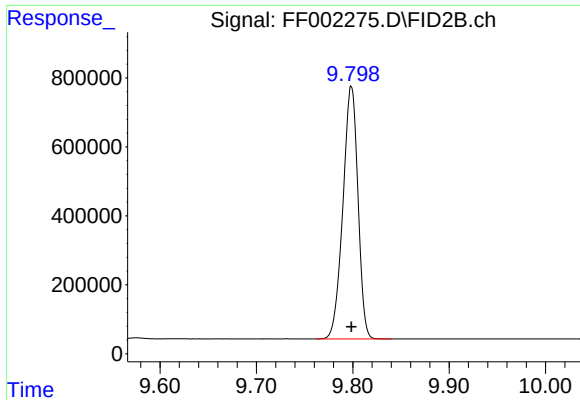

#5 N-HEXADECANE


R.T.: 9.799 min
Delta R.T.: 0.000 min
Response: 7902952
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

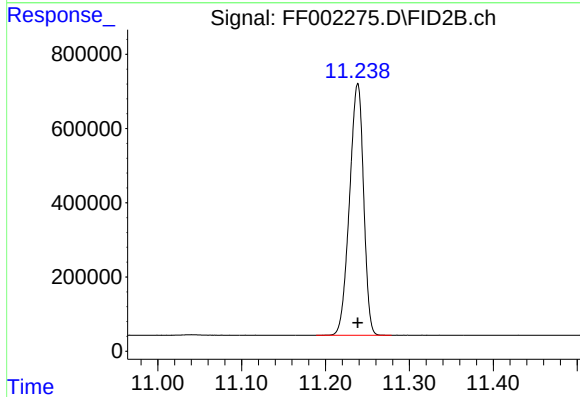


#6 N-OCTADECANE

R.T.: 11.238 min
Delta R.T.: 0.000 min
Response: 7894033
Conc: 50.00 ug/ml

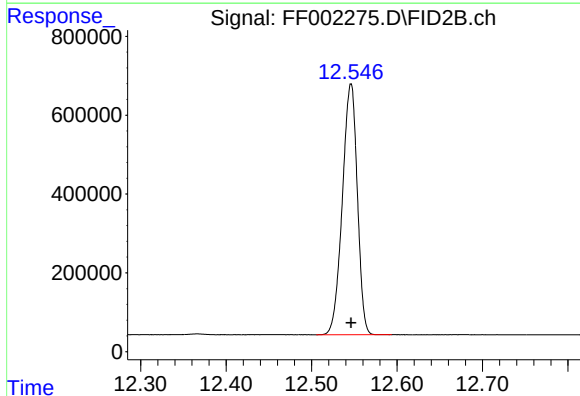


#7 N-EICOSANE

R.T.: 12.546 min
Delta R.T.: 0.000 min
Response: 7751327
Conc: 50.00 ug/ml

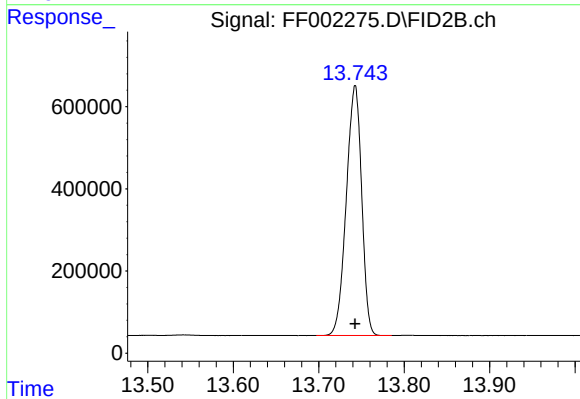

#8 N-DOCOSANE


R.T.: 13.743 min
Delta R.T.: 0.000 min
Response: 7592808
Conc: 50.00 ug/ml

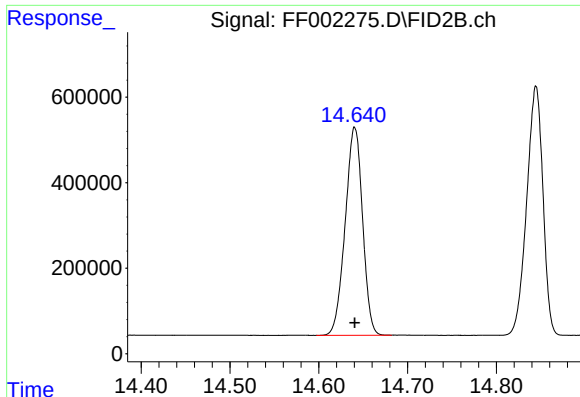

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.640 min
Delta R.T.: 0.000 min
Response: 6616282
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

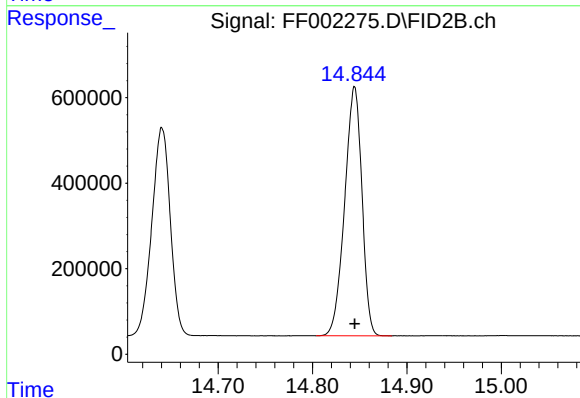


#10 N-TETRACOSANE

R.T.: 14.845 min
Delta R.T.: 0.000 min
Response: 7407511
Conc: 50.00 ug/ml

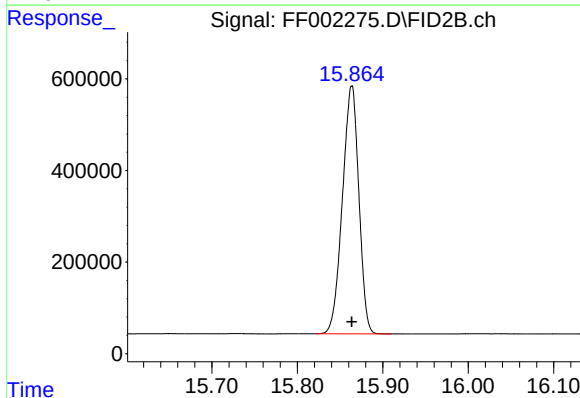


#11 N-HEXACOSANE

R.T.: 15.864 min
Delta R.T.: 0.000 min
Response: 7235462
Conc: 50.00 ug/ml

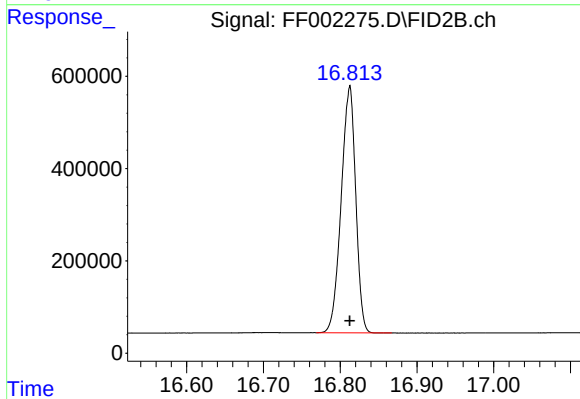

#12 N-OCTACOSANE


R.T.: 16.812 min
Delta R.T.: 0.000 min
Response: 7035966
Conc: 50.00 ug/ml

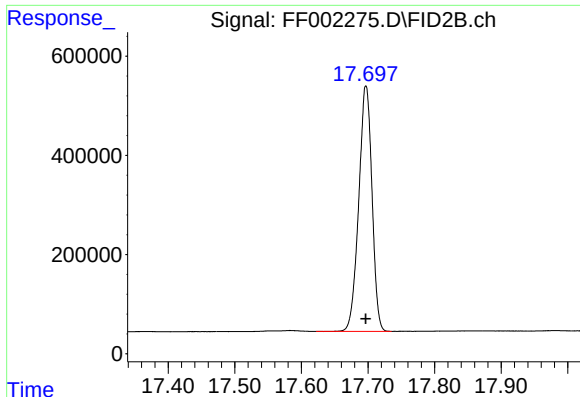

#13 N-TRIACONTANE


R.T.: 17.697 min
Delta R.T.: 0.000 min
Response: 6846242
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

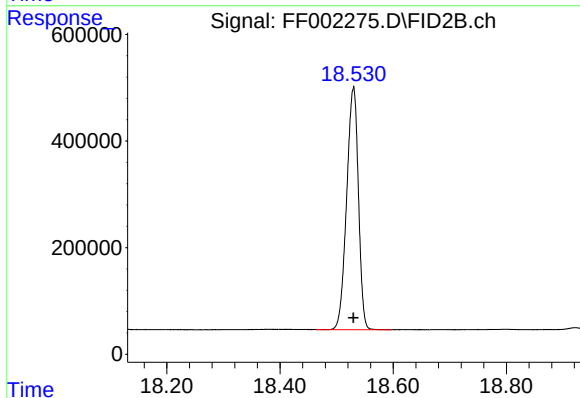


#14 N-DOTRIACONTANE

R.T.: 18.530 min
Delta R.T.: 0.000 min
Response: 6552347
Conc: 50.00 ug/ml

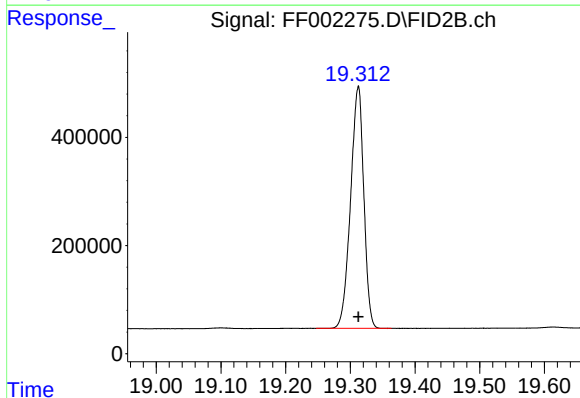


#15 N-TETRATRIACONTANE

R.T.: 19.312 min
Delta R.T.: 0.000 min
Response: 6357421
Conc: 50.00 ug/ml

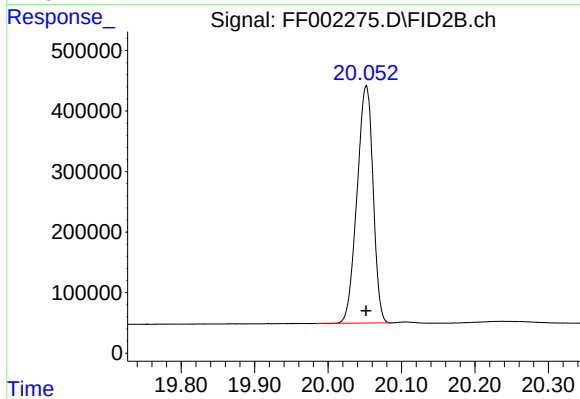

#16 N-HEXATRIACONTANE


R.T.: 20.052 min
Delta R.T.: 0.000 min
Response: 5948774
Conc: 50.00 ug/ml

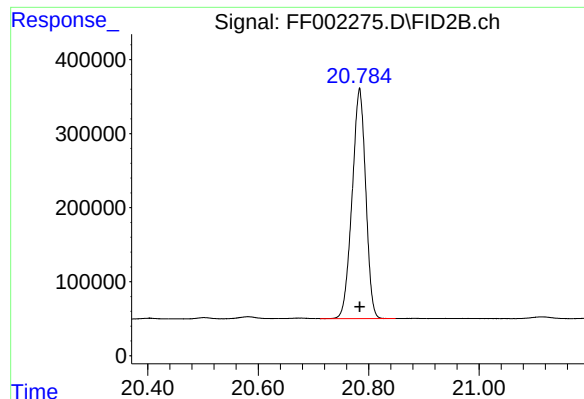

#17 N-OCTATRIACONTANE

R.T.: 20.784 min
Delta R.T.: 0.000 min
Response: 5311576
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

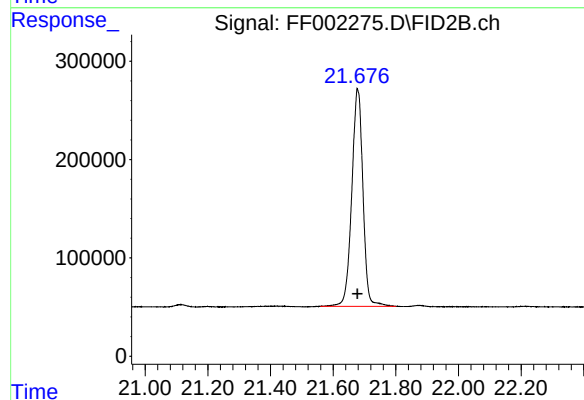

#18 N-TETRACONTANE

R.T.: 21.678 min
Delta R.T.: 0.000 min
Response: 5465698
Conc: 50.00 ug/ml