

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
 Data File : FF002279.D
 Signal(s) : FID2B.ch
 Acq On : 01 Oct 2018 12:10
 Operator : AJ\SJ
 Sample : FF100118ICV
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 FF100118ICV

Integration File: Sample.e
 Quant Time: Oct 01 12:32:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.641	6677949	46.822 ug/ml
Target Compounds			
1) N-OCTANE	2.289	7356614	46.540 ug/ml
2) N-DECANE	4.391	7539244	46.542 ug/ml
3) N-DODECANE	6.411	7665820	46.600 ug/ml
4) N-TETRADECANE	8.201	7765166	46.616 ug/ml
5) N-HEXADECANE	9.799	7838757	46.806 ug/ml
6) N-OCTADECANE	11.238	7868410	46.861 ug/ml
7) N-EICOSANE	12.546	7767441	46.900 ug/ml
8) N-DOCOSANE	13.743	7646685	46.863 ug/ml
10) N-TETRACOSANE	14.845	7480546	46.783 ug/ml
11) N-HEXACOSANE	15.864	7332892	46.818 ug/ml
12) N-OCTACOSANE	16.813	7154886	46.773 ug/ml
13) N-TRIACONTANE	17.700	6986853	46.710 ug/ml
14) N-DOTRIACONTANE	18.533	6758988	46.898 ug/ml
15) N-TETRATRIACONTANE	19.315	6540901	47.096 ug/ml
16) N-HEXATRIACONTANE	20.055	6176950	47.941 ug/ml
17) N-OCTATRIACONTANE	20.787	5479275	47.970 ug/ml
18) N-TETRACONTANE	21.684	5605479	49.596 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
Data File : FF002279.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2018 12:10
Operator : AJ\SJ
Sample : FF100118ICV
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
FF100118ICV

Integration File: Sample.e
Quant Time: Oct 01 12:32:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

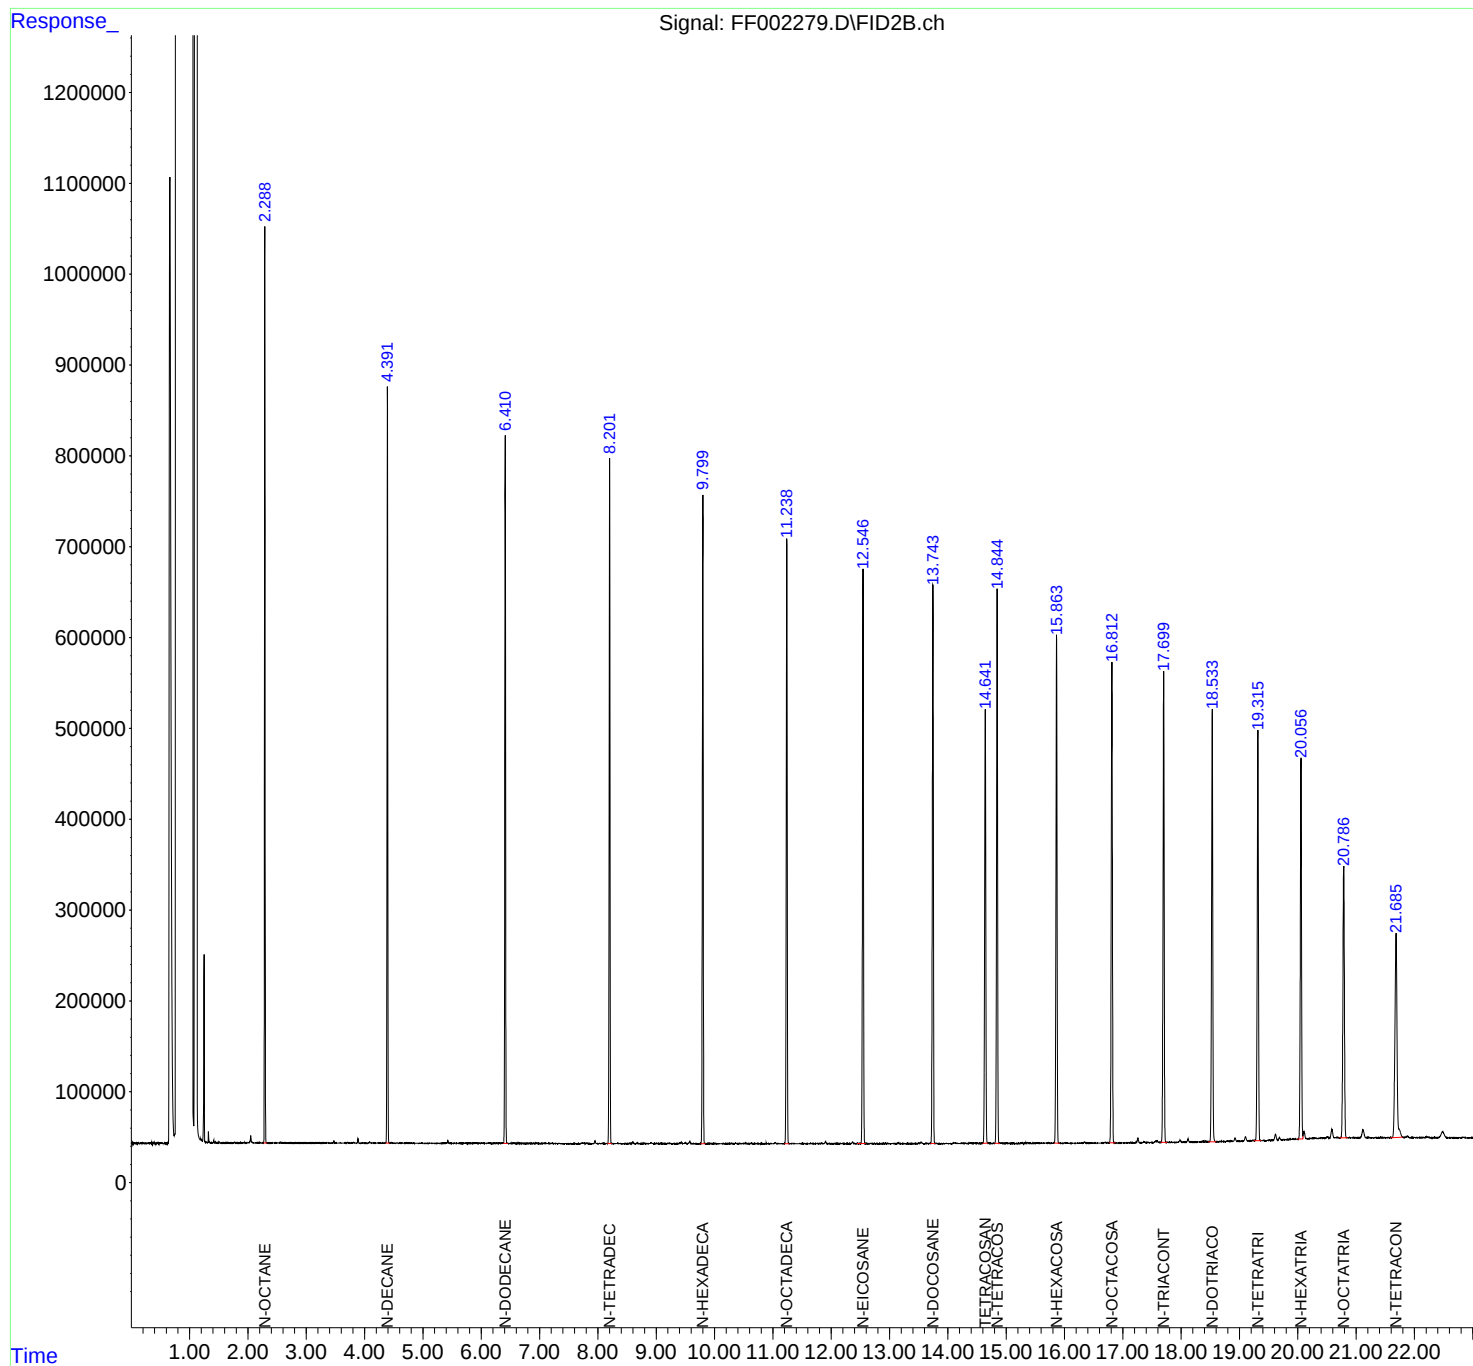


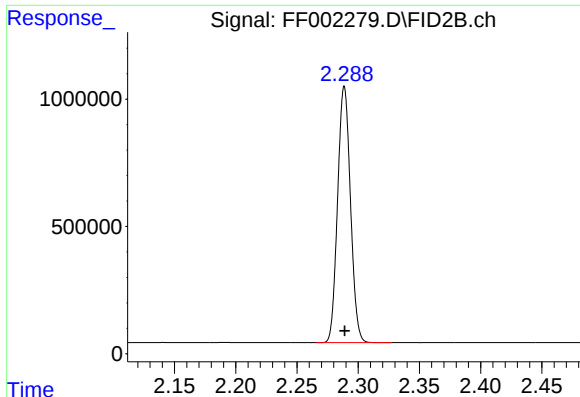

#1 N-OCTANE


R.T.: 2.289 min
Delta R.T.: 0.000 min
Response: 7356614
Conc: 46.54 ug/ml

Instrument :
FID_F
ClientSampleId :
FF100118ICV

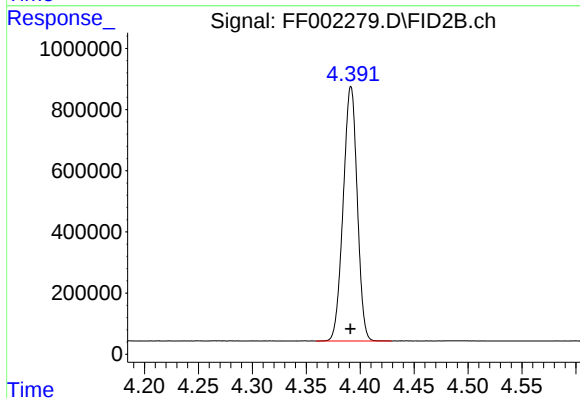


#2 N-DECANE

R.T.: 4.391 min
Delta R.T.: 0.000 min
Response: 7539244
Conc: 46.54 ug/ml

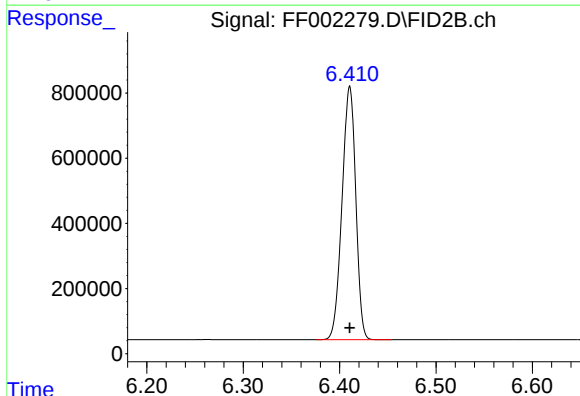


#3 N-DODECANE

R.T.: 6.411 min
Delta R.T.: 0.000 min
Response: 7665820
Conc: 46.60 ug/ml

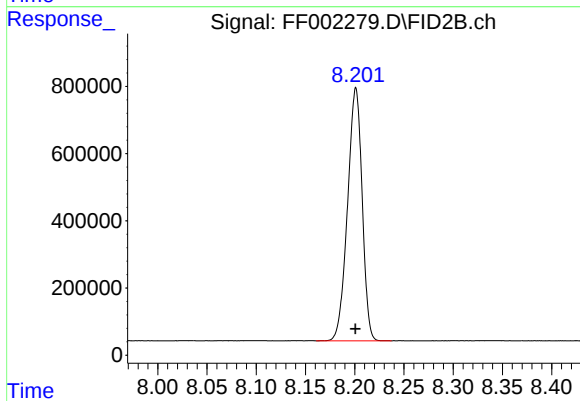

#4 N-TETRADECANE


R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 7765166
Conc: 46.62 ug/ml

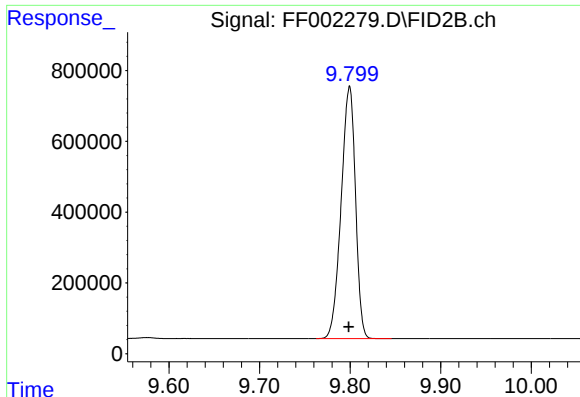

#5 N-HEXADECANE


R.T.: 9.799 min
Delta R.T.: 0.000 min
Response: 7838757
Conc: 46.81 ug/ml

Instrument :
FID_F
ClientSampleId :
FF100118ICV

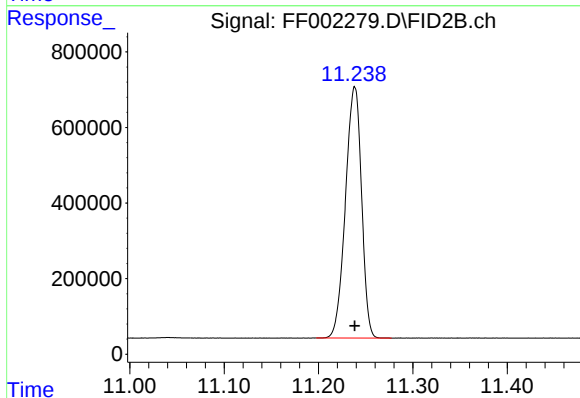


#6 N-OCTADECANE

R.T.: 11.238 min
Delta R.T.: 0.000 min
Response: 7868410
Conc: 46.86 ug/ml

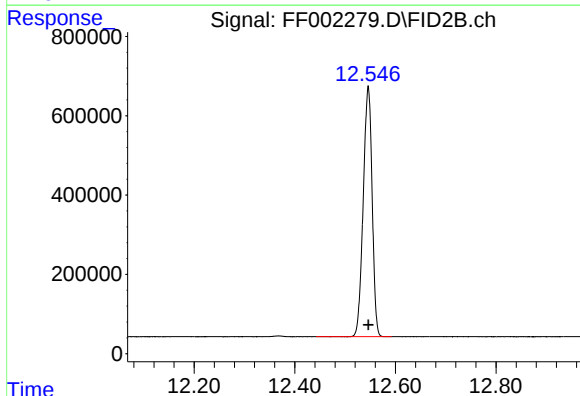


#7 N-EICOSANE

R.T.: 12.546 min
Delta R.T.: 0.000 min
Response: 7767441
Conc: 46.90 ug/ml

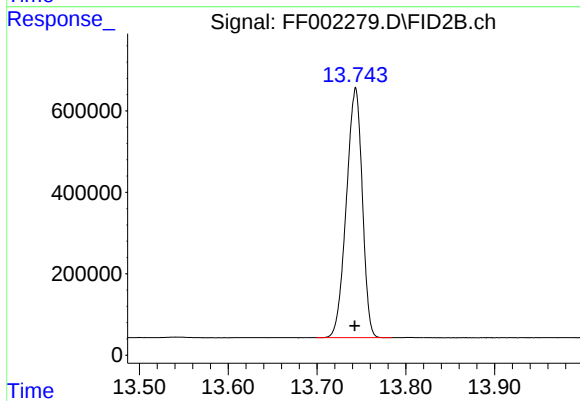

#8 N-DOCOSANE


R.T.: 13.743 min
Delta R.T.: 0.000 min
Response: 7646685
Conc: 46.86 ug/ml

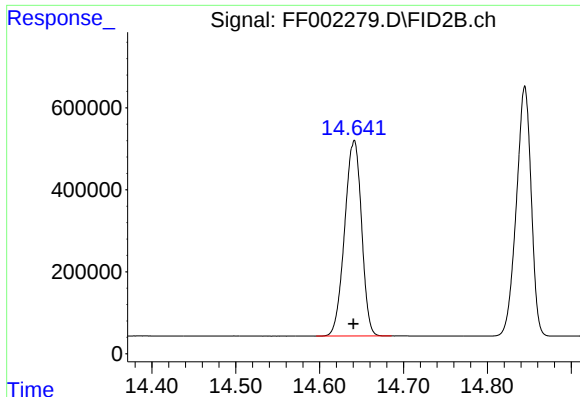

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.641 min
Delta R.T.: 0.000 min
Response: 6677949
Conc: 46.82 ug/ml

Instrument :
FID_F
ClientSampleId :
FF100118ICV

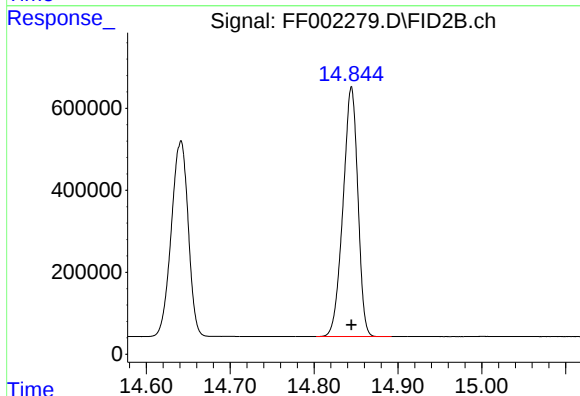


#10 N-TETRACOSANE

R.T.: 14.845 min
Delta R.T.: 0.000 min
Response: 7480546
Conc: 46.78 ug/ml

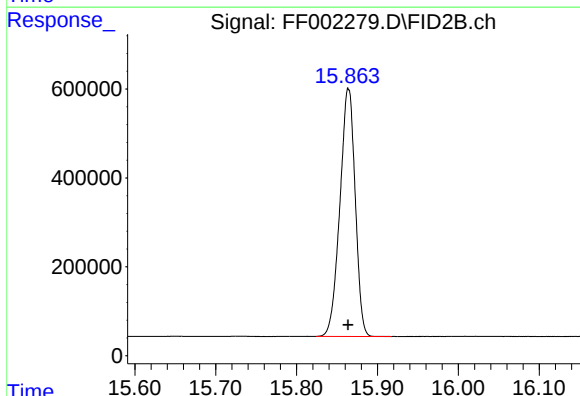


#11 N-HEXACOSANE

R.T.: 15.864 min
Delta R.T.: 0.000 min
Response: 7332892
Conc: 46.82 ug/ml

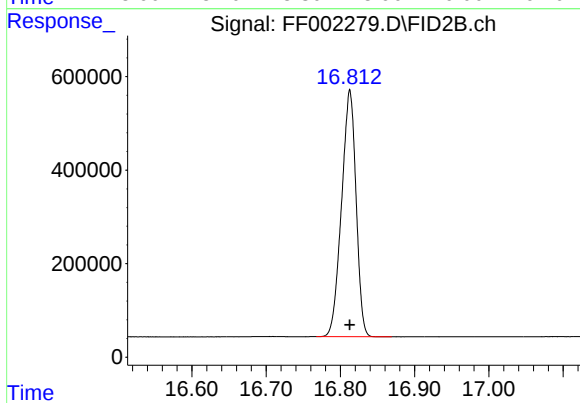

#12 N-OCTACOSANE


R.T.: 16.813 min
Delta R.T.: 0.000 min
Response: 7154886
Conc: 46.77 ug/ml

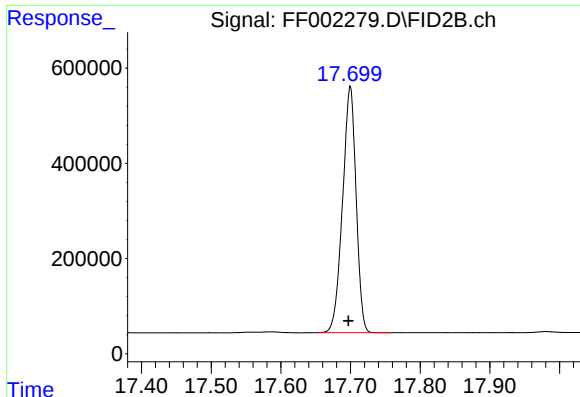

#13 N-TRIACONTANE


R.T.: 17.700 min
Delta R.T.: 0.003 min
Response: 6986853
Conc: 46.71 ug/ml

Instrument :
FID_F
ClientSampleId :
FF100118ICV

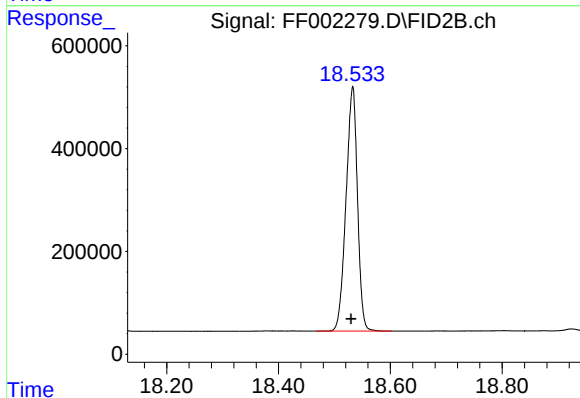


#14 N-DOTRIACONTANE

R.T.: 18.533 min
Delta R.T.: 0.003 min
Response: 6758988
Conc: 46.90 ug/ml

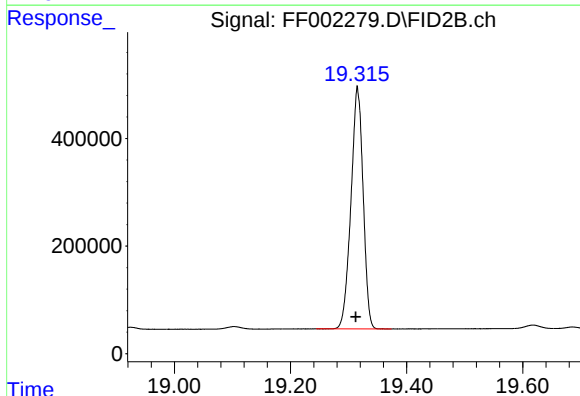


#15 N-TETRATRIACONTANE

R.T.: 19.315 min
Delta R.T.: 0.003 min
Response: 6540901
Conc: 47.10 ug/ml

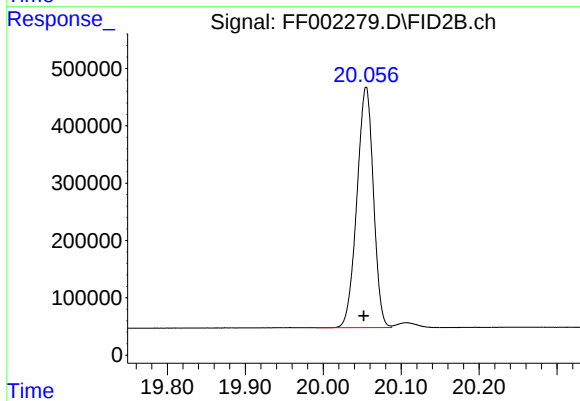

#16 N-HEXATRIACONTANE


R.T.: 20.055 min
Delta R.T.: 0.003 min
Response: 6176950
Conc: 47.94 ug/ml

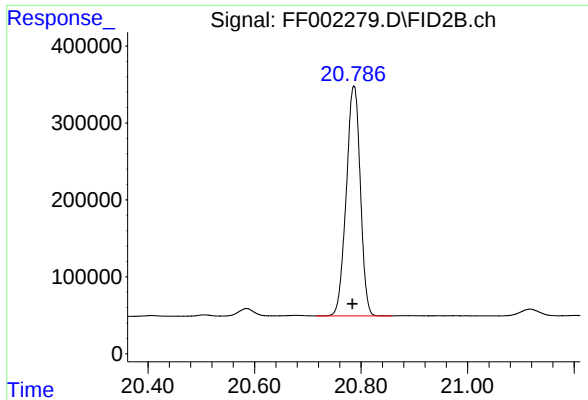

#17 N-OCTATRIACONTANE

R.T.: 20.787 min
Delta R.T.: 0.003 min
Response: 5479275
Conc: 47.97 ug/ml

Instrument :
FID_F
ClientSampleId :
FF100118ICV

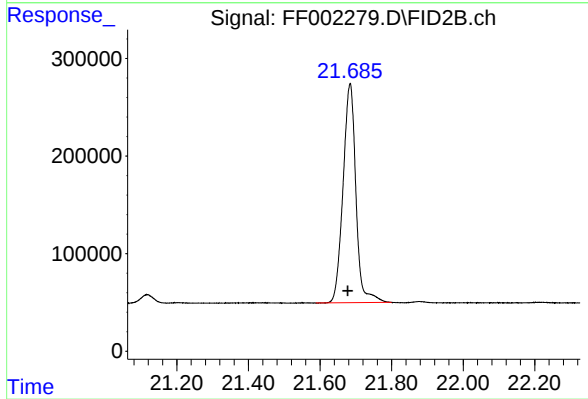

#18 N-TETRACONTANE

R.T.: 21.684 min
Delta R.T.: 0.007 min
Response: 5605479
Conc: 49.60 ug/ml