

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
 Data File : FF002283.D
 Signal(s) : FID2B.ch
 Acq On : 01 Oct 2018 14:15
 Operator : AJ\SJ
 Sample : PB113351BS
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB113351BS

Integration File: Sample.e
 Quant Time: Oct 02 03:45:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.637	2769446	19.418 ug/ml
Target Compounds			
2) N-DECANE	4.384	3083057	19.033 ug/ml
3) N-DODECANE	6.403	3142431	19.103 ug/ml
4) N-TETRADECANE	8.194	3191741	19.161 ug/ml
5) N-HEXADECANE	9.794	3219358	19.223 ug/ml
6) N-OCTADECANE	11.234	3241016	19.302 ug/ml
7) N-EICOSANE	12.542	3200058	19.322 ug/ml
8) N-DOCOSANE	13.738	3155536	19.339 ug/ml
10) N-TETRACOSANE	14.841	3090223	19.326 ug/ml
11) N-HEXACOSANE	15.860	3036237	19.385 ug/ml
12) N-OCTACOSANE	16.808	2986819	19.526 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
Data File : FF002283.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2018 14:15
Operator : AJ\SJ
Sample : PB113351BS
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB113351BS

Integration File: Sample.e
Quant Time: Oct 02 03:45:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

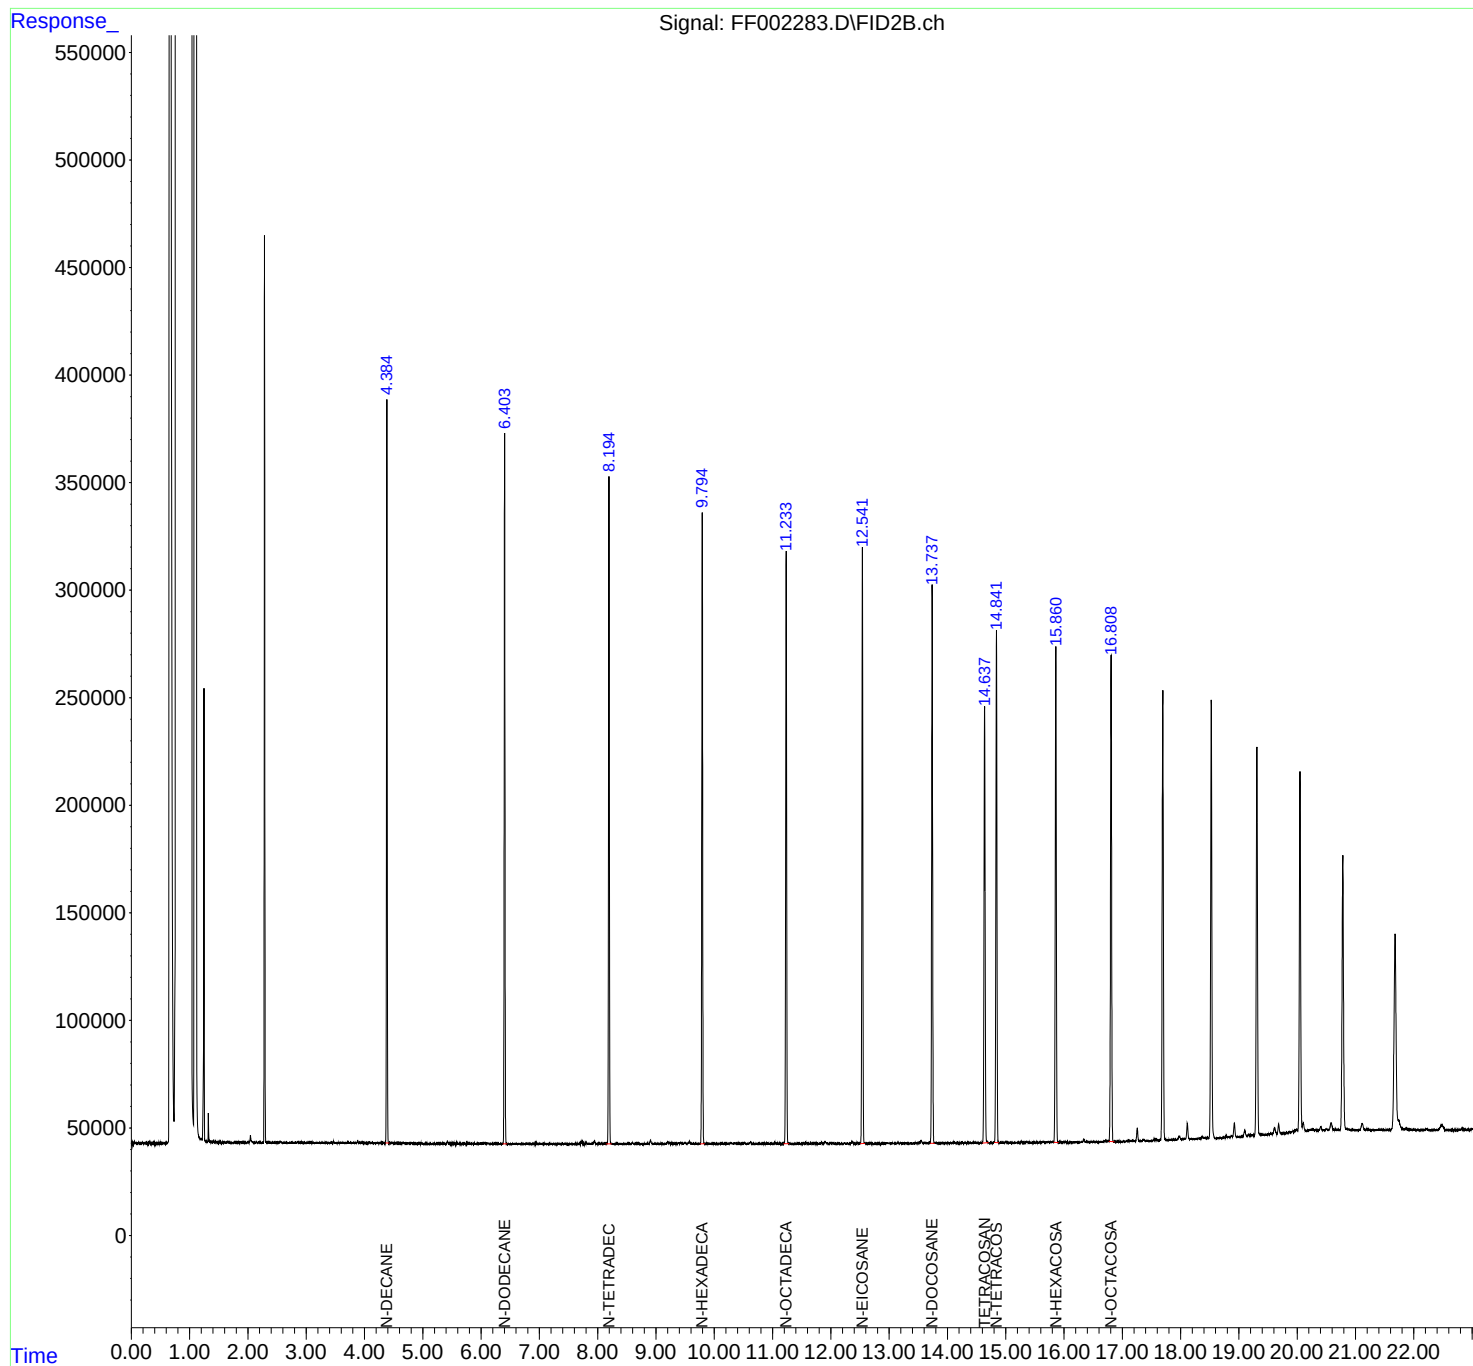


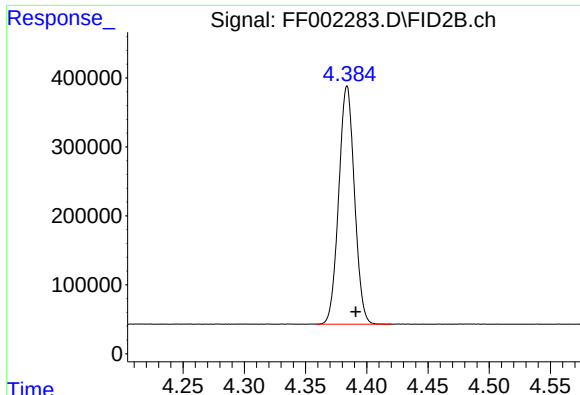

#2 N-DECANE


R.T.: 4.384 min
Delta R.T.: -0.007 min
Response: 3083057
Conc: 19.03 ug/ml

Instrument :
FID_F
ClientSampleId :
PB113351BS

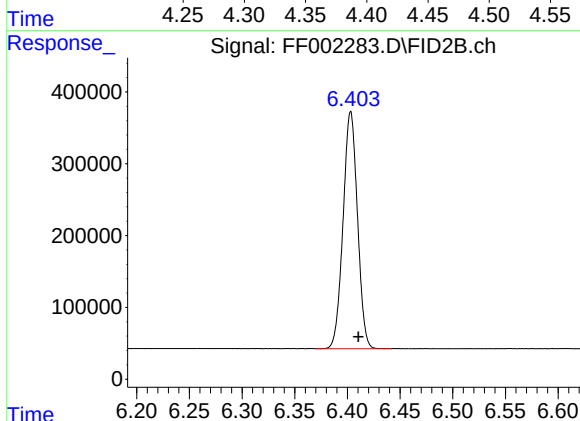


#3 N-DODECANE

R.T.: 6.403 min
Delta R.T.: -0.007 min
Response: 3142431
Conc: 19.10 ug/ml

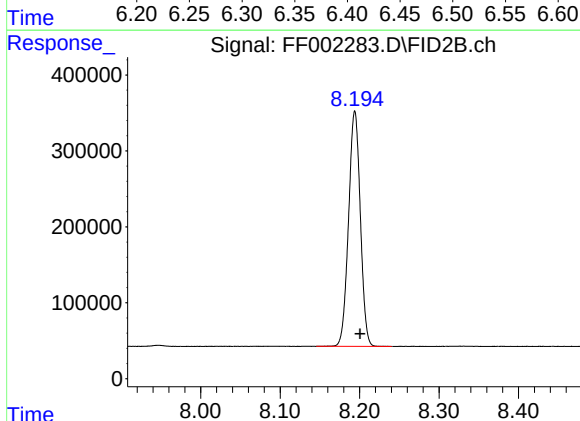


#4 N-TETRADECANE

R.T.: 8.194 min
Delta R.T.: -0.007 min
Response: 3191741
Conc: 19.16 ug/ml

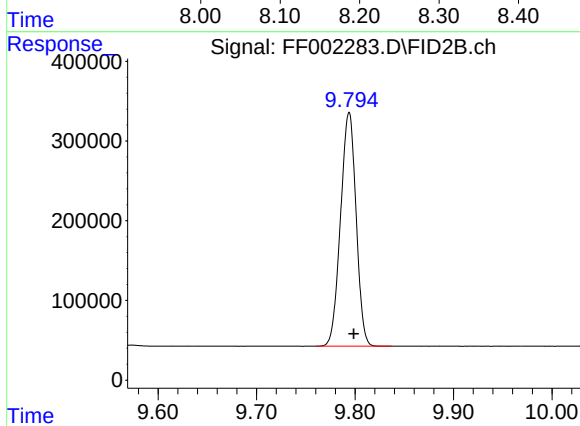

#5 N-HEXADECANE


R.T.: 9.794 min
Delta R.T.: -0.005 min
Response: 3219358
Conc: 19.22 ug/ml

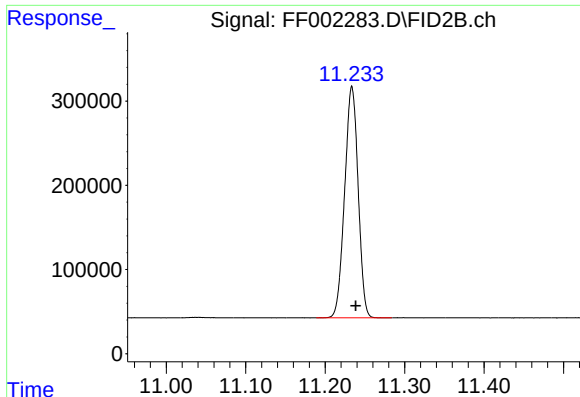

#6 N-OCTADECANE


R.T.: 11.234 min
Delta R.T.: -0.005 min
Response: 3241016
Conc: 19.30 ug/ml

Instrument :
FID_F
ClientSampleId :
PB113351BS

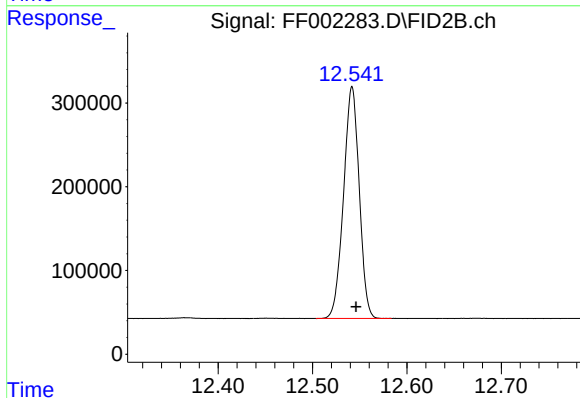


#7 N-EICOSANE

R.T.: 12.542 min
Delta R.T.: -0.004 min
Response: 3200058
Conc: 19.32 ug/ml

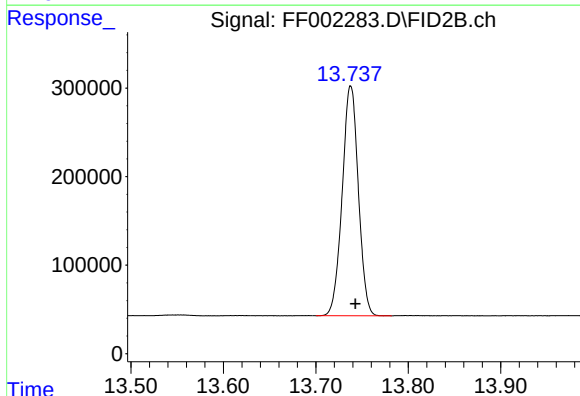


#8 N-DOCOSANE

R.T.: 13.738 min
Delta R.T.: -0.005 min
Response: 3155536
Conc: 19.34 ug/ml

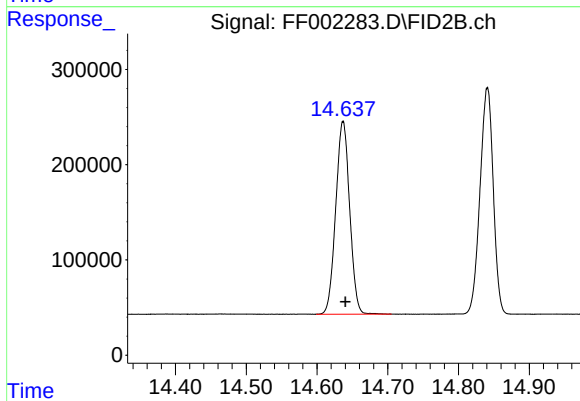

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.637 min
Delta R.T.: -0.004 min
Response: 2769446
Conc: 19.42 ug/ml

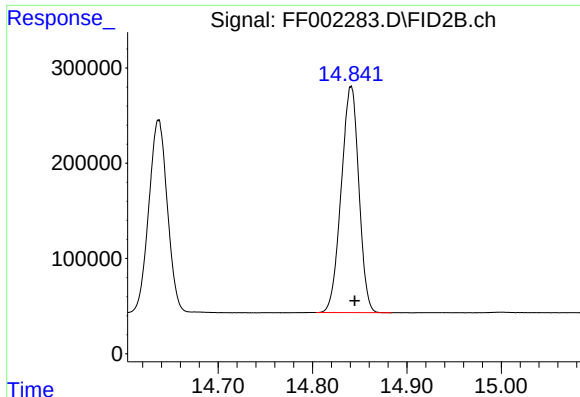

#10 N-TETRACOSANE


R.T.: 14.841 min
Delta R.T.: -0.004 min
Response: 3090223
Conc: 19.33 ug/ml

Instrument :
FID_F
ClientSampleId :
PB113351BS

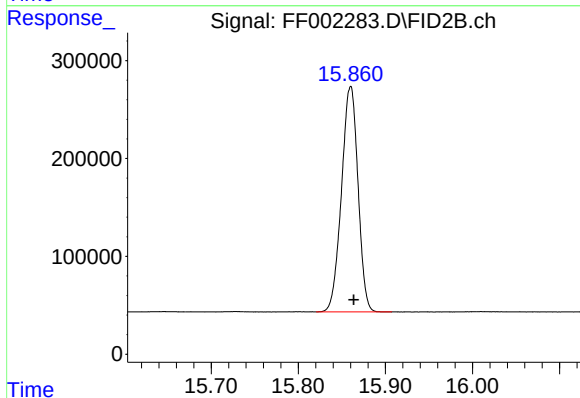

#11 N-HEXACOSANE

R.T.: 15.860 min
Delta R.T.: -0.004 min
Response: 3036237
Conc: 19.39 ug/ml

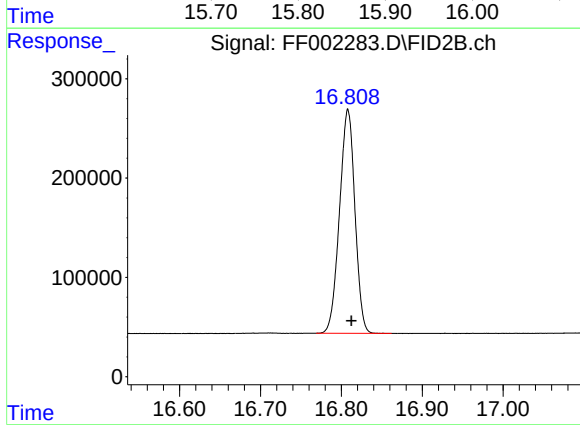

#12 N-OCTACOSANE

R.T.: 16.808 min
Delta R.T.: -0.004 min
Response: 2986819
Conc: 19.53 ug/ml