

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
 Data File : FF002296.D
 Signal(s) : FID2B.ch
 Acq On : 01 Oct 2018 20:50
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: Sample.e
 Quant Time: Oct 02 03:48:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.641	6523590	45.740 ug/ml
Target Compounds			
2) N-DECANE	4.388	7782404	48.043 ug/ml
3) N-DODECANE	6.407	7875904	47.877 ug/ml
4) N-TETRADECANE	8.198	7926370	47.584 ug/ml
5) N-HEXADECANE	9.797	7941803	47.421 ug/ml
6) N-OCTADECANE	11.238	7908157	47.098 ug/ml
7) N-EICOSANE	12.546	7723195	46.633 ug/ml
8) N-DOCOSANE	13.743	7510717	46.029 ug/ml
10) N-TETRACOSANE	14.845	7253652	45.364 ug/ml
11) N-HEXACOSANE	15.866	7012343	44.771 ug/ml
12) N-OCTACOSANE	16.814	6774656	44.288 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
Data File : FF002296.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2018 20:50
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: Sample.e
Quant Time: Oct 02 03:48:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

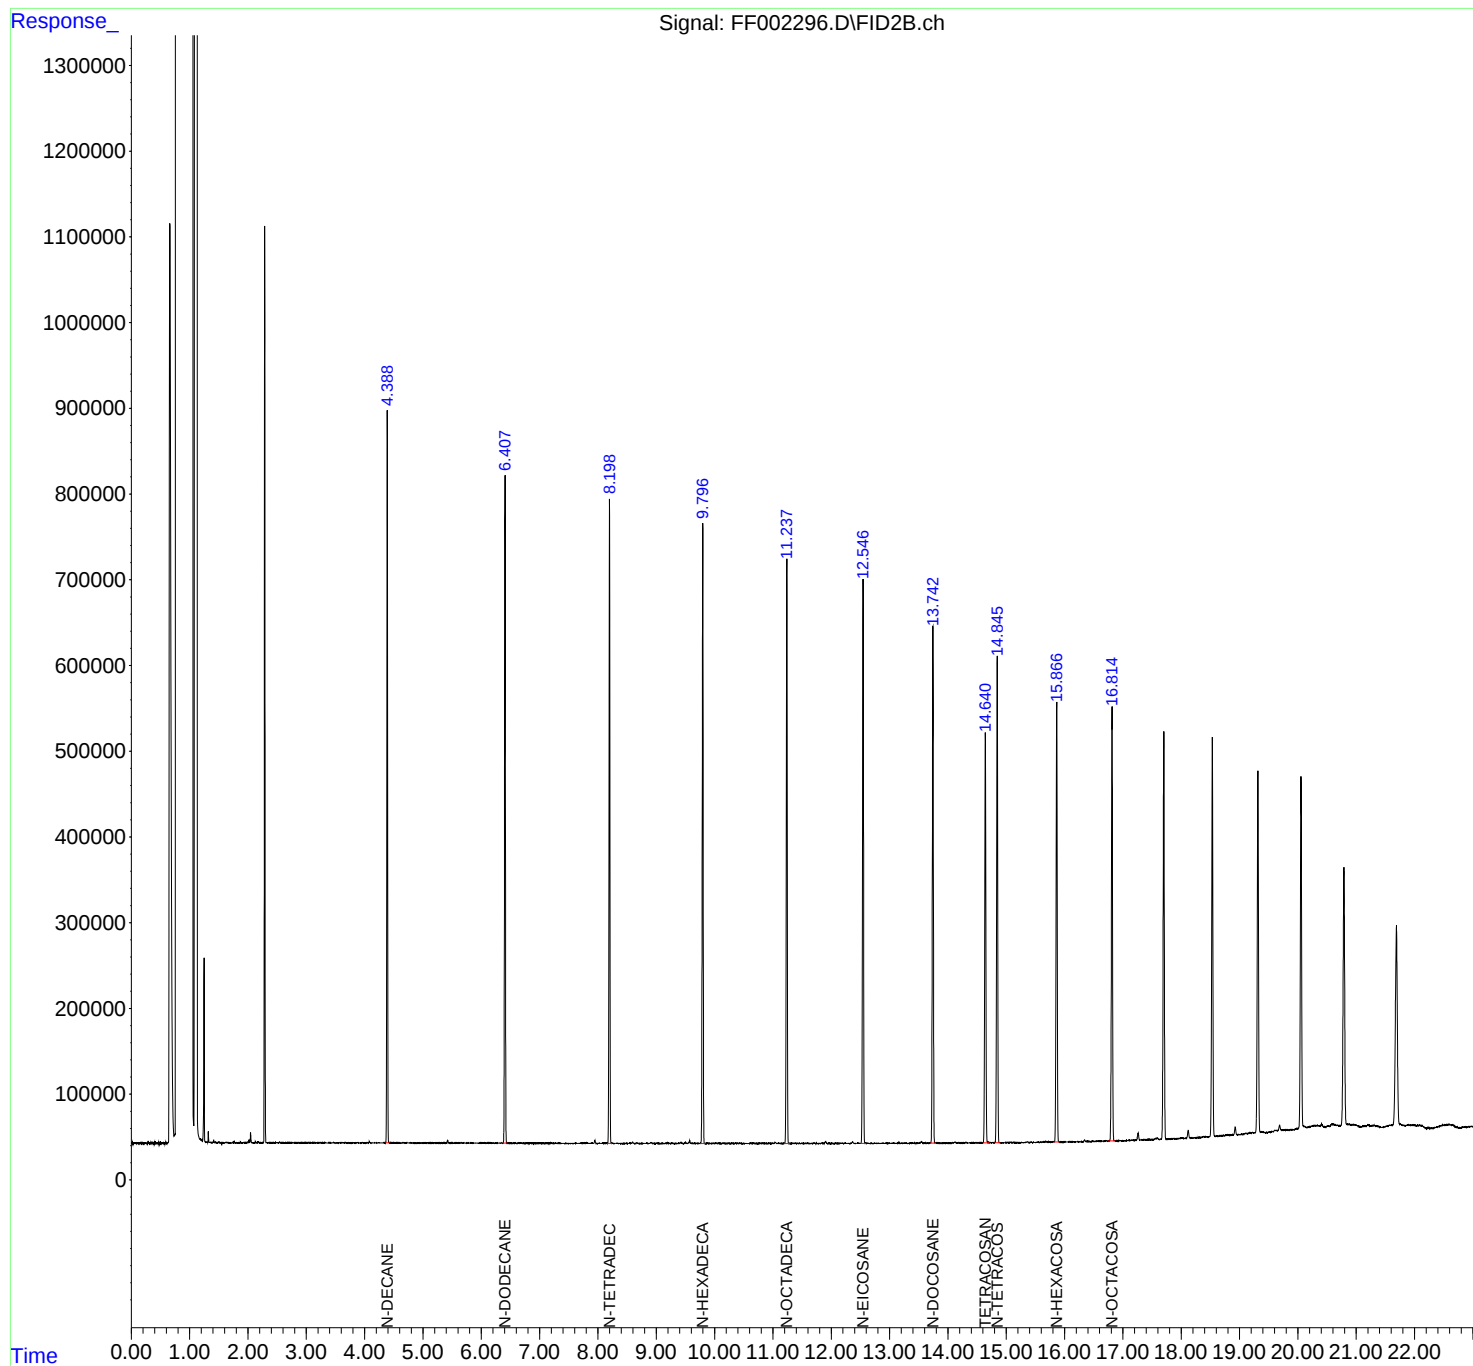


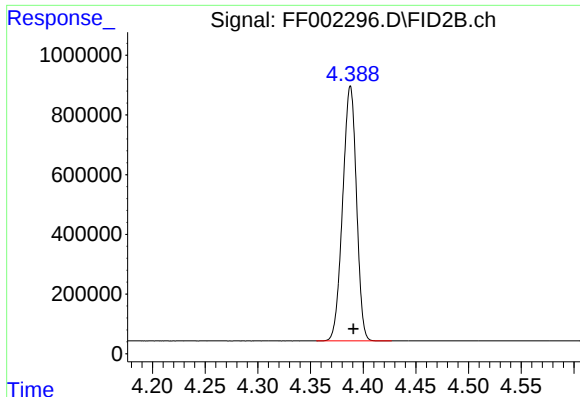

#2 N-DECANE


R.T.: 4.388 min
Delta R.T.: -0.003 min
Response: 7782404
Conc: 48.04 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

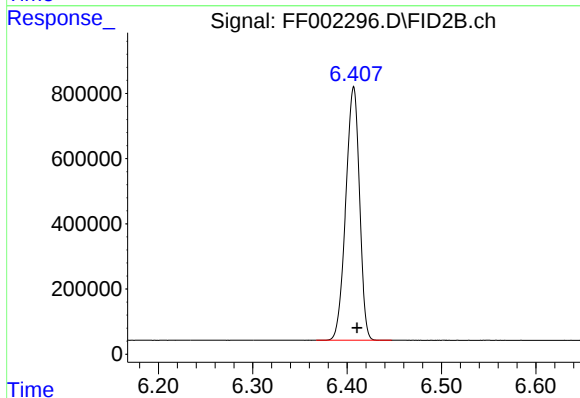


#3 N-DODECANE

R.T.: 6.407 min
Delta R.T.: -0.004 min
Response: 7875904
Conc: 47.88 ug/ml

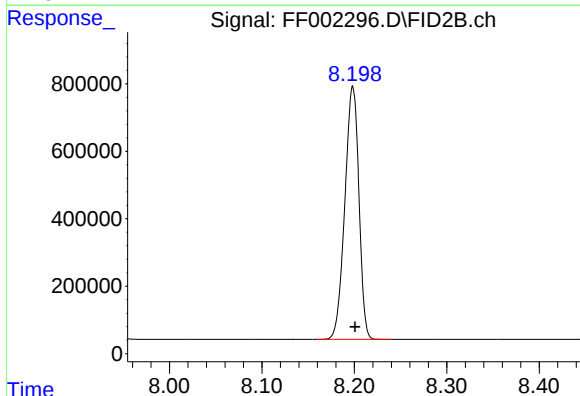


#4 N-TETRADECANE

R.T.: 8.198 min
Delta R.T.: -0.002 min
Response: 7926370
Conc: 47.58 ug/ml

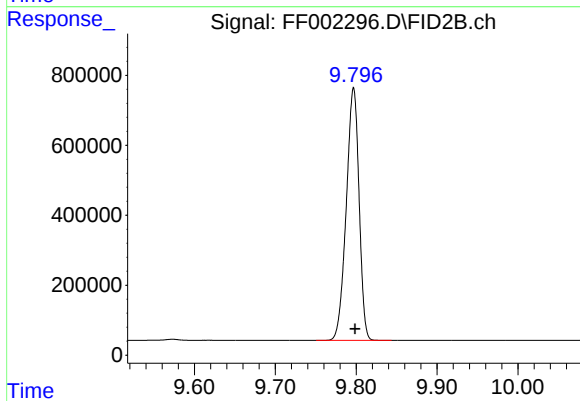

#5 N-HEXADECANE


R.T.: 9.797 min
Delta R.T.: -0.002 min
Response: 7941803
Conc: 47.42 ug/ml

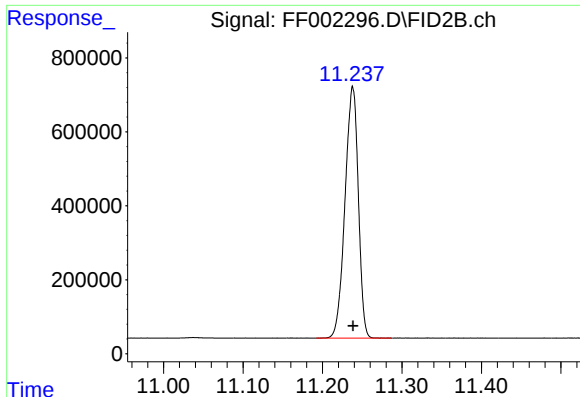

#6 N-OCTADECANE


R.T.: 11.238 min
Delta R.T.: 0.000 min
Response: 7908157
Conc: 47.10 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

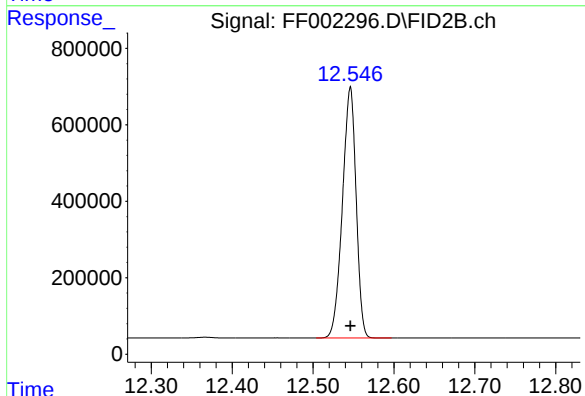


#7 N-EICOSANE

R.T.: 12.546 min
Delta R.T.: 0.000 min
Response: 7723195
Conc: 46.63 ug/ml

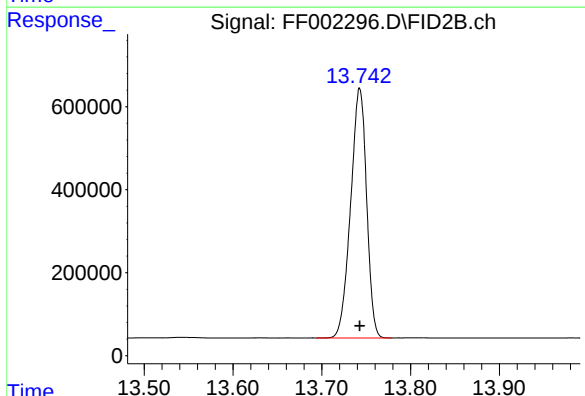


#8 N-DOCOSANE

R.T.: 13.743 min
Delta R.T.: 0.000 min
Response: 7510717
Conc: 46.03 ug/ml

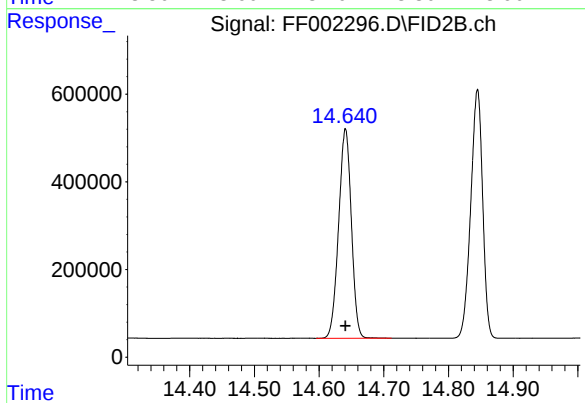

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.641 min
Delta R.T.: 0.000 min
Response: 6523590
Conc: 45.74 ug/ml

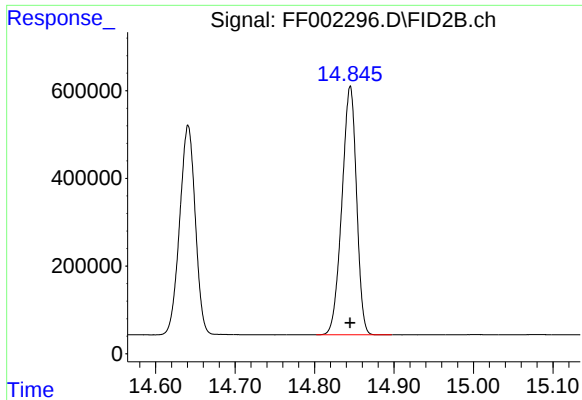

#10 N-TETRACOSANE


R.T.: 14.845 min
Delta R.T.: 0.000 min
Response: 7253652
Conc: 45.36 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

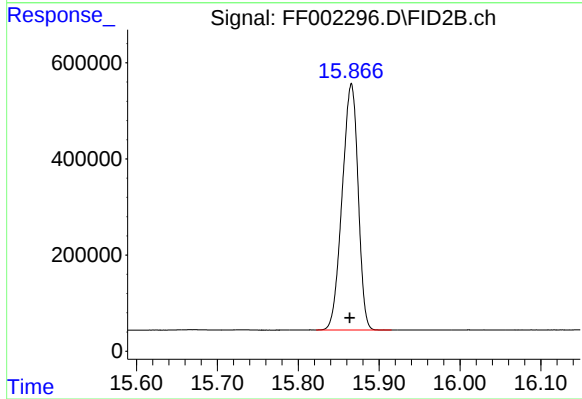

#11 N-HEXACOSANE

R.T.: 15.866 min
Delta R.T.: 0.002 min
Response: 7012343
Conc: 44.77 ug/ml

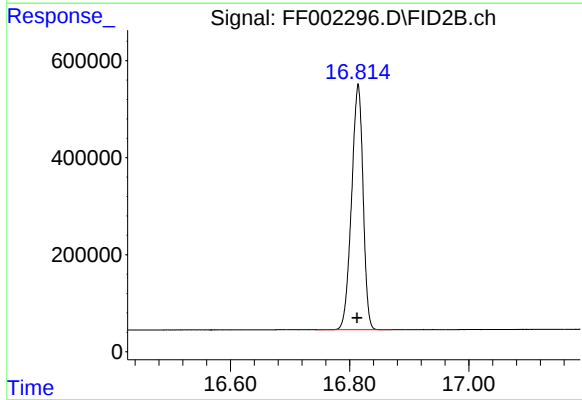

#12 N-OCTACOSANE

R.T.: 16.814 min
Delta R.T.: 0.002 min
Response: 6774656
Conc: 44.29 ug/ml