

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
 Data File : FF002298.D
 Signal(s) : FID2B.ch
 Acq On : 01 Oct 2018 21:50
 Operator : AJ\SJ
 Sample : WATER IDOC-02
 Misc : FOR DD AND RM
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 WATER IDOC-02

Integration File: Sample.e
 Quant Time: Oct 02 03:49:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.637	2786833	19.540 ug/ml
Target Compounds			
2) N-DECANE	4.386	3334150	20.583 ug/ml
3) N-DODECANE	6.404	3370143	20.487 ug/ml
4) N-TETRADECANE	8.195	3384474	20.318 ug/ml
5) N-HEXADECANE	9.793	3381751	20.193 ug/ml
6) N-OCTADECANE	11.233	3370368	20.073 ug/ml
7) N-EICOSANE	12.541	3297677	19.912 ug/ml
8) N-DOCOSANE	13.739	3214688	19.701 ug/ml
10) N-TETRACOSANE	14.840	3110843	19.455 ug/ml
11) N-HEXACOSANE	15.860	3011298	19.226 ug/ml
12) N-OCTACOSANE	16.808	2915146	19.057 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
Data File : FF002298.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2018 21:50
Operator : AJ\SJ
Sample : WATER IDOC-02
Misc : FOR DD AND RM
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WATER IDOC-02

Integration File: Sample.e
Quant Time: Oct 02 03:49:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

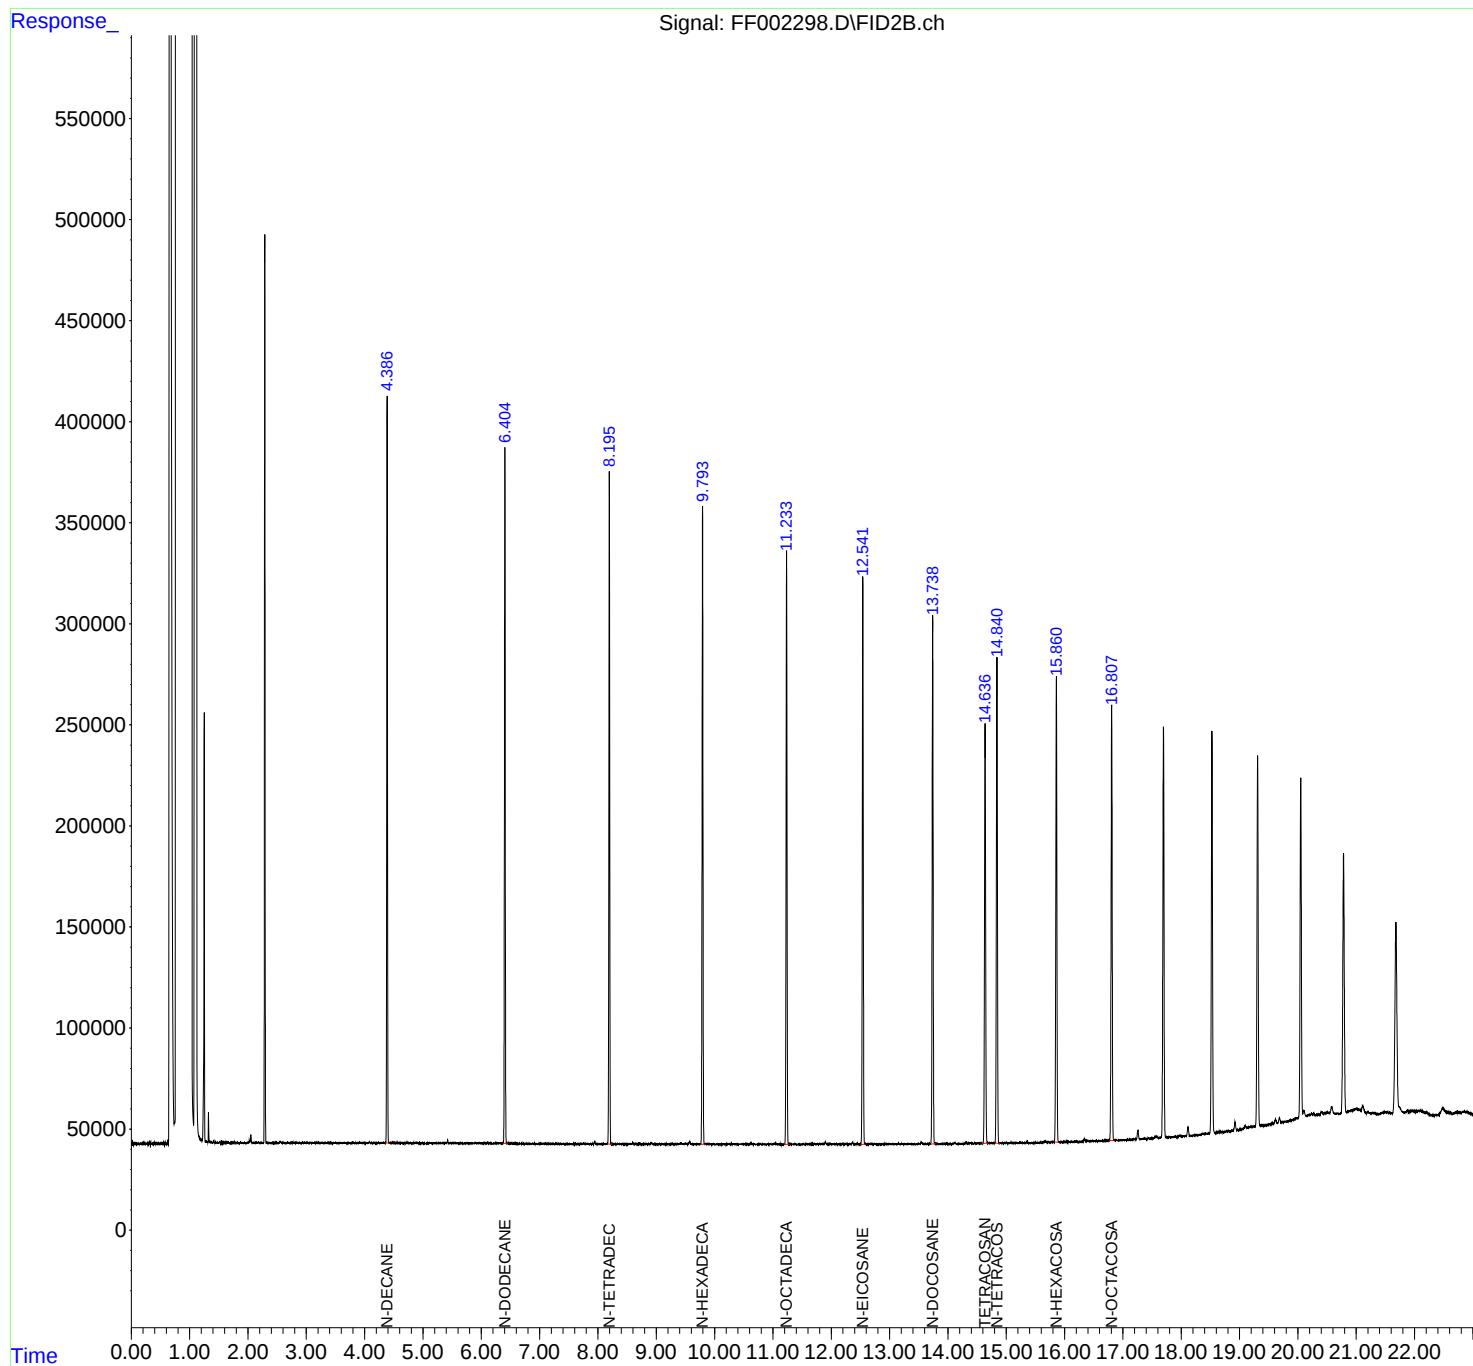


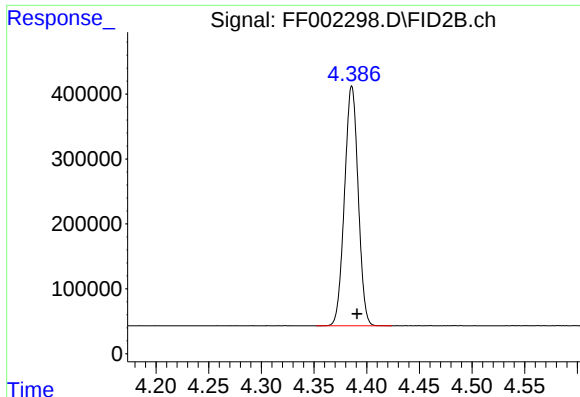

#2 N-DECANE


R.T.: 4.386 min
Delta R.T.: -0.005 min
Response: 3334150
Conc: 20.58 ug/ml

Instrument :
FID_F
ClientSampleId :
WATER IDOC-02

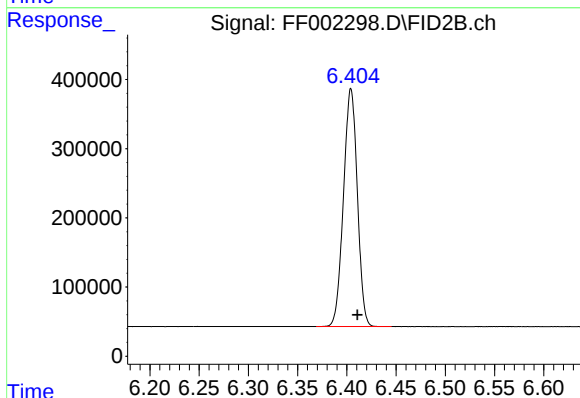


#3 N-DODECANE

R.T.: 6.404 min
Delta R.T.: -0.006 min
Response: 3370143
Conc: 20.49 ug/ml

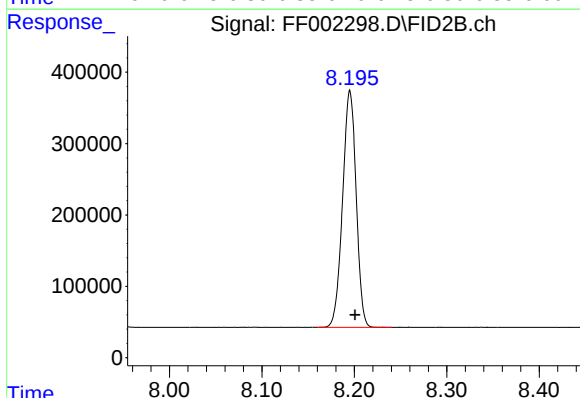


#4 N-TETRADECANE

R.T.: 8.195 min
Delta R.T.: -0.005 min
Response: 3384474
Conc: 20.32 ug/ml

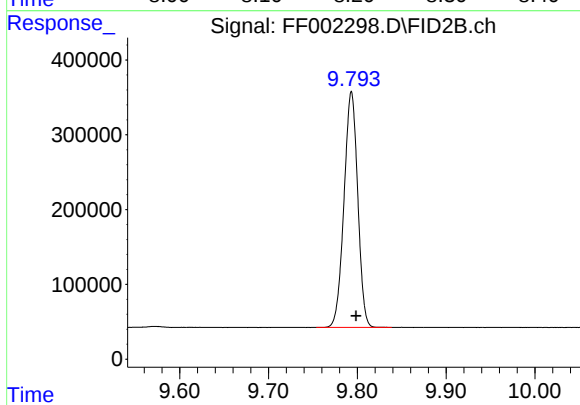

#5 N-HEXADECANE


R.T.: 9.793 min
Delta R.T.: -0.005 min
Response: 3381751
Conc: 20.19 ug/ml

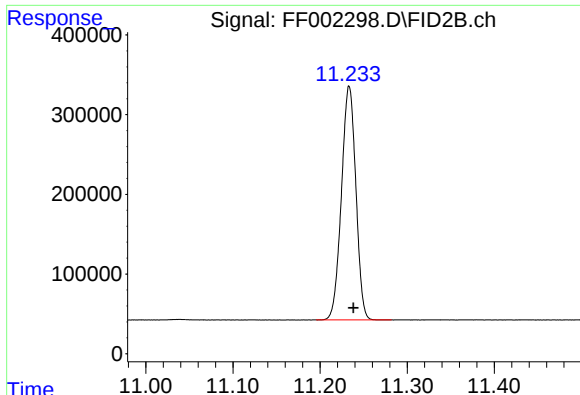

#6 N-OCTADECANE


R.T.: 11.233 min
Delta R.T.: -0.005 min
Response: 3370368
Conc: 20.07 ug/ml

Instrument :
FID_F
ClientSampleId :
WATER IDOC-02

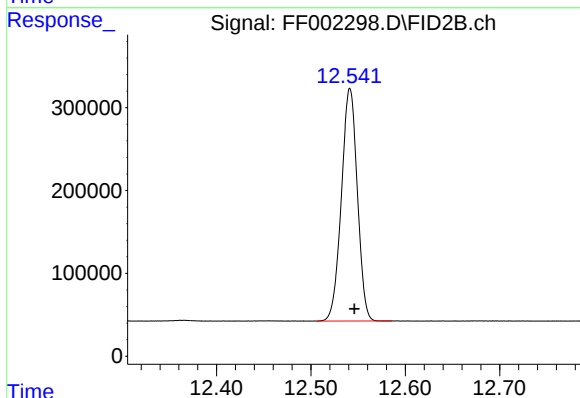


#7 N-EICOSANE

R.T.: 12.541 min
Delta R.T.: -0.005 min
Response: 3297677
Conc: 19.91 ug/ml

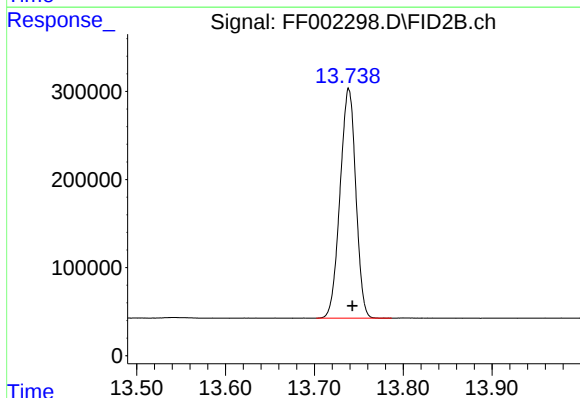


#8 N-DOCOSANE

R.T.: 13.739 min
Delta R.T.: -0.004 min
Response: 3214688
Conc: 19.70 ug/ml

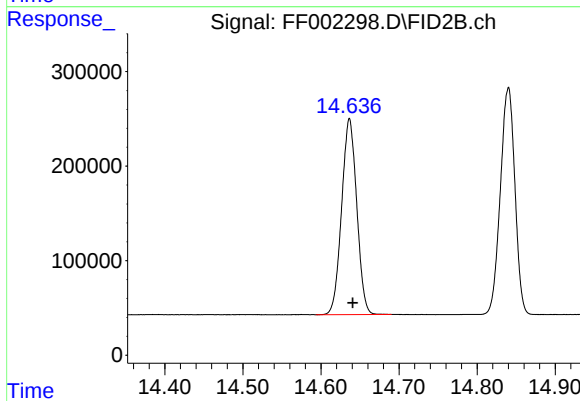

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.637 min
Delta R.T.: -0.004 min
Response: 2786833
Conc: 19.54 ug/ml

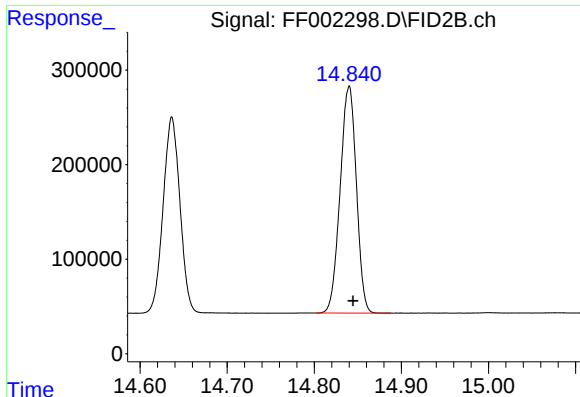

#10 N-TETRACOSANE


R.T.: 14.840 min
Delta R.T.: -0.005 min
Response: 3110843
Conc: 19.45 ug/ml

Instrument :
FID_F
ClientSampleId :
WATER IDOC-02

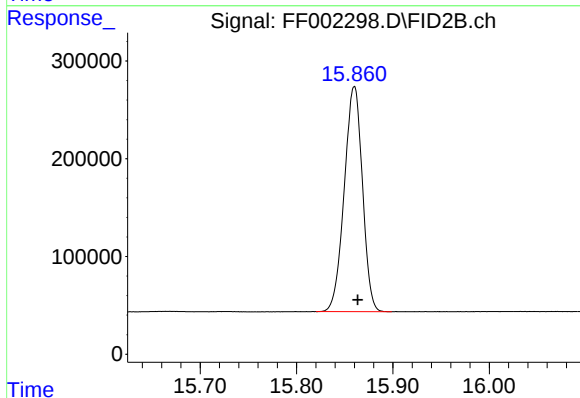

#11 N-HEXACOSANE

R.T.: 15.860 min
Delta R.T.: -0.004 min
Response: 3011298
Conc: 19.23 ug/ml

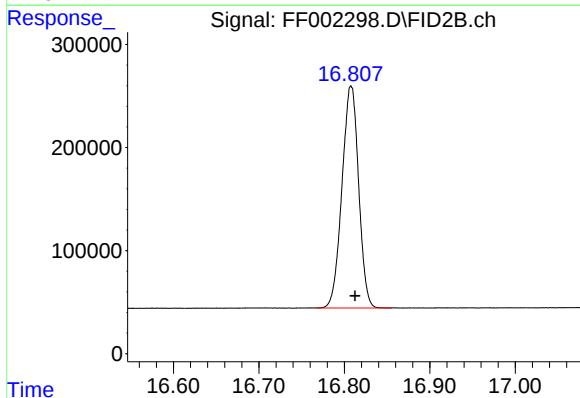

#12 N-OCTACOSANE

R.T.: 16.808 min
Delta R.T.: -0.005 min
Response: 2915146
Conc: 19.06 ug/ml