

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
 Data File : FF002300.D
 Signal(s) : FID2B.ch
 Acq On : 01 Oct 2018 22:50
 Operator : AJ\SJ
 Sample : WATER IDOC-04
 Misc : FOR DD AND RM
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 WATER IDOC-04

Integration File: Sample.e
 Quant Time: Oct 02 03:49:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:14:42 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.638	2797671	19.616 ug/ml
Target Compounds			
2) N-DECANE	4.386	3353179	20.700 ug/ml
3) N-DODECANE	6.404	3375697	20.521 ug/ml
4) N-TETRADECANE	8.195	3384632	20.319 ug/ml
5) N-HEXADECANE	9.794	3381247	20.190 ug/ml
6) N-OCTADECANE	11.234	3369305	20.066 ug/ml
7) N-EICOSANE	12.542	3292229	19.879 ug/ml
8) N-DOCOSANE	13.740	3205547	19.645 ug/ml
10) N-TETRACOSANE	14.841	3103415	19.408 ug/ml
11) N-HEXACOSANE	15.861	3033032	19.365 ug/ml
12) N-OCTACOSANE	16.810	3042191	19.888 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100118\
Data File : FF002300.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2018 22:50
Operator : AJ\SJ
Sample : WATER IDOC-04
Misc : FOR DD AND RM
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
WATER IDOC-04

Integration File: Sample.e
Quant Time: Oct 02 03:49:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100118.M
Quant Title :
QLast Update : Mon Oct 01 12:14:42 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

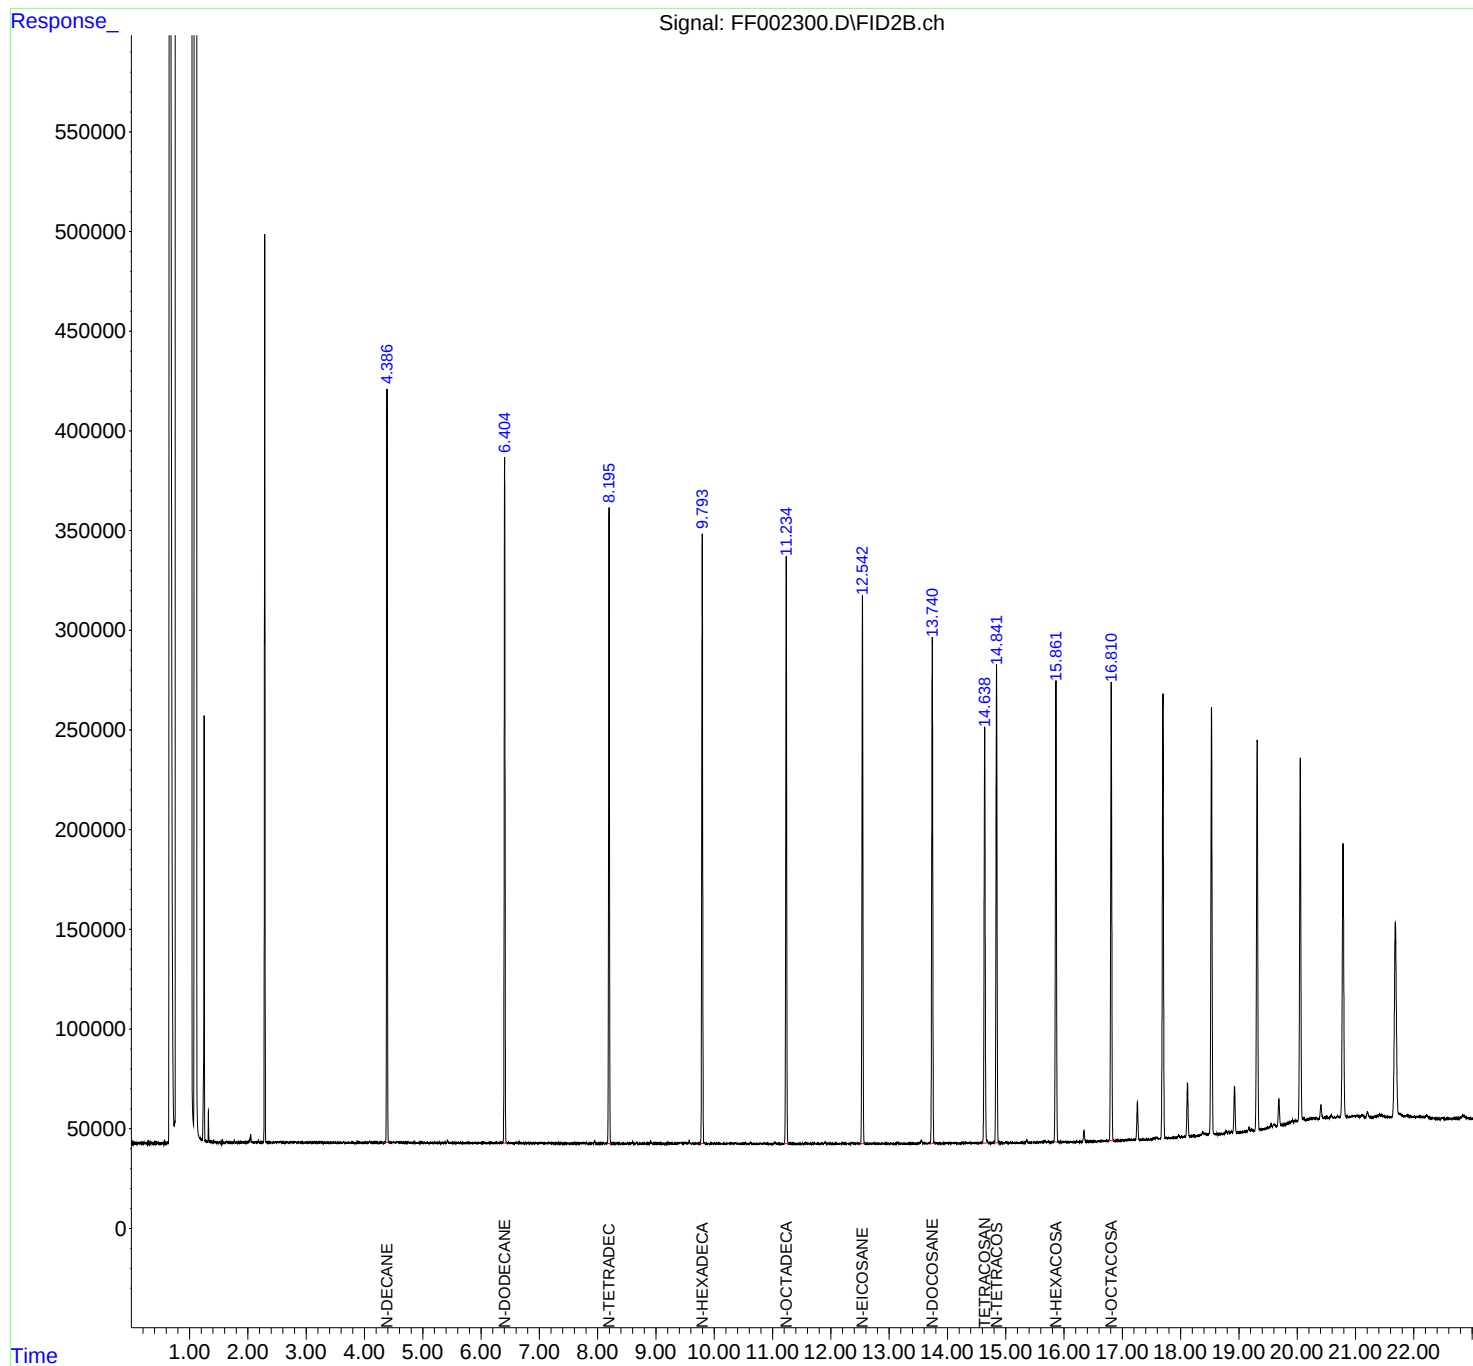


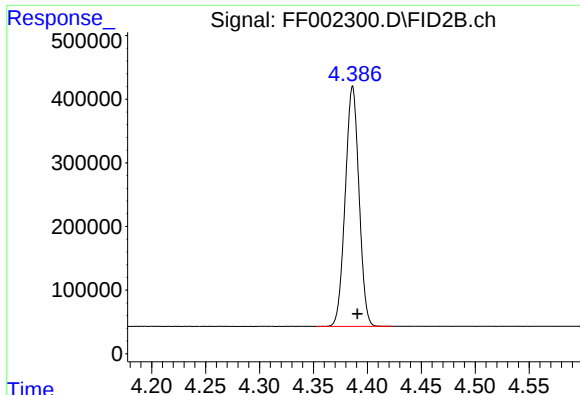

#2 N-DECANE


R.T.: 4.386 min
Delta R.T.: -0.005 min
Response: 3353179
Conc: 20.70 ug/ml

Instrument :
FID_F
ClientSampleId :
WATER IDOC-04

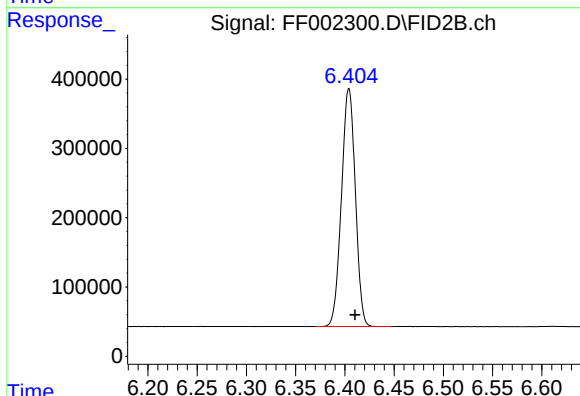


#3 N-DODECANE

R.T.: 6.404 min
Delta R.T.: -0.006 min
Response: 3375697
Conc: 20.52 ug/ml

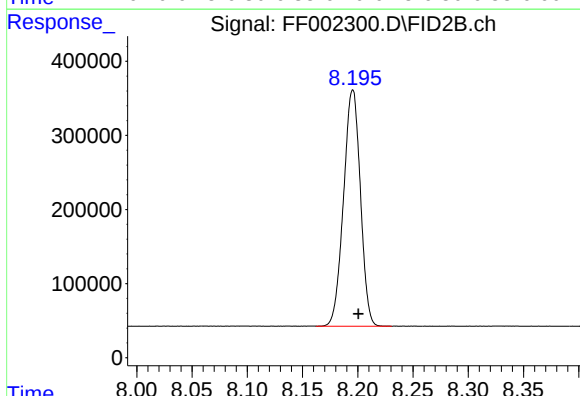


#4 N-TETRADECANE

R.T.: 8.195 min
Delta R.T.: -0.005 min
Response: 3384632
Conc: 20.32 ug/ml

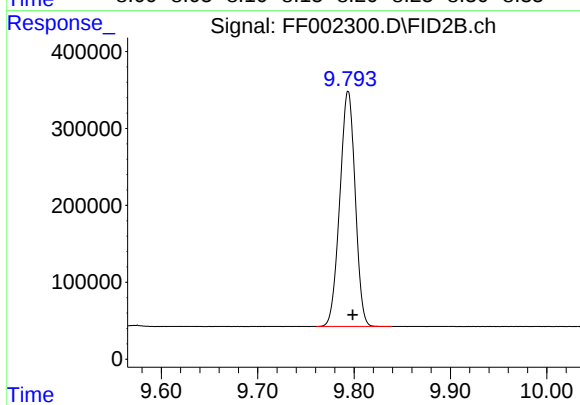

#5 N-HEXADECANE


R.T.: 9.794 min
Delta R.T.: -0.005 min
Response: 3381247
Conc: 20.19 ug/ml

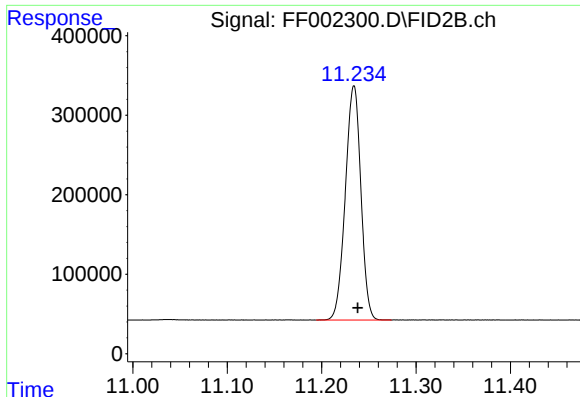

#6 N-OCTADECANE


R.T.: 11.234 min
Delta R.T.: -0.004 min
Response: 3369305
Conc: 20.07 ug/ml

Instrument :
FID_F
ClientSampleId :
WATER IDOC-04

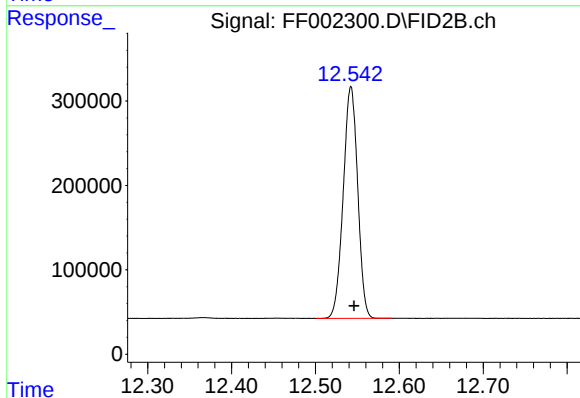


#7 N-EICOSANE

R.T.: 12.542 min
Delta R.T.: -0.004 min
Response: 3292229
Conc: 19.88 ug/ml

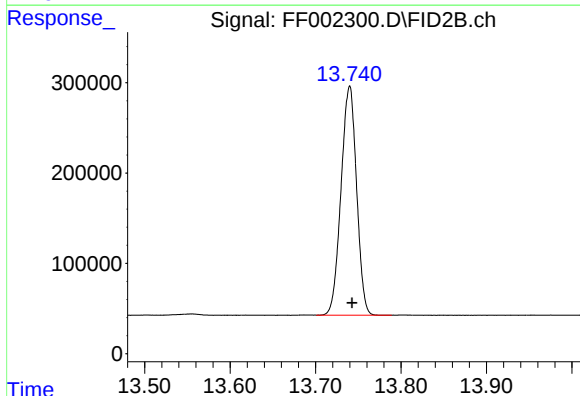


#8 N-DOCOSANE

R.T.: 13.740 min
Delta R.T.: -0.003 min
Response: 3205547
Conc: 19.65 ug/ml

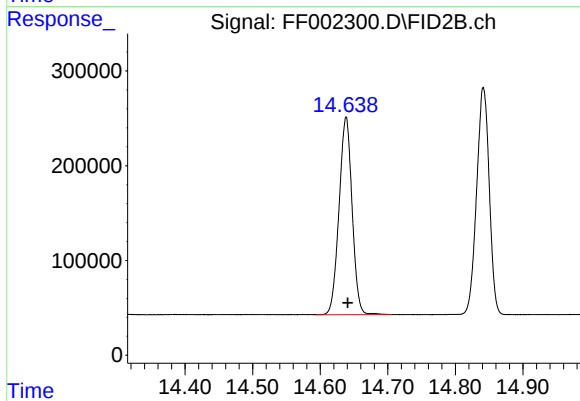

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.638 min
Delta R.T.: -0.002 min
Response: 2797671
Conc: 19.62 ug/ml

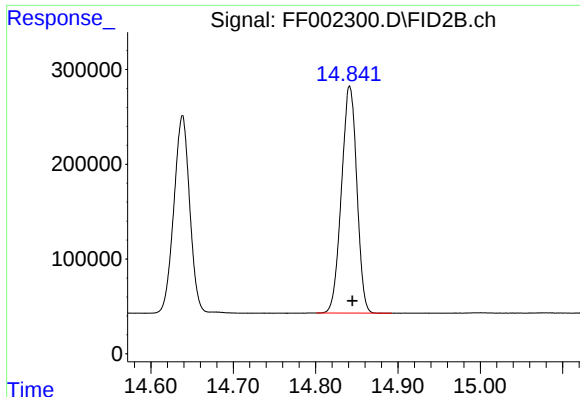

#10 N-TETRACOSANE


R.T.: 14.841 min
Delta R.T.: -0.003 min
Response: 3103415
Conc: 19.41 ug/ml

Instrument :
FID_F
ClientSampleId :
WATER IDOC-04

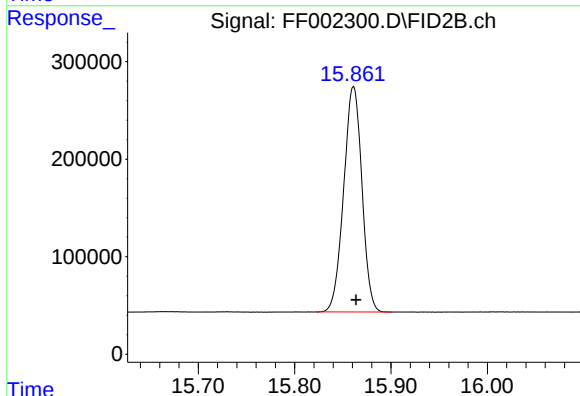

#11 N-HEXACOSANE

R.T.: 15.861 min
Delta R.T.: -0.003 min
Response: 3033032
Conc: 19.36 ug/ml

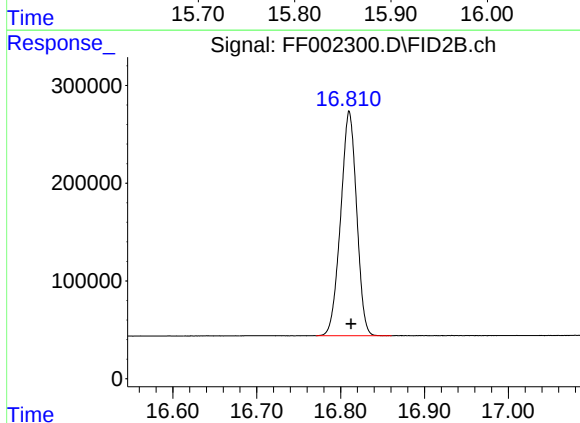

#12 N-OCTACOSANE

R.T.: 16.810 min
Delta R.T.: -0.002 min
Response: 3042191
Conc: 19.89 ug/ml