

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100121\
Data File : FF009054.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2021 11:21
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 01 22:29:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.492	4636426	32.834 ug/ml
12) N-OCTACOSANE	16.890	3952026	32.302 ug/ml
13) N-TRIACONTANE	17.773	346257	2.963 ug/ml
14) N-DOTRIACONTANE	18.603	464701	4.306 ug/ml
15) N-TETRATRIACONTANE	19.382	398396	4.067 ug/ml
16) N-HEXATRIACONTANE	20.121	269007	3.077 ug/ml
17) N-OCTATRIACONTANE	20.860	155726	1.955 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100121\
Data File : FF009054.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2021 11:21
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 01 22:29:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

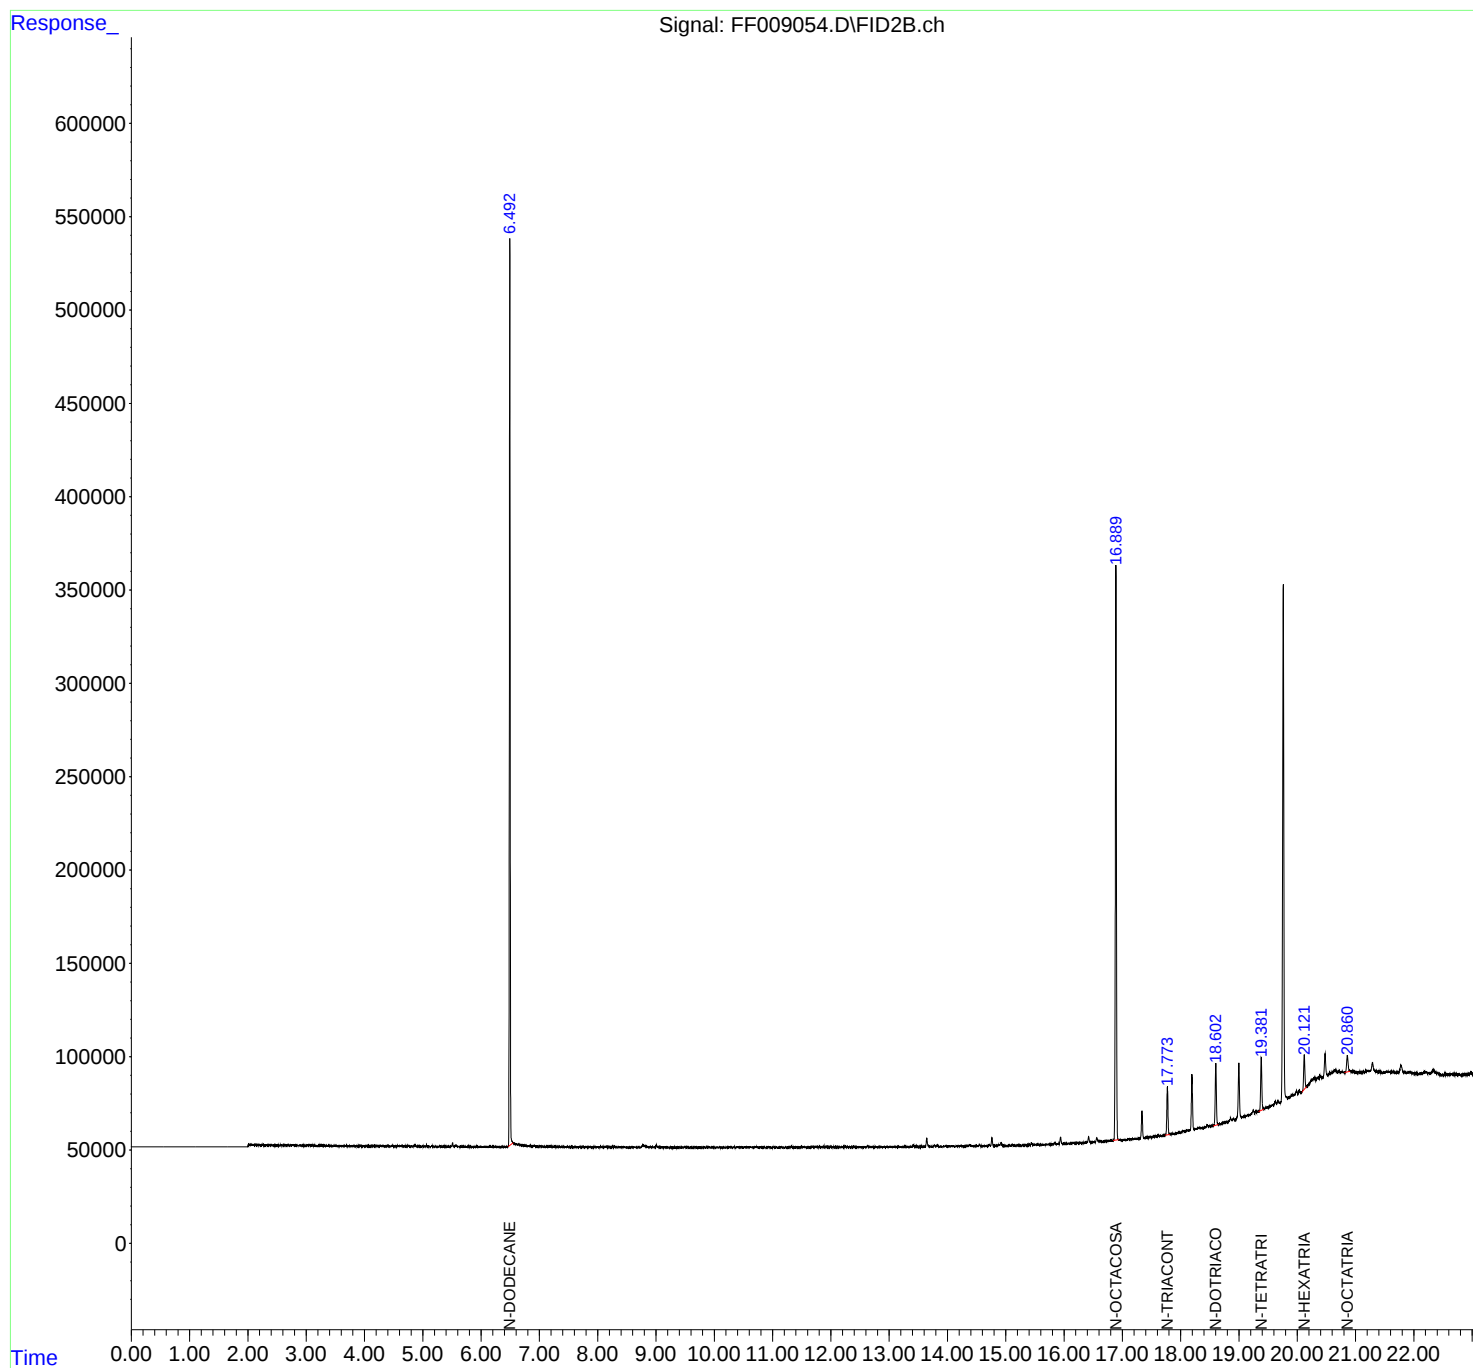


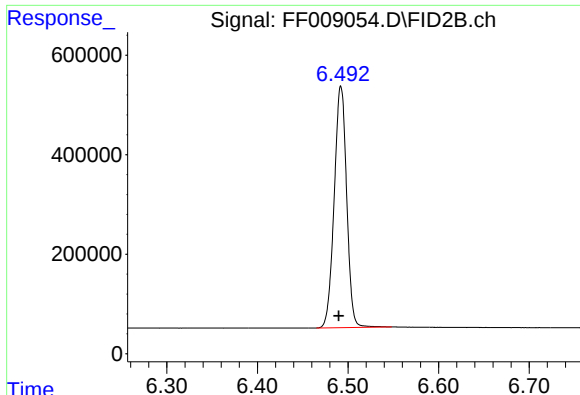

#3 N-DODECANE


R.T.: 6.492 min
Delta R.T.: 0.002 min
Response: 4636426
Conc: 32.83 ug/ml

Instrument :
FID_F
ClientSampleId :

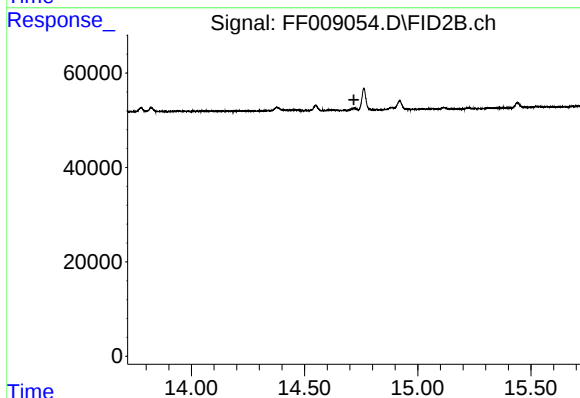


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.718 min
Response: 0
Conc: N.D.

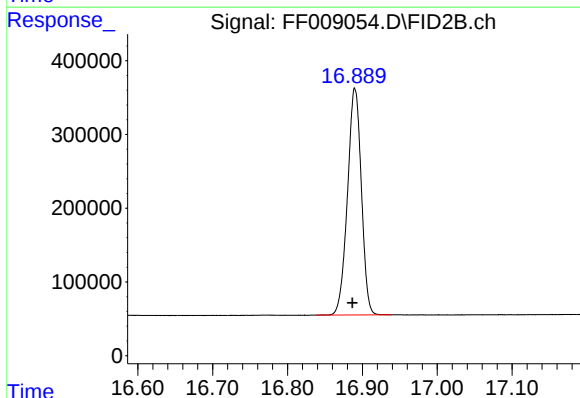


#12 N-OCTACOSANE

R.T.: 16.890 min
Delta R.T.: 0.003 min
Response: 3952026
Conc: 32.30 ug/ml

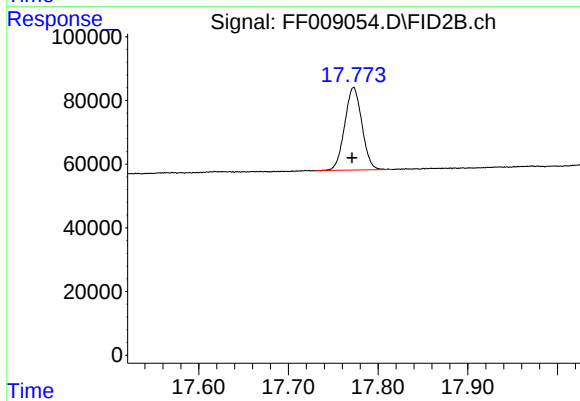

#13 N-TRIACONTANE


R.T.: 17.773 min
Delta R.T.: 0.002 min
Response: 346257
Conc: 2.96 ug/ml

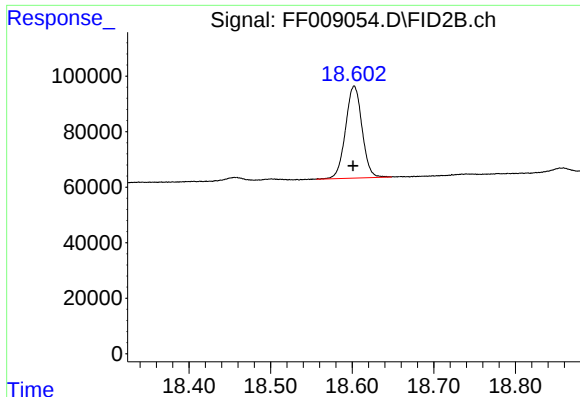

#14 N-DOTRIACONTANE


R.T.: 18.603 min
Delta R.T.: 0.001 min
Response: 464701
Conc: 4.31 ug/ml

Instrument :
FID_F
ClientSampleId :

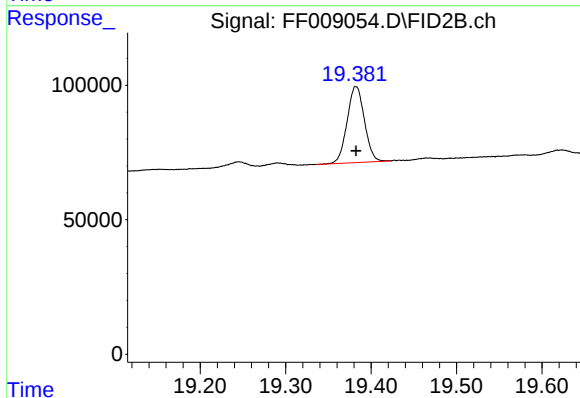


#15 N-TETRATRIACONTANE

R.T.: 19.382 min
Delta R.T.: 0.000 min
Response: 398396
Conc: 4.07 ug/ml

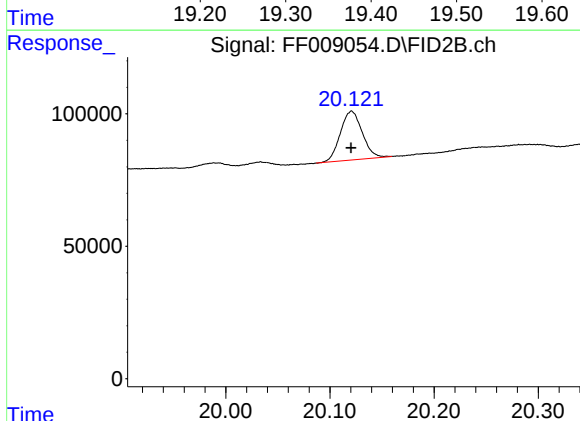

#16 N-HEXATRIACONTANE

R.T.: 20.121 min
Delta R.T.: 0.000 min
Response: 269007
Conc: 3.08 ug/ml

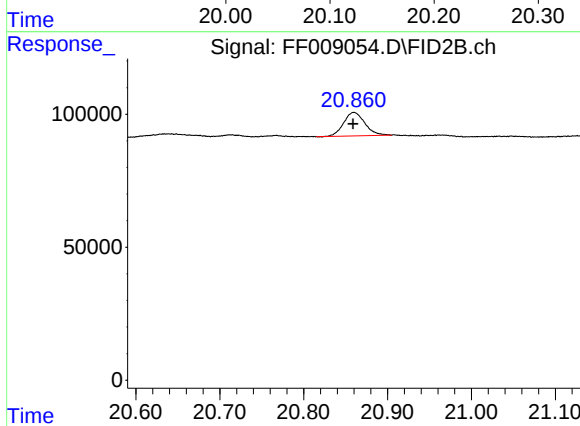

#17 N-OCTATRIACONTANE

R.T.: 20.860 min
Delta R.T.: 0.001 min
Response: 155726
Conc: 1.96 ug/ml