

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF100121\  
Data File : FF009056.D  
Signal(s) : FID2B.ch  
Acq On : 01 Oct 2021 12:22  
Operator : DD\AJ  
Sample : M3976-06 20X  
Misc :  
ALS Vial : 56 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Oct 01 22:29:57 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF090721.M  
Quant Title :  
QLast Update : Wed Sep 08 10:20:54 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T. | Response | Conc Units |
|-----------------------------|------|----------|------------|
| -----                       |      |          |            |
| System Monitoring Compounds |      |          |            |
| Target Compounds            |      |          |            |
| -----                       |      |          |            |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF100121\  
Data File : FF009056.D  
Signal(s) : FID2B.ch  
Acq On : 01 Oct 2021 12:22  
Operator : DD\AJ  
Sample : M3976-06 20X  
Misc :  
ALS Vial : 56 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Oct 01 22:29:57 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF090721.M  
Quant Title :  
QLast Update : Wed Sep 08 10:20:54 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

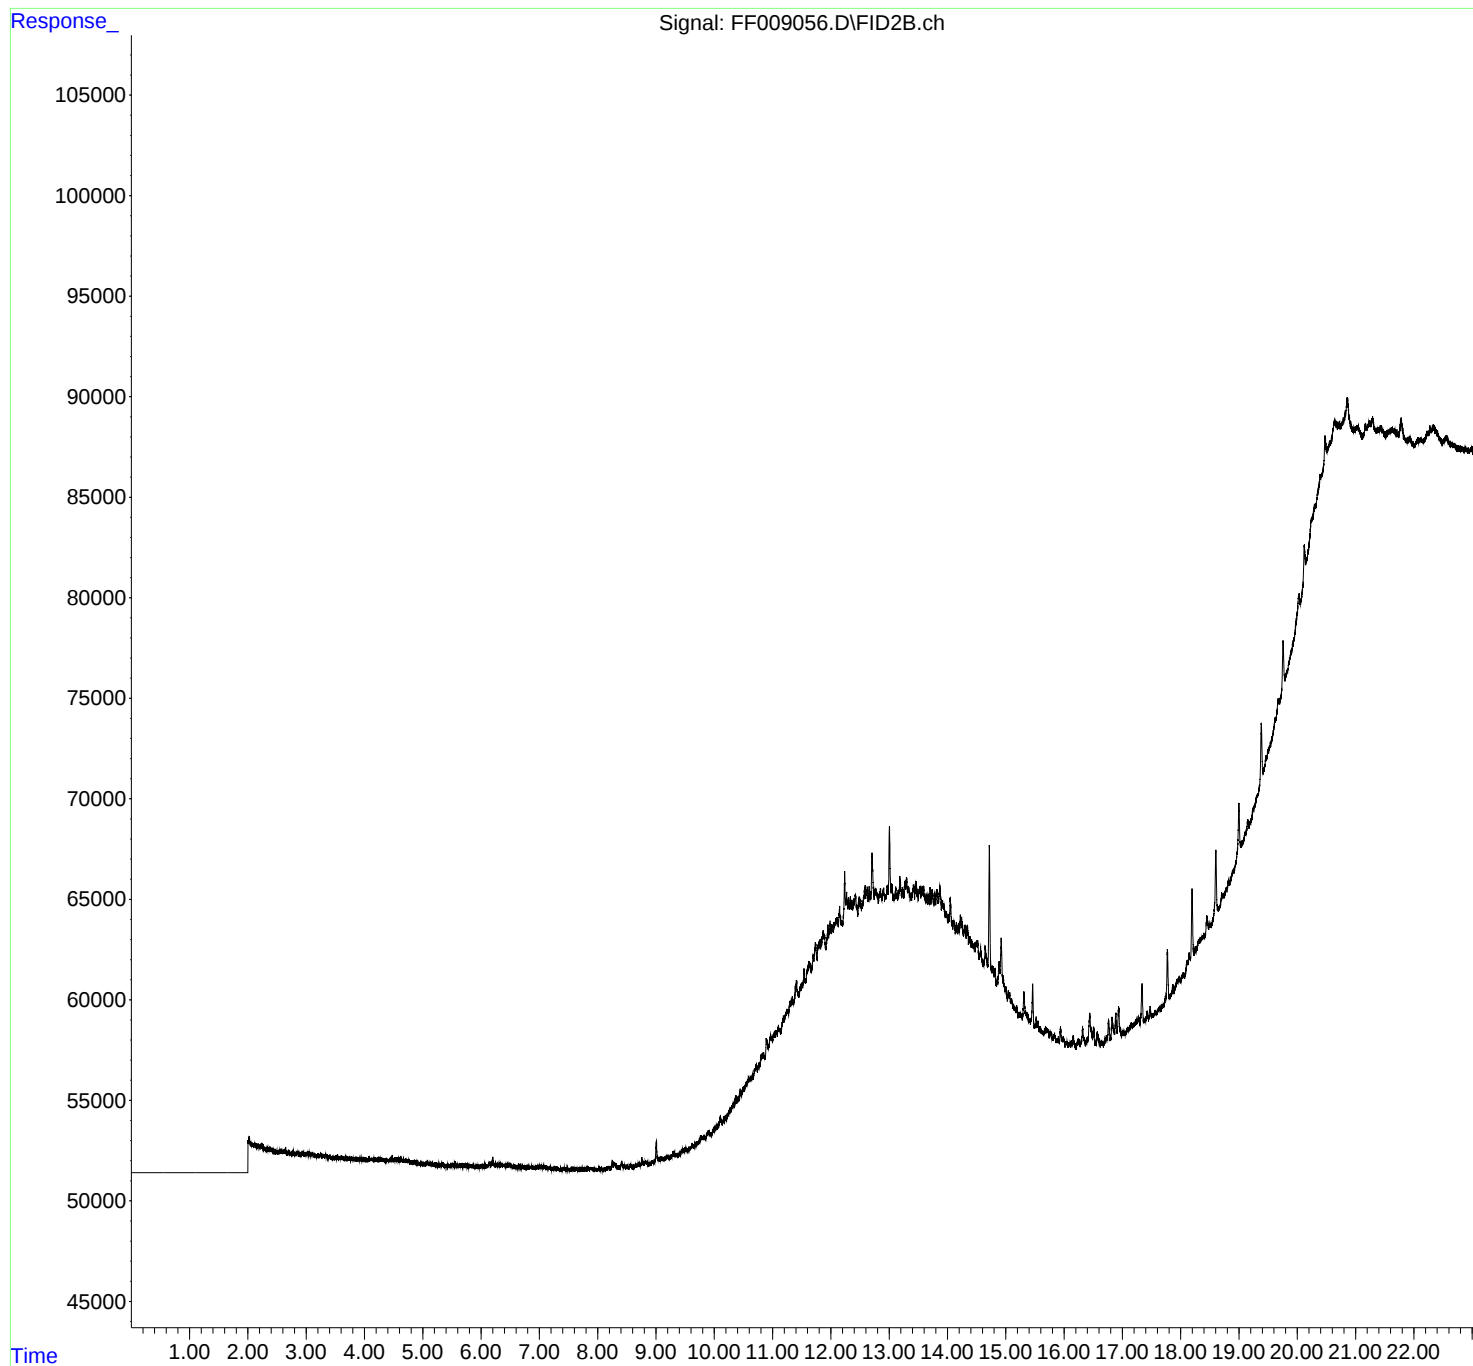

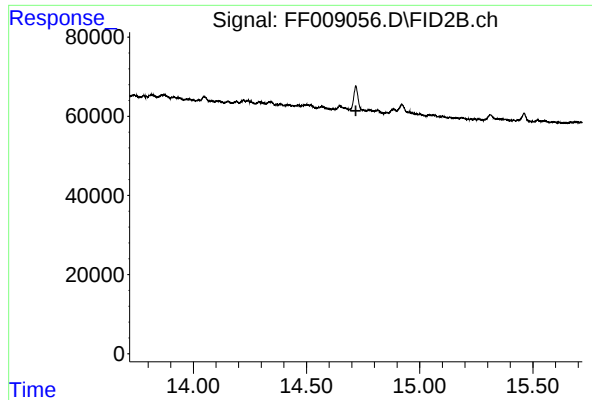

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.718 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_F  
ClientSampleId :