

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100121\
Data File : FF009054.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2021 11:21
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 01 22:29:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.492	4636426	32.834 ug/ml
12) N-OCTACOSANE	16.890	3952026	32.302 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF100121\
Data File : FF009054.D
Signal(s) : FID2B.ch
Acq On : 01 Oct 2021 11:21
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 01 22:29:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090721.M
Quant Title :
QLast Update : Wed Sep 08 10:20:54 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

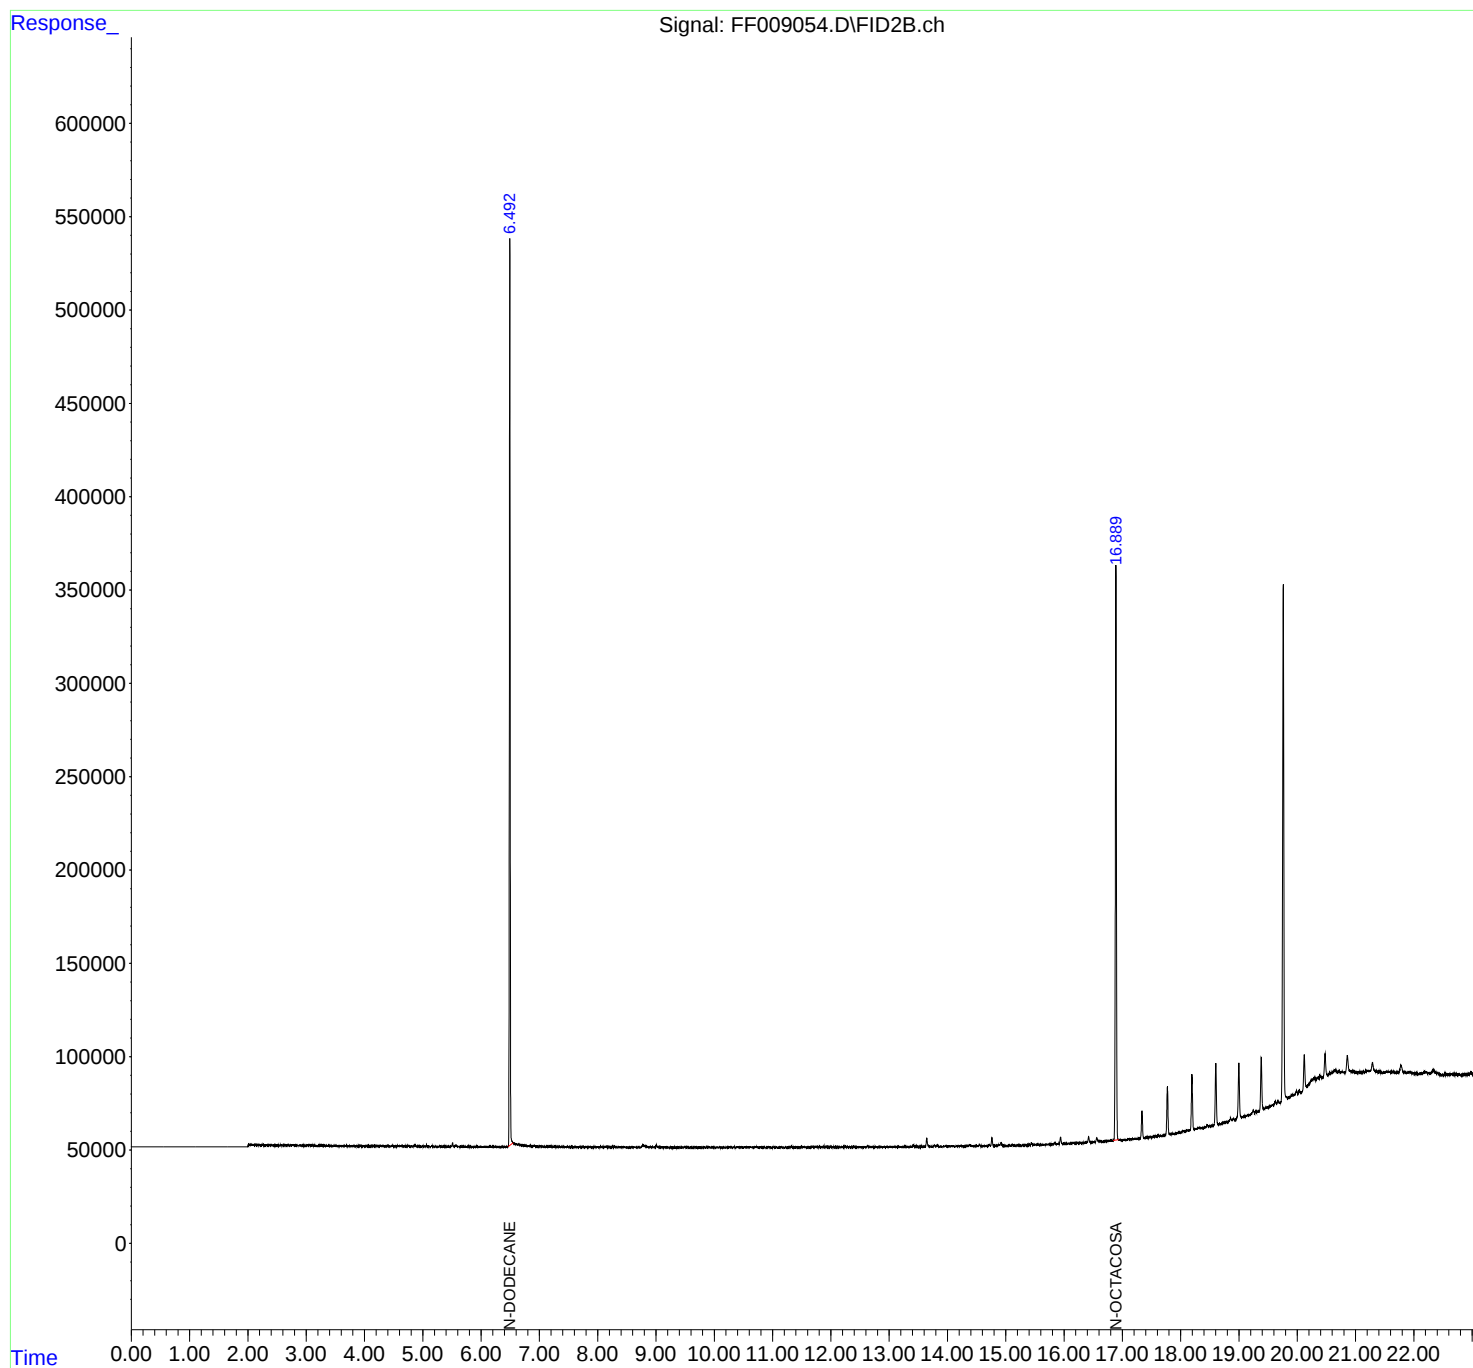


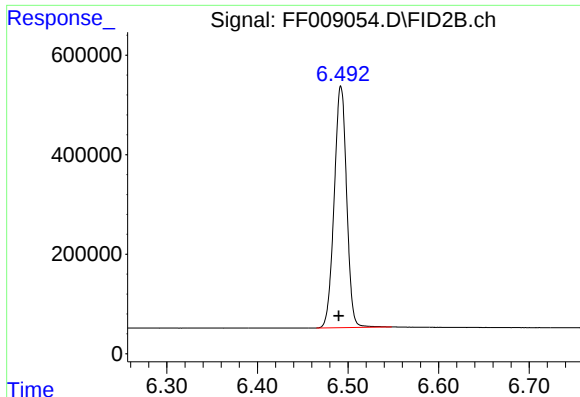

#3 N-DODECANE


R.T.: 6.492 min
Delta R.T.: 0.002 min
Response: 4636426
Conc: 32.83 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

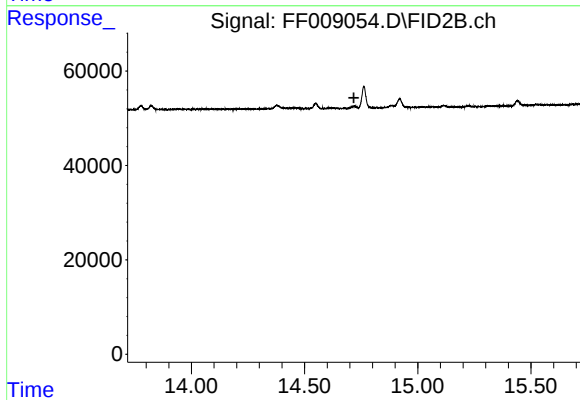

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.718 min
Response: 0
Conc: N.D.

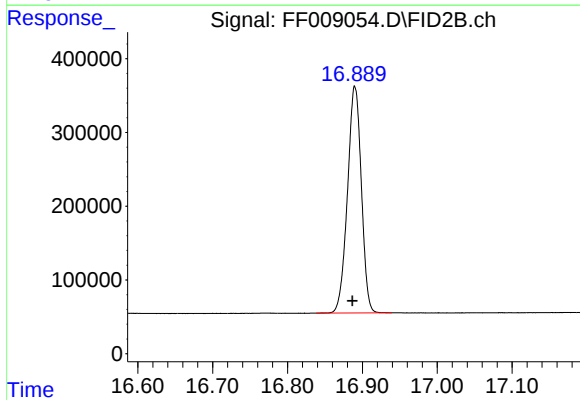

#12 N-OCTACOSANE

R.T.: 16.890 min
Delta R.T.: 0.003 min
Response: 3952026
Conc: 32.30 ug/ml